

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0085034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 4:45
 Operator : YP\AJ
 Sample : N1715-28 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-81A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2022
 Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 06:51:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.594	389780	76239	1.394	1.695
2) SA Decachlor...	10.434	8.622	329781	68846	1.881m	1.874
Target Compounds						
26) L6 AR-1254-1	6.566	5.490	51794	9971	5.281	3.727 #
27) L6 AR-1254-2	6.789	5.639	76446	11534	5.151	4.890
28) L6 AR-1254-3	7.161	6.042	67002	13116	4.425m	3.489m
29) L6 AR-1254-4	7.451	6.273	48159	12003	4.490m	5.121
30) L6 AR-1254-5	7.876	6.693	80357	18906	6.824m	5.588

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO085034.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 4:45
Operator : YP\AJ
Sample : N1715-28 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 06:51:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

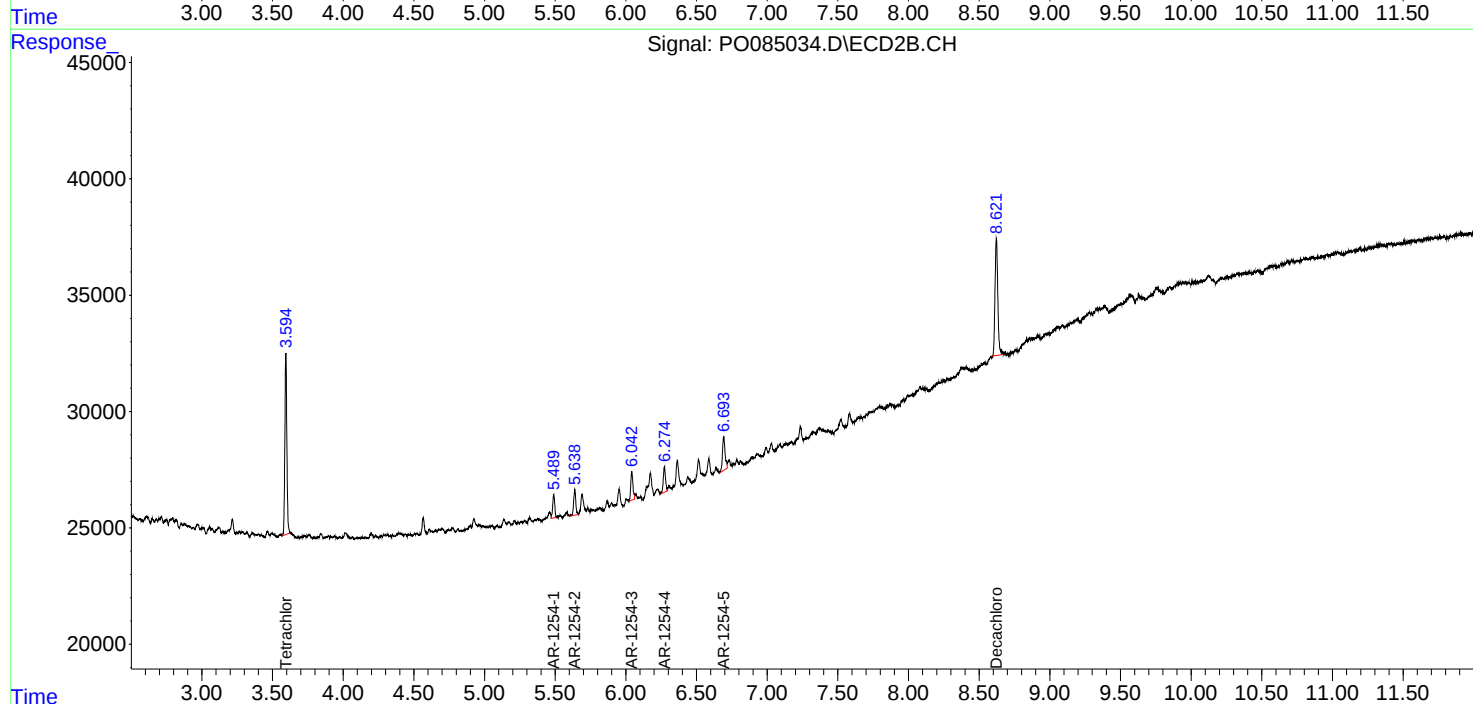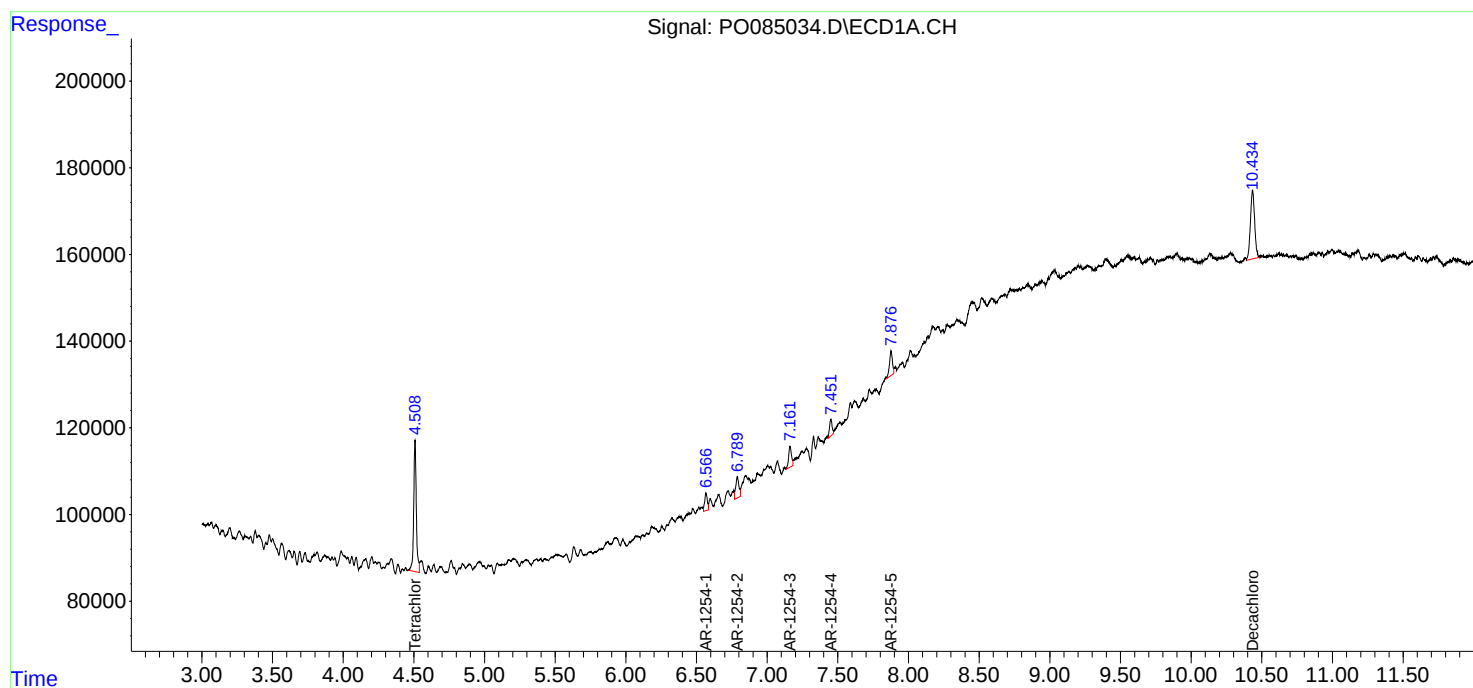

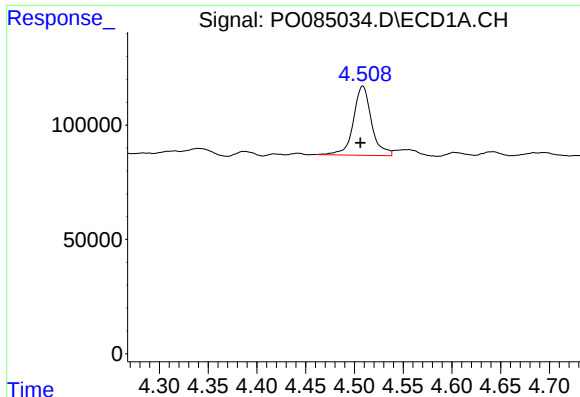


#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 389780
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

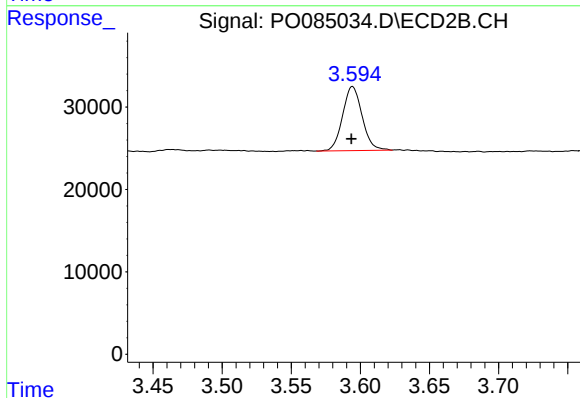


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 76239
Conc: 1.70 ng/ml

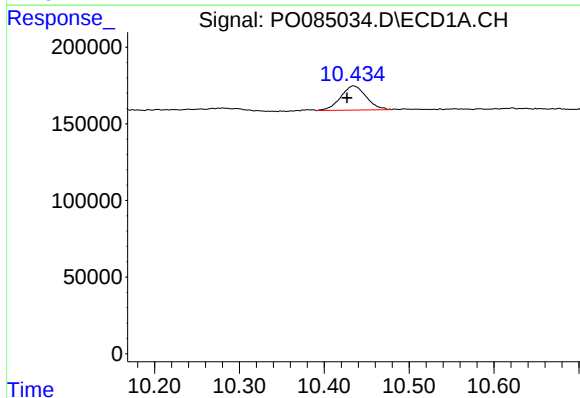


#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.007 min
Response: 329781
Conc: 1.88 ng/ml m

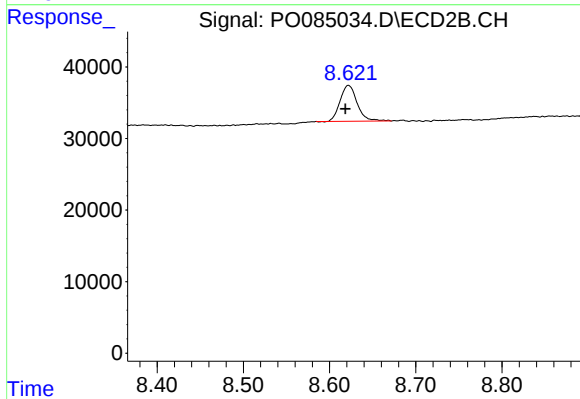

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: 0.004 min
Response: 68846
Conc: 1.87 ng/ml

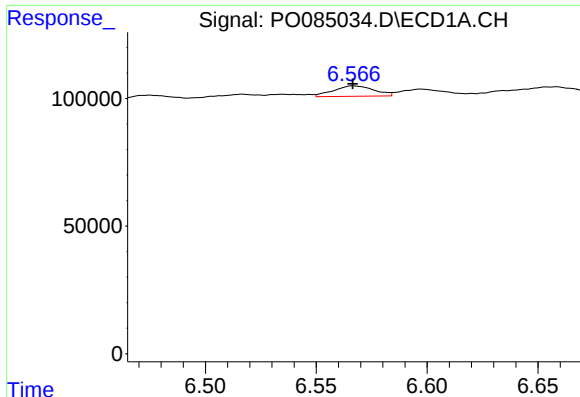


#26 AR-1254-1

R.T.: 6.566 min
Delta R.T.: 0.000 min
Response: 51794
Conc: 5.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

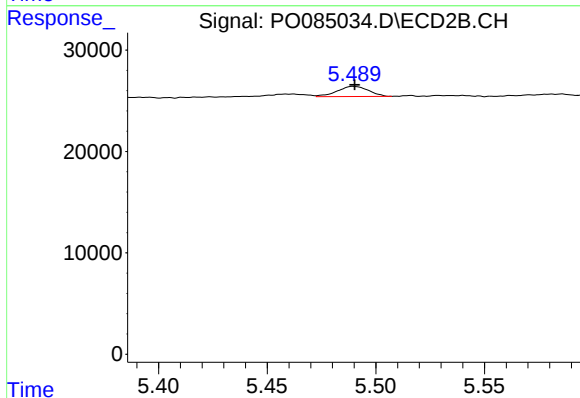


#26 AR-1254-1

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 9971
Conc: 3.73 ng/ml

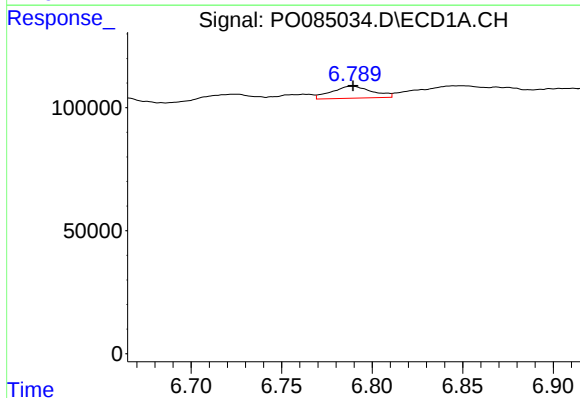


#27 AR-1254-2

R.T.: 6.789 min
Delta R.T.: 0.000 min
Response: 76446
Conc: 5.15 ng/ml

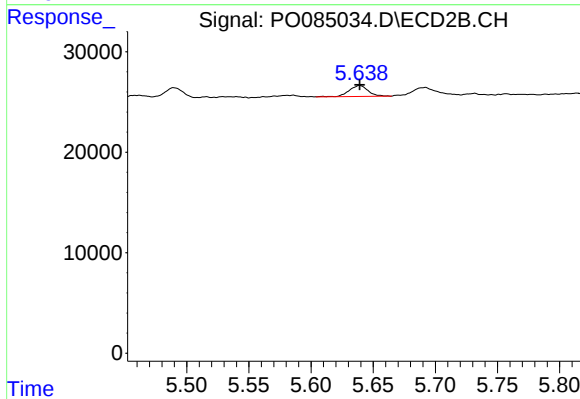

#27 AR-1254-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 11534
Conc: 4.89 ng/ml

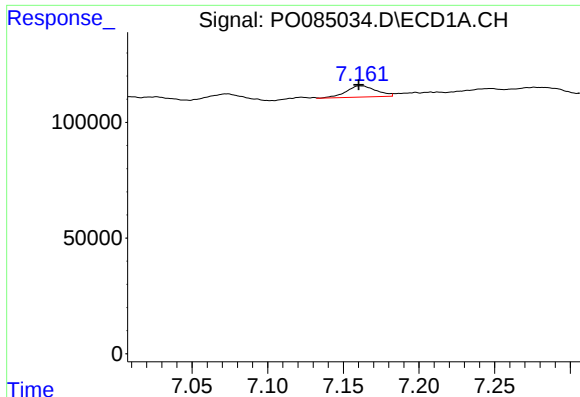


#28 AR-1254-3

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 67002
Conc: 4.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

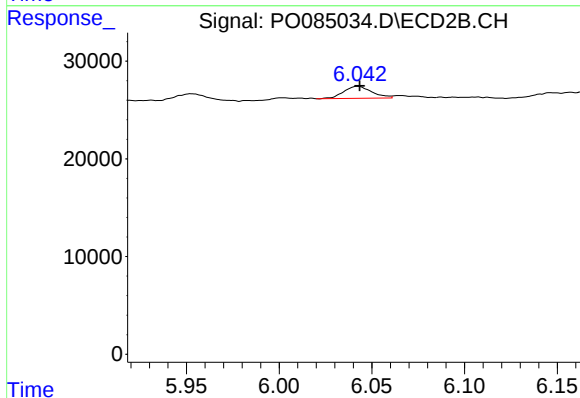


#28 AR-1254-3

R.T.: 6.042 min
Delta R.T.: -0.001 min
Response: 13116
Conc: 3.49 ng/ml m

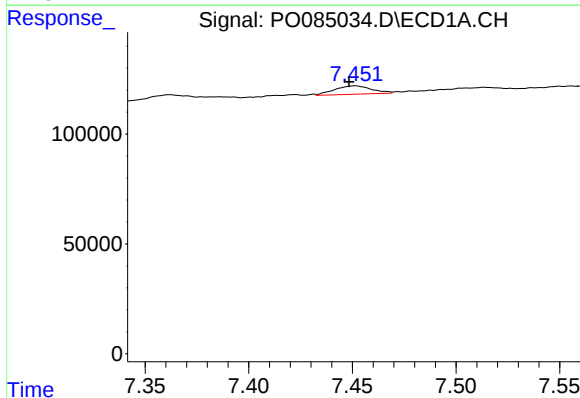


#29 AR-1254-4

R.T.: 7.451 min
Delta R.T.: 0.002 min
Response: 48159
Conc: 4.49 ng/ml m

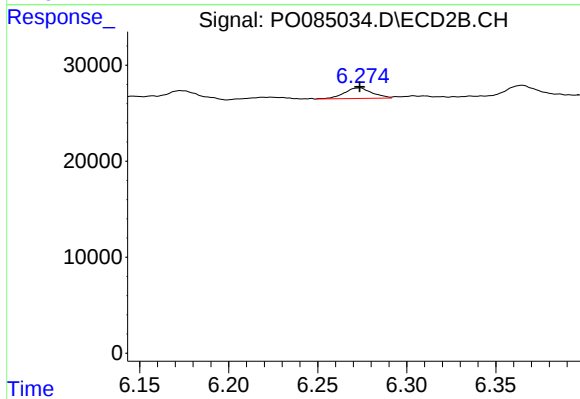

#29 AR-1254-4

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 12003
Conc: 5.12 ng/ml

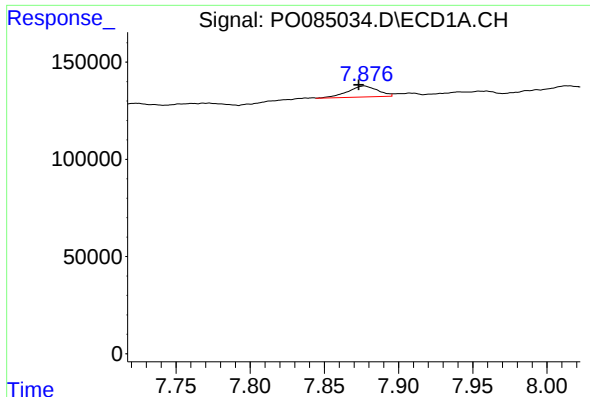


#30 AR-1254-5

R.T.: 7.876 min
Delta R.T.: 0.003 min
Response: 80357
Conc: 6.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

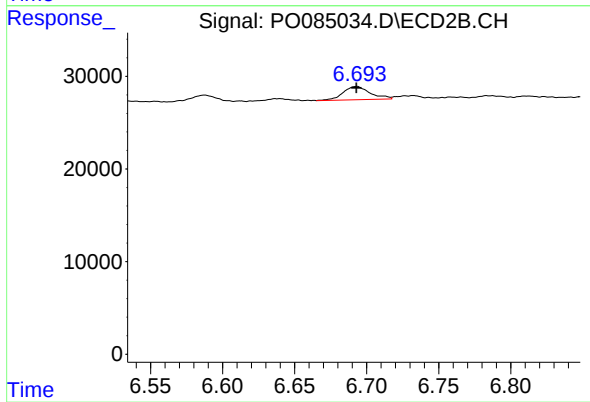

#30 AR-1254-5

R.T.: 6.693 min
Delta R.T.: 0.000 min
Response: 18906
Conc: 5.59 ng/ml