

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0085039.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 6:05
 Operator : YP\AJ
 Sample : N1716-07 10X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEE379T-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/03/2022
 Supervised By :Ankita Jodhani 03/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 06:53:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.595	283277	81454	1.013	1.811 #
2) SA Decachlor...	10.436	8.621	227334	60797	1.297	1.655m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
Data File : P0085039.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 6:05
Operator : YP\AJ
Sample : N1716-07 10X
Misc :
ALS Vial : 52 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
HEE379T-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/03/2022
Supervised By :Ankita Jodhani 03/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 06:53:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

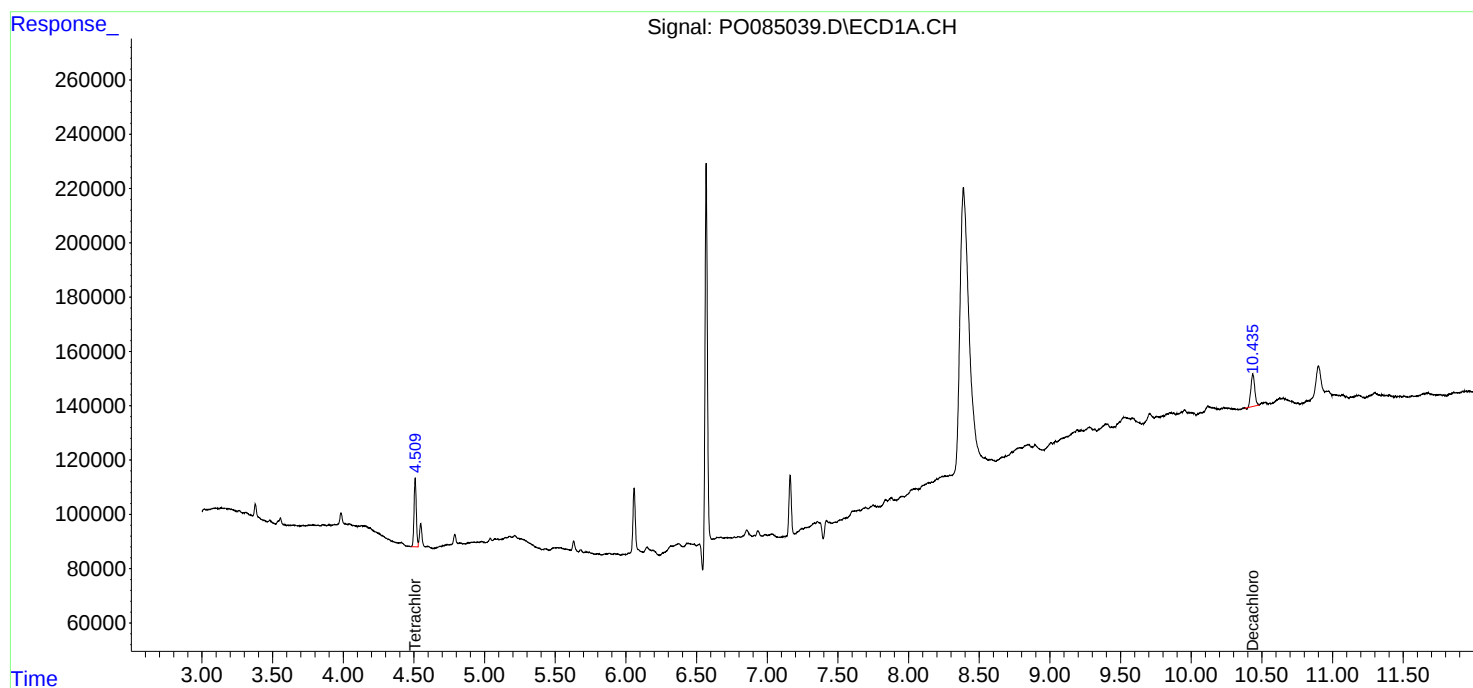

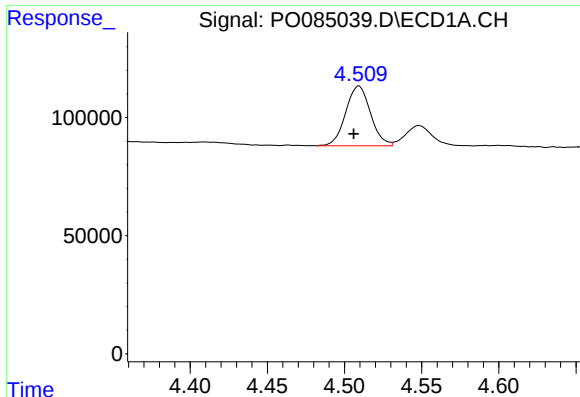


#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 283277
Conc: 1.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEE379T-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/03/2022
Supervised By :Ankita Jodhani 03/03/2022

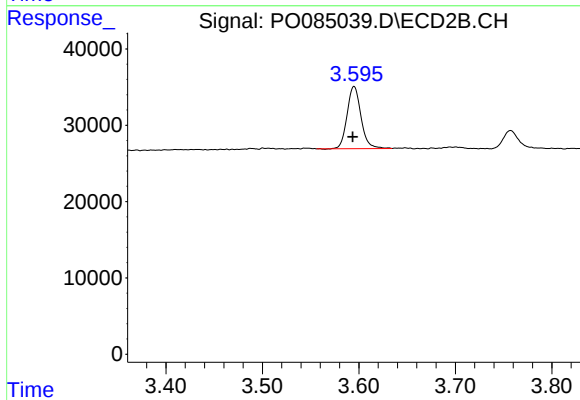


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.002 min
Response: 81454
Conc: 1.81 ng/ml

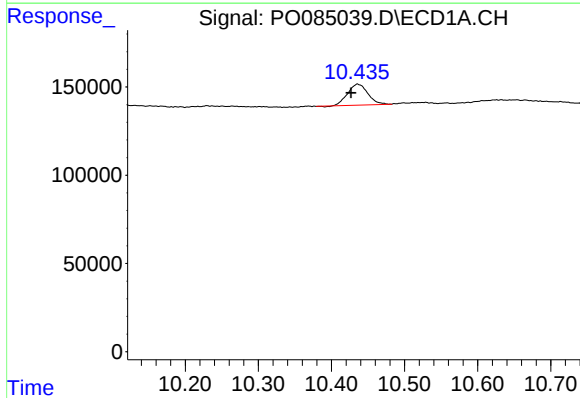

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.009 min
Response: 227334
Conc: 1.30 ng/ml

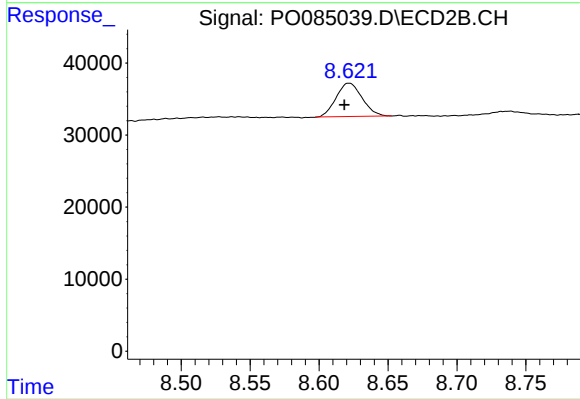

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: 0.003 min
Response: 60797
Conc: 1.65 ng/ml m