

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030323\
 Data File : PD074107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 10:16
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 21:28:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
6) B	beta-BHC	4.556f	0.000	187938	0	0.125	N.D. #
7) B	delta-BHC	4.779	0.000	2199462	0	0.785	N.D. #
8) B	Heptachlo...	5.698	0.000	5441608	0	1.911	N.D. #
13) MA	Dieldrin	0.000	5.356	0	115191	N.D.	0.078 #
14) MA	Endrin	0.000	5.663f	0	410310	N.D.	0.314 #
15) B	Endosulfa...	6.846f	0.000	128206	0	0.044	N.D. #
19) B	Endosulfa...	0.000	6.352	0	197472	N.D.	0.163 #
21) B	Endrin ke...	7.695f	0.000	787999	0	0.269	N.D. #
22)	Mirex	8.161f	7.025	301748	64421	0.134	0.056 #
24)	Chlordane-2	0.000	4.362	0	1879111	N.D.	31.394 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030323\
Data File : PD074107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 10:16
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 21:28:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

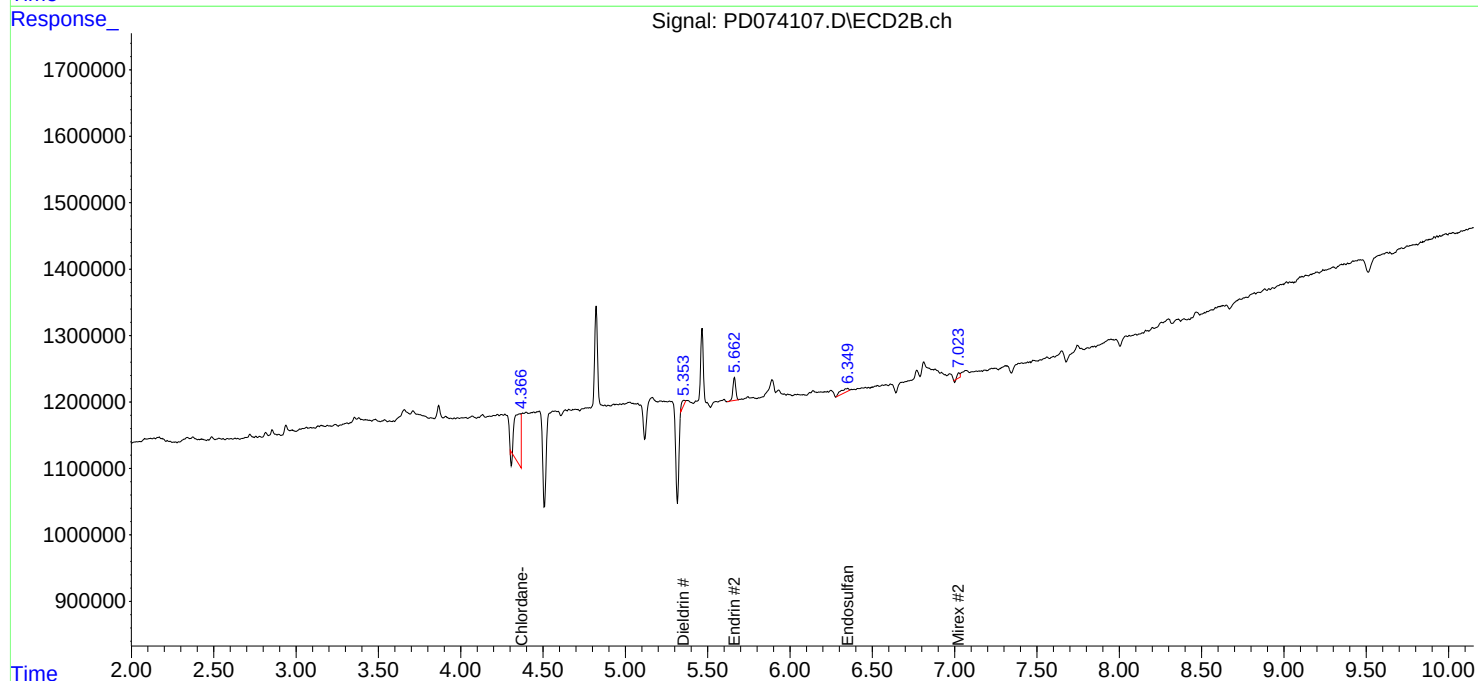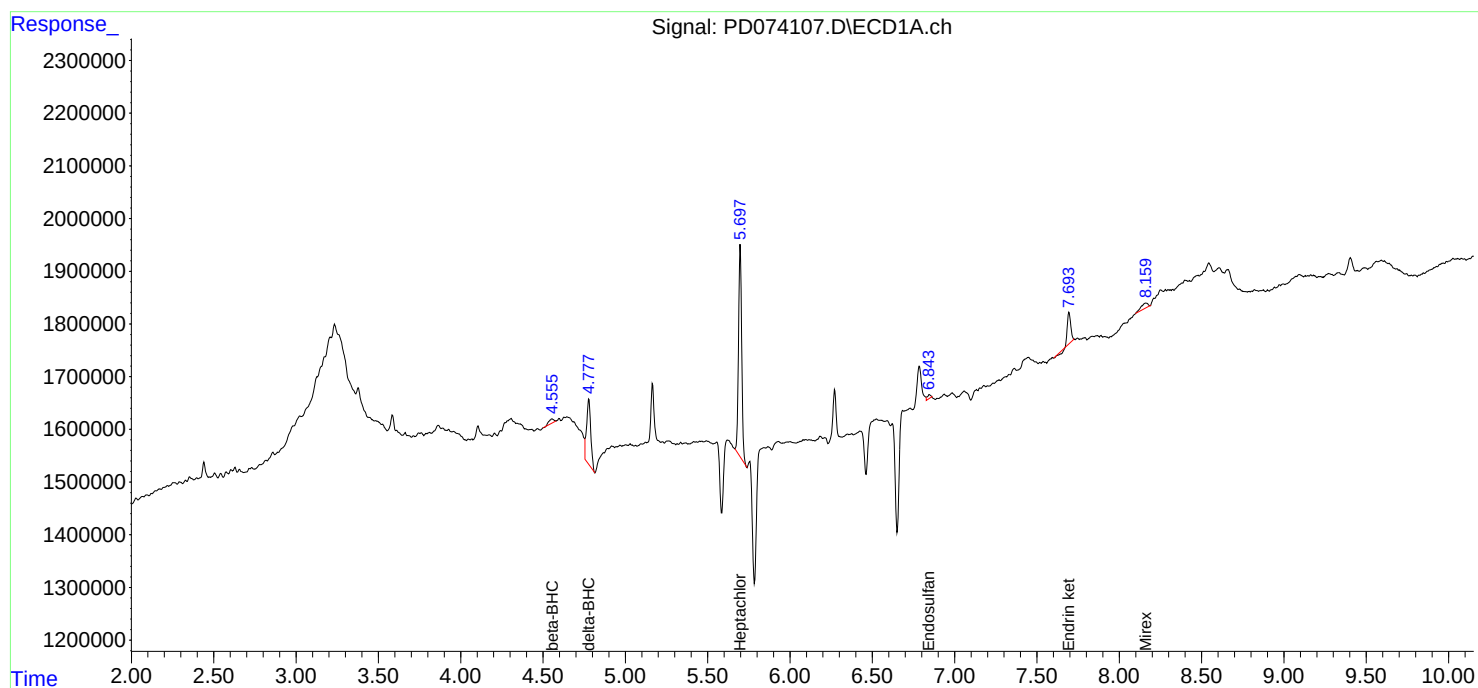


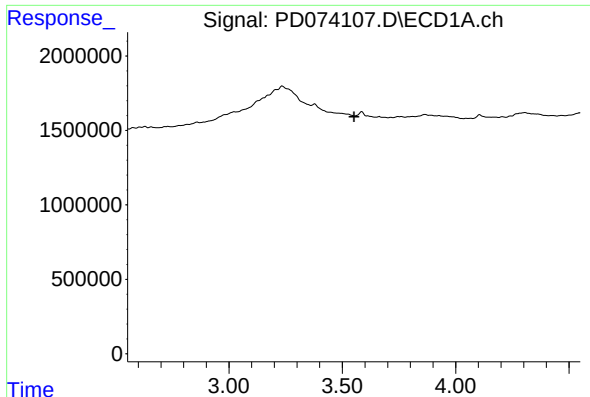

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

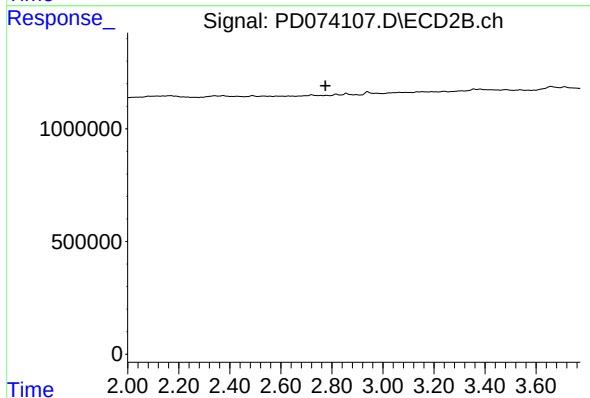


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.774 min
Response: 0
Conc: N.D.

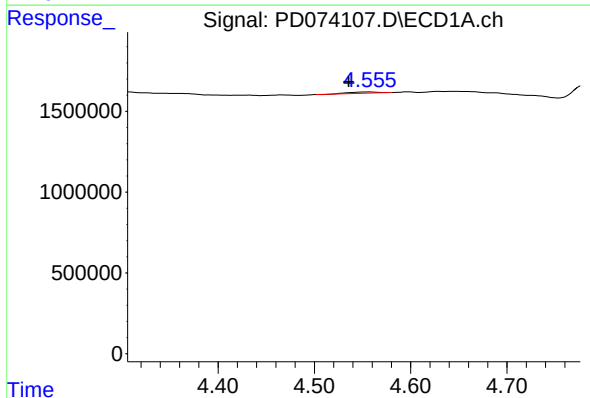


#6 beta-BHC

R.T.: 4.556 min
Delta R.T.: 0.020 min
Response: 187938
Conc: 0.13 ng/ml

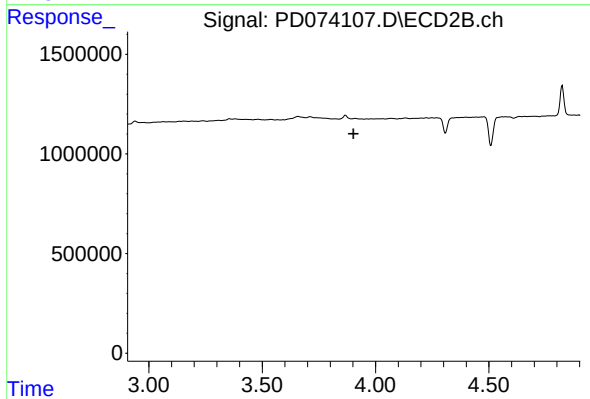

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.903 min
Response: 0
Conc: N.D.

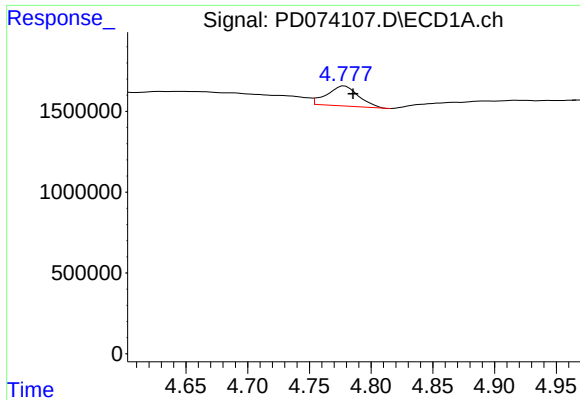

#7 delta-BHC


R.T.: 4.779 min
Delta R.T.: -0.007 min
Response: 2199462
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :

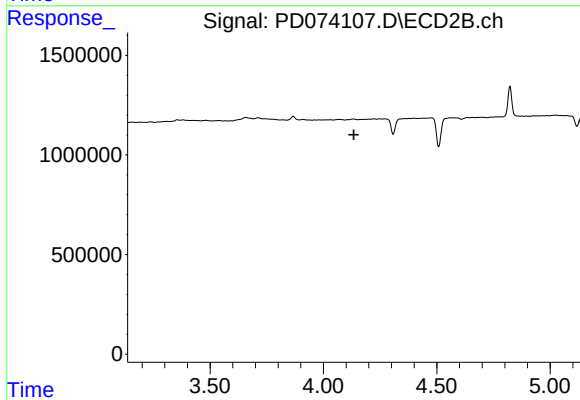


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.135 min
Response: 0
Conc: N.D.

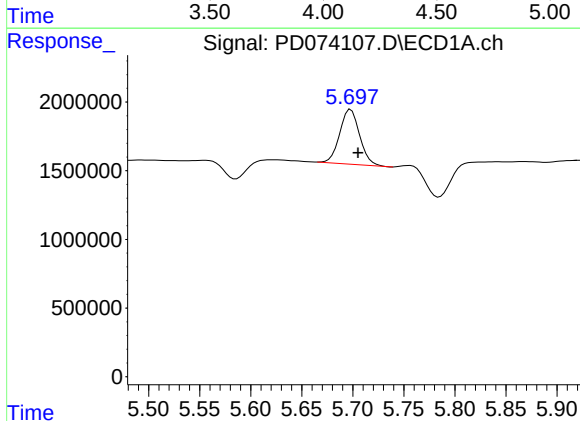


#8 Heptachlor epoxide

R.T.: 5.698 min
Delta R.T.: -0.007 min
Response: 5441608
Conc: 1.91 ng/ml

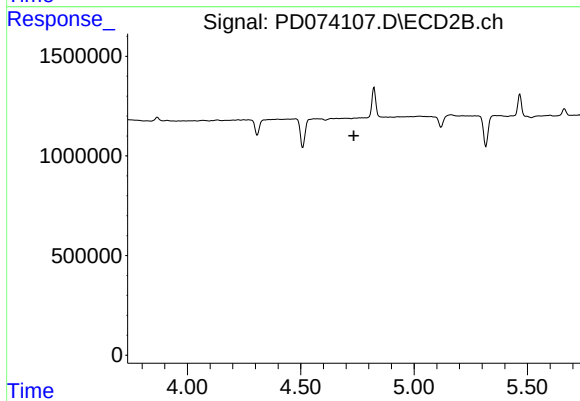

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

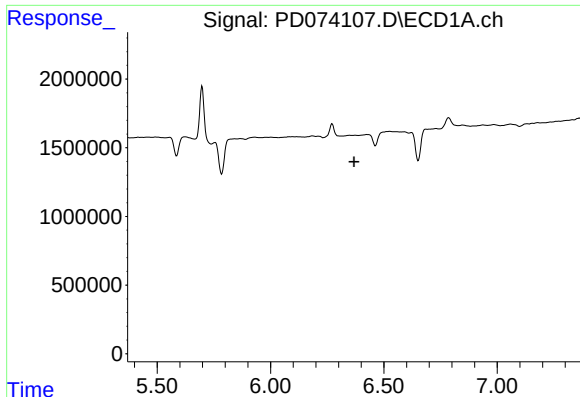

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

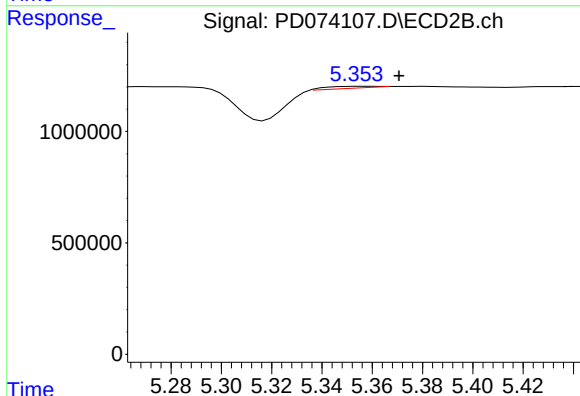


#13 Dieldrin

R.T.: 5.356 min
Delta R.T.: -0.014 min
Response: 115191
Conc: 0.08 ng/ml

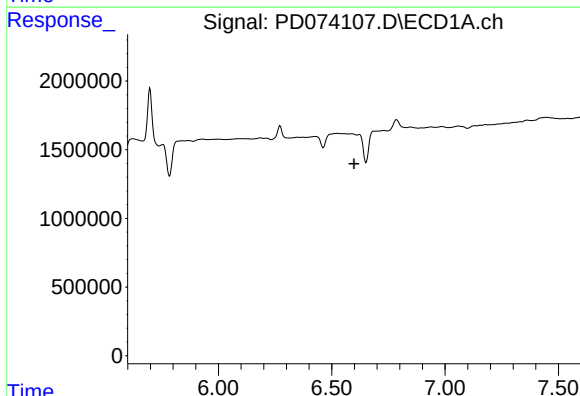


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.599 min
Response: 0
Conc: N.D.

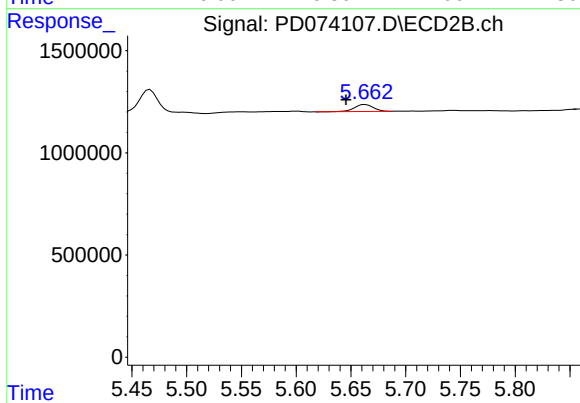

#14 Endrin


R.T.: 5.663 min
Delta R.T.: 0.017 min
Response: 410310
Conc: 0.31 ng/ml

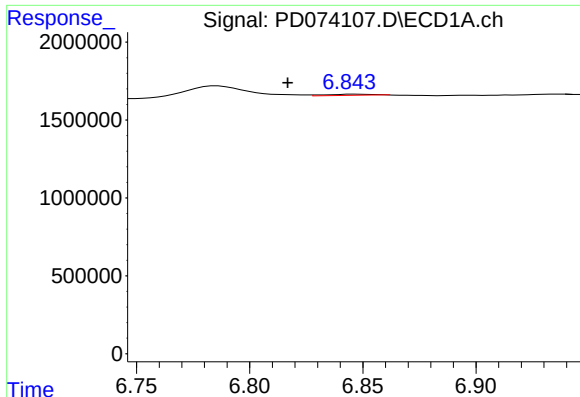

#15 Endosulfan II


R.T.: 6.846 min
Delta R.T.: 0.029 min
Response: 128206
Conc: 0.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

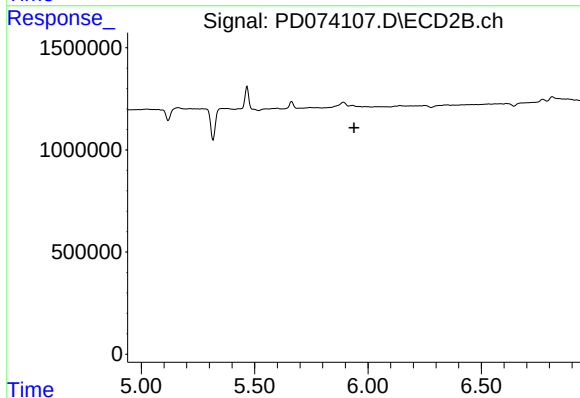


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

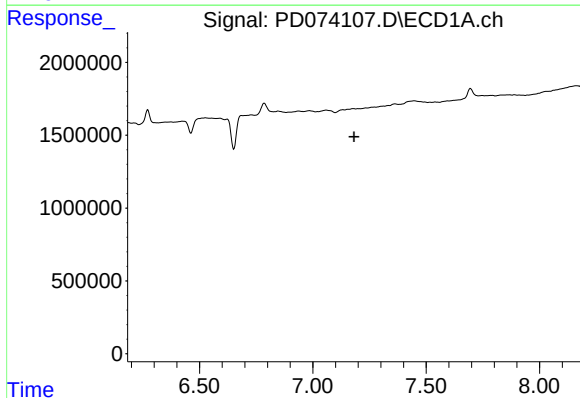


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

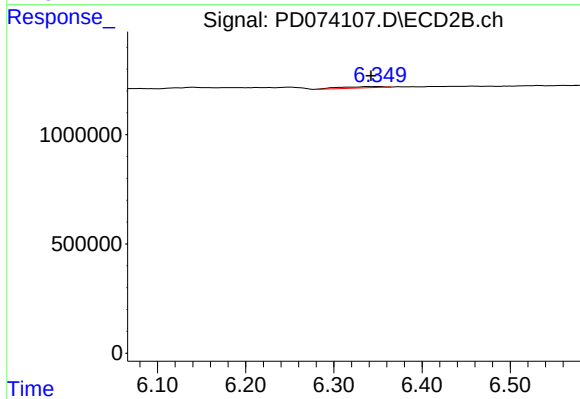

#19 Endosulfan Sulfate


R.T.: 6.352 min
Delta R.T.: 0.009 min
Response: 197472
Conc: 0.16 ng/ml

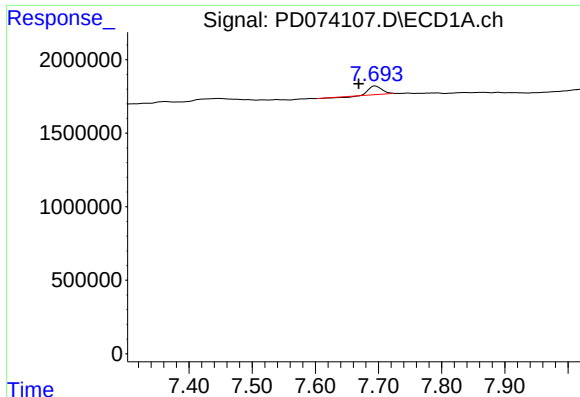

#21 Endrin ketone


R.T.: 7.695 min
Delta R.T.: 0.026 min
Response: 787999
Conc: 0.27 ng/ml

Instrument :
ECD_O
ClientSampleId :

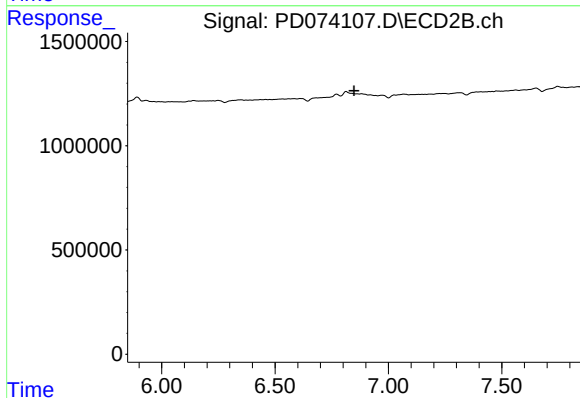


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

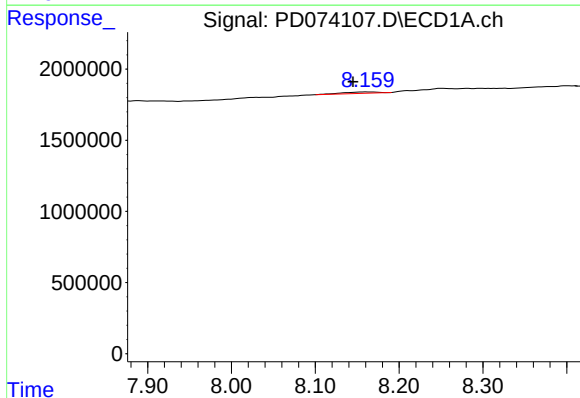


#22 Mirex

R.T.: 8.161 min
Delta R.T.: 0.016 min
Response: 301748
Conc: 0.13 ng/ml

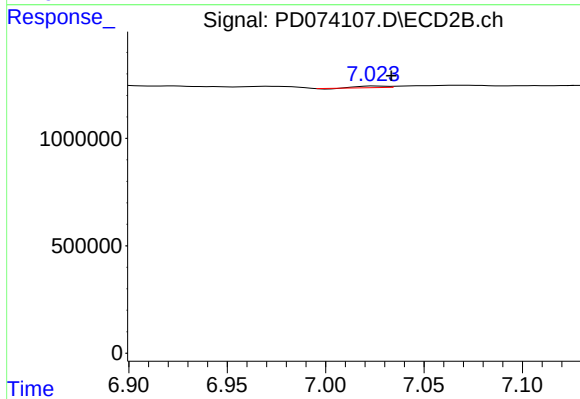

#22 Mirex


R.T.: 7.025 min
Delta R.T.: -0.008 min
Response: 64421
Conc: 0.06 ng/ml

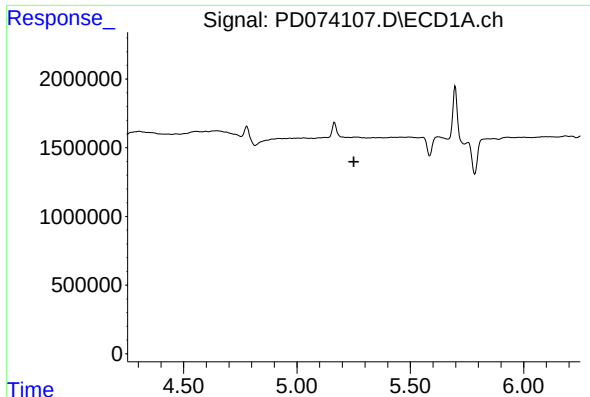

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

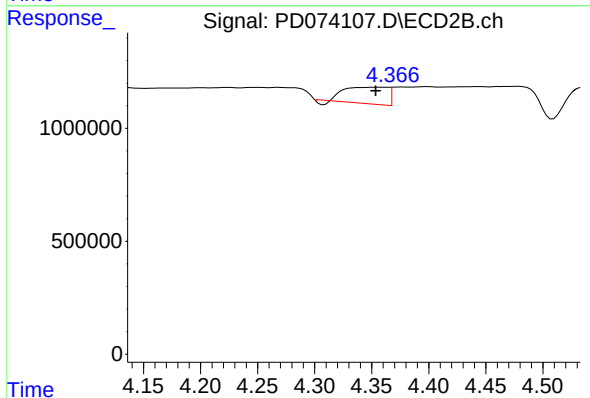


#24 Chlordane-2

R.T.: 4.362 min
Delta R.T.: 0.009 min
Response: 1879111
Conc: 31.39 ng/ml

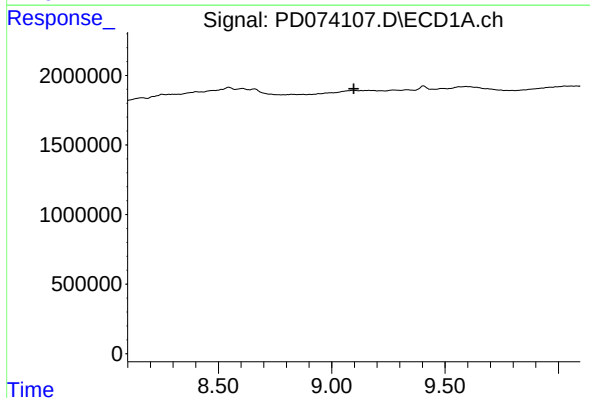

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.098 min
Response: 0
Conc: N.D.

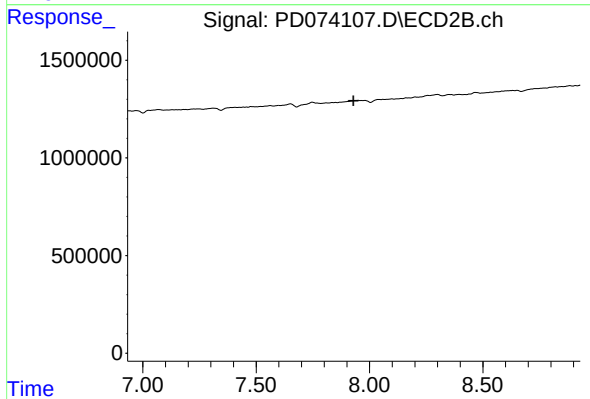

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.929 min
Response: 0
Conc: N.D.