

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030323\
 Data File : PD074108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 10:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 21:28:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.775	45354683	22985504	19.796	19.407
28)	SA Decachlor...	9.100	7.930	57912709	25179086	21.727	20.565
Target Compounds							
4)	MA Heptachlor	4.922	0.000	422382	0	0.123	N.D. #
6)	B beta-BHC	0.000	3.914	0	260812	N.D.	0.355 #
7)	B delta-BHC	4.779	0.000	5219768	0	1.862	N.D. #
8)	B Heptachlo...	5.701	0.000	977264	0	0.343	N.D. #
14)	MA Endrin	0.000	5.662f	0	167985	N.D.	0.129 #
15)	B Endosulfa...	6.791f	0.000	1739829	0	0.598	N.D. #
21)	B Endrin ke...	7.698f	0.000	1437515	0	0.490	N.D. #
22)	Mirex	8.171f	0.000	156445	0	0.069	N.D. #
27)	Chlordane-5	0.000	5.972f	0	238888	N.D.	3.715 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030323\
Data File : PD074108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 10:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 21:28:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

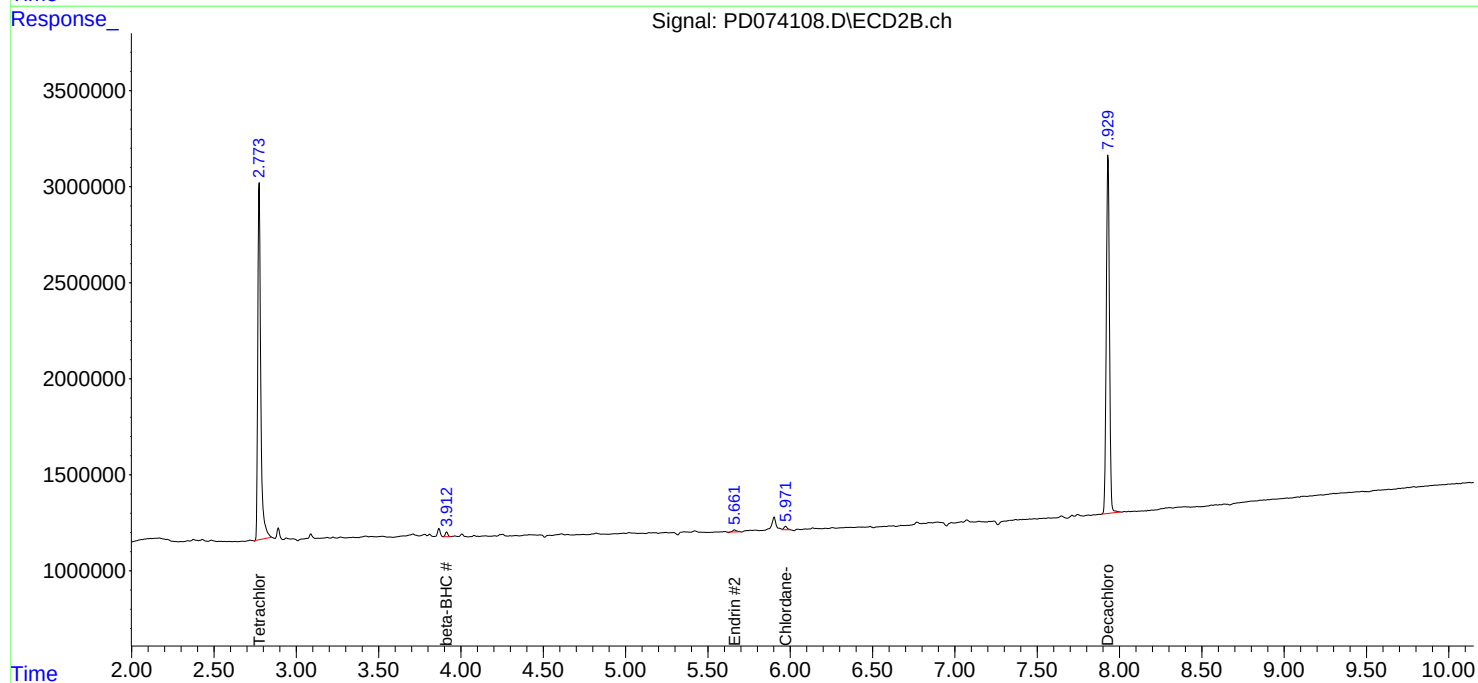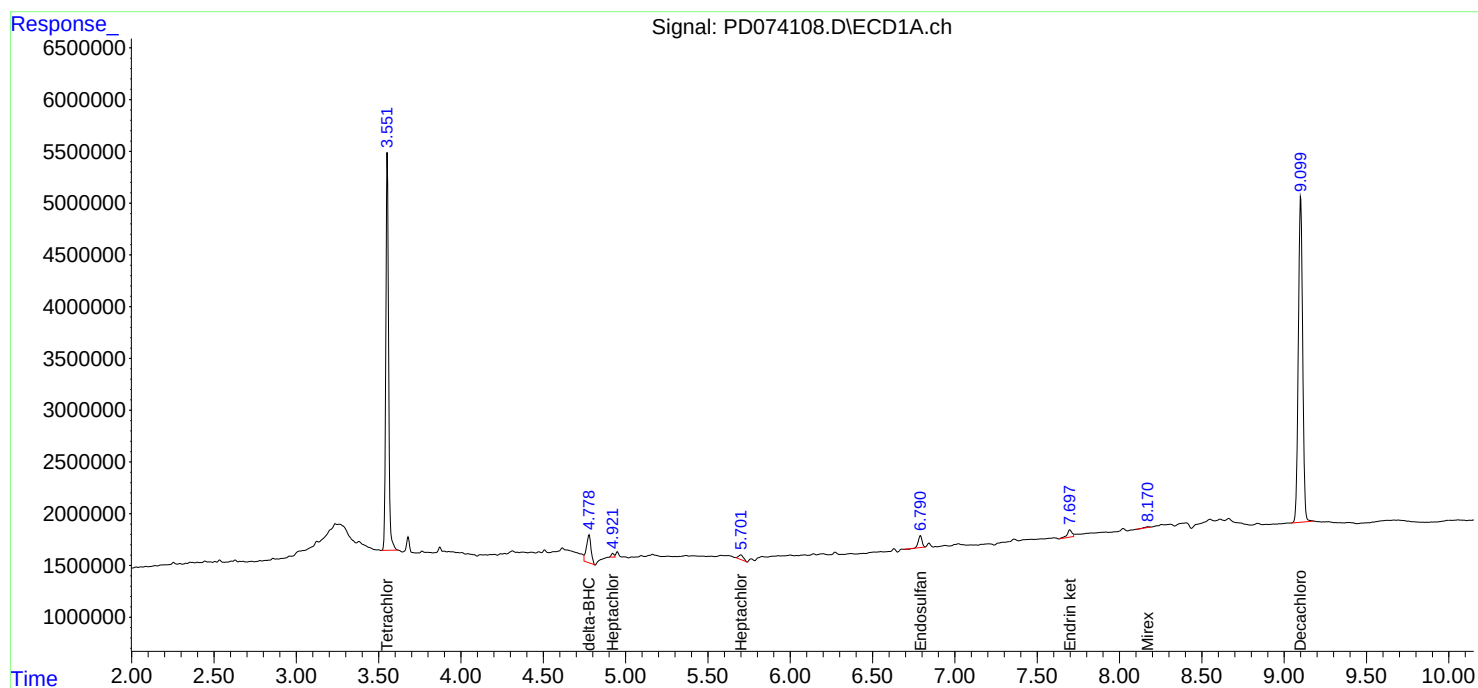


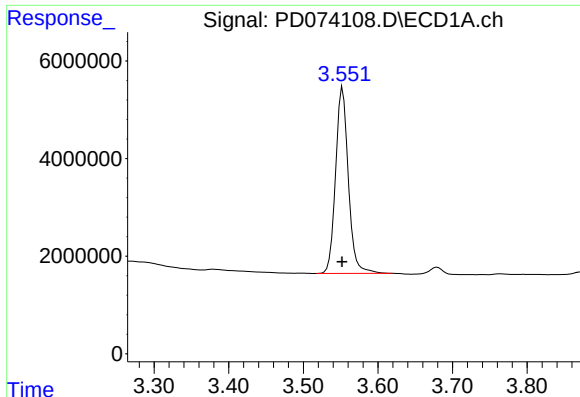

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 45354683
Conc: 19.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

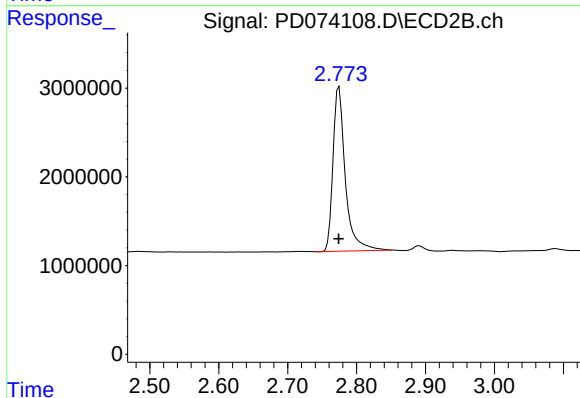


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 22985504
Conc: 19.41 ng/ml

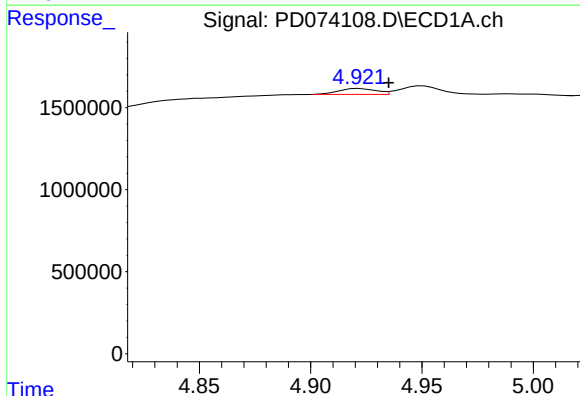


#4 Heptachlor

R.T.: 4.922 min
Delta R.T.: -0.013 min
Response: 422382
Conc: 0.12 ng/ml

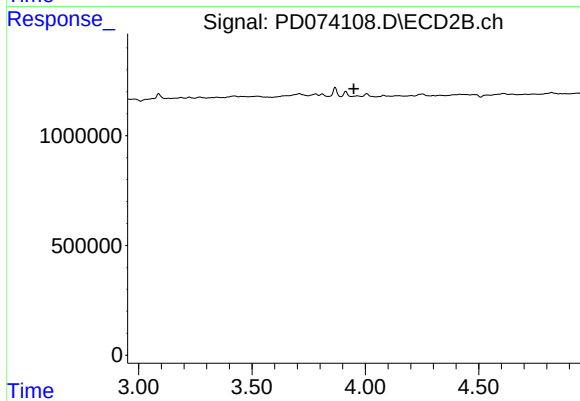

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.950 min
Response: 0
Conc: N.D.

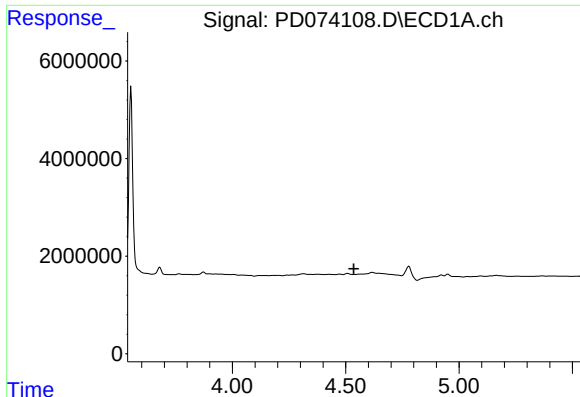

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.536 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

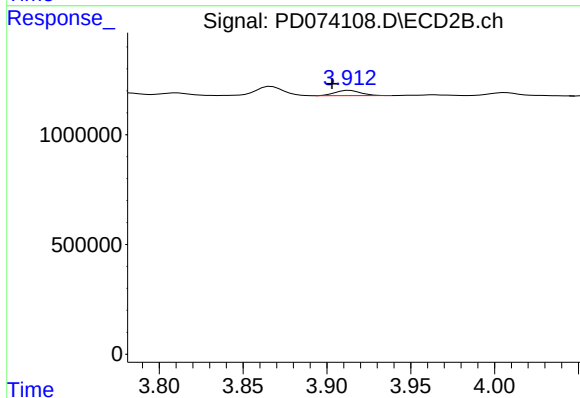


#6 beta-BHC

R.T.: 3.914 min
Delta R.T.: 0.010 min
Response: 260812
Conc: 0.35 ng/ml

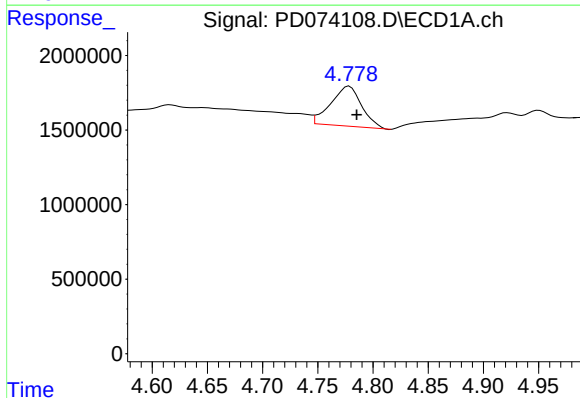


#7 delta-BHC

R.T.: 4.779 min
Delta R.T.: -0.007 min
Response: 5219768
Conc: 1.86 ng/ml

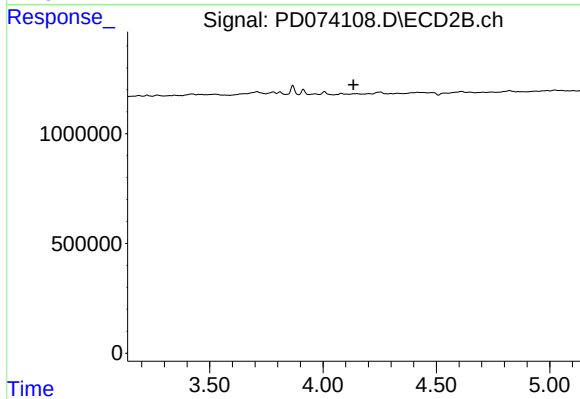

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.135 min
Response: 0
Conc: N.D.

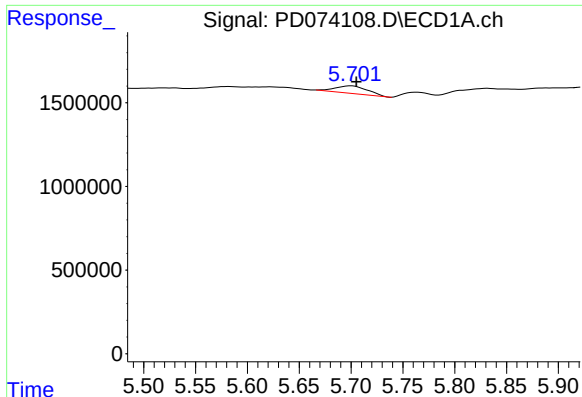

#8 Heptachlor epoxide


R.T.: 5.701 min
Delta R.T.: -0.004 min
Response: 977264
Conc: 0.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

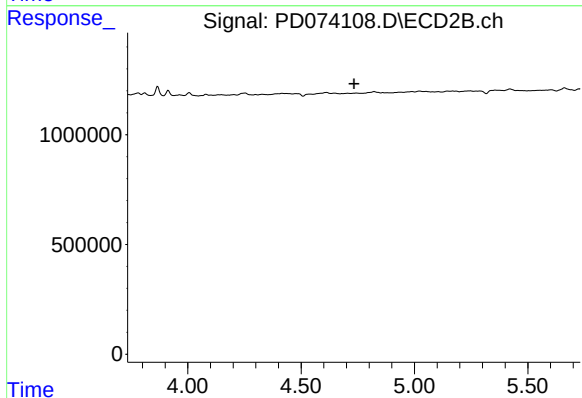


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

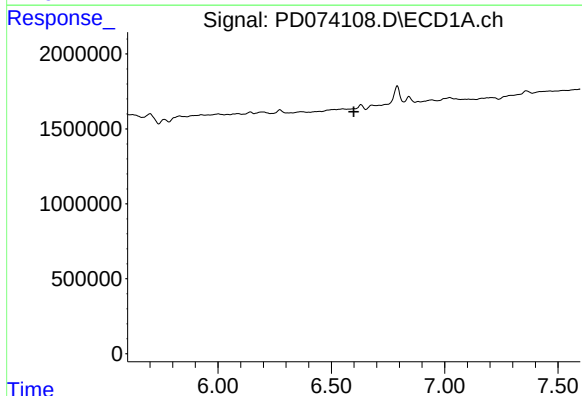


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.599 min
Response: 0
Conc: N.D.

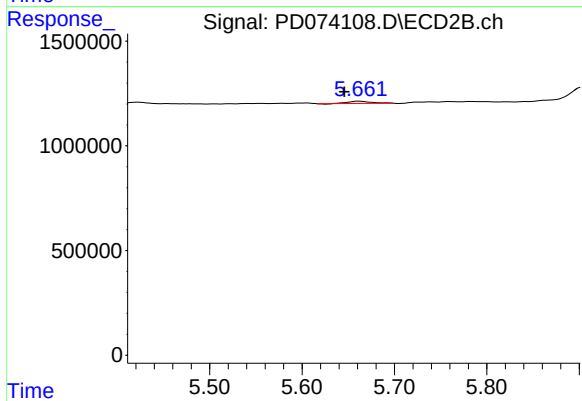

#14 Endrin


R.T.: 5.662 min
Delta R.T.: 0.016 min
Response: 167985
Conc: 0.13 ng/ml

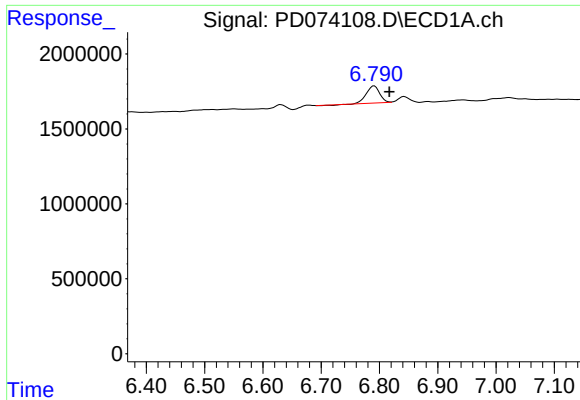

#15 Endosulfan II


R.T.: 6.791 min
Delta R.T.: -0.026 min
Response: 1739829
Conc: 0.60 ng/ml

Instrument :
ECD_O
ClientSampleId :

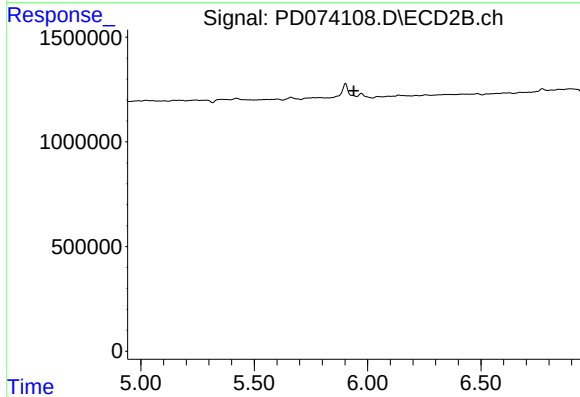


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

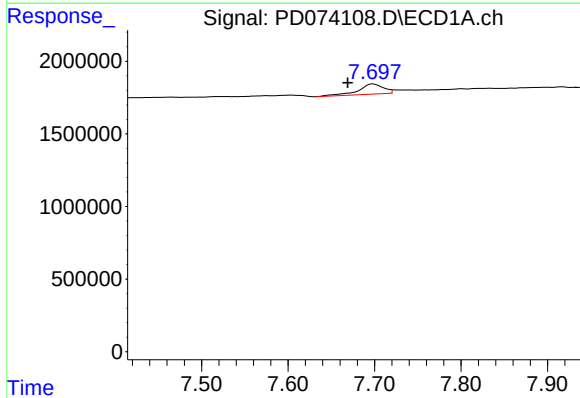


#21 Endrin ketone

R.T.: 7.698 min
Delta R.T.: 0.029 min
Response: 1437515
Conc: 0.49 ng/ml

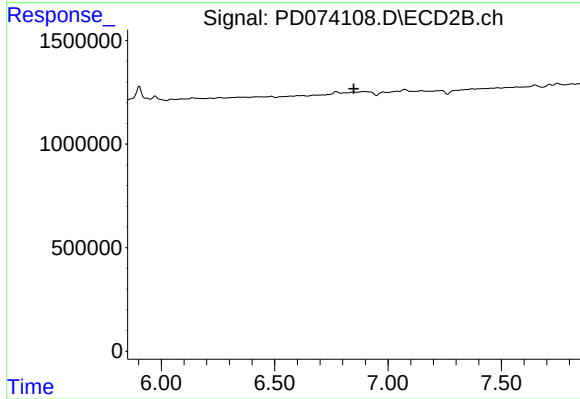

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

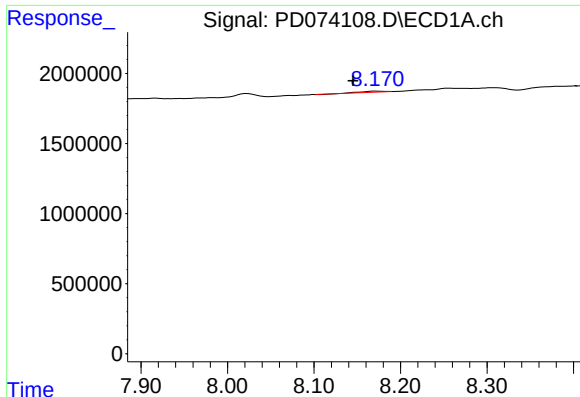

#22 Mirex


R.T.: 8.171 min
Delta R.T.: 0.026 min
Response: 156445
Conc: 0.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

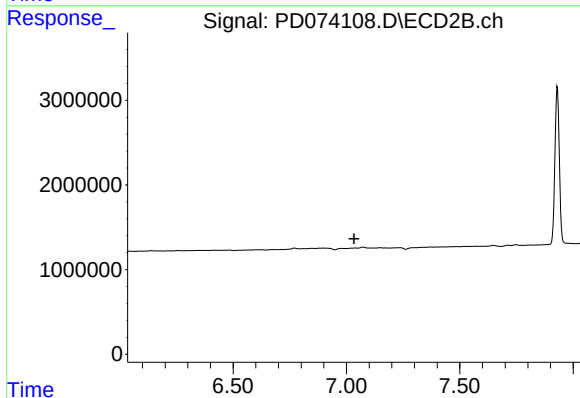


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

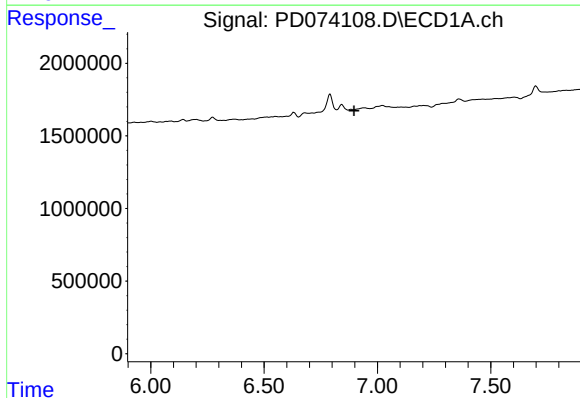


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.897 min
Response: 0
Conc: N.D.

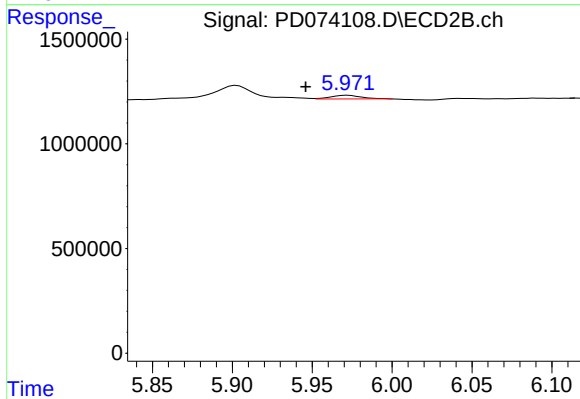

#27 Chlordane-5


R.T.: 5.972 min
Delta R.T.: 0.026 min
Response: 238888
Conc: 3.71 ng/ml

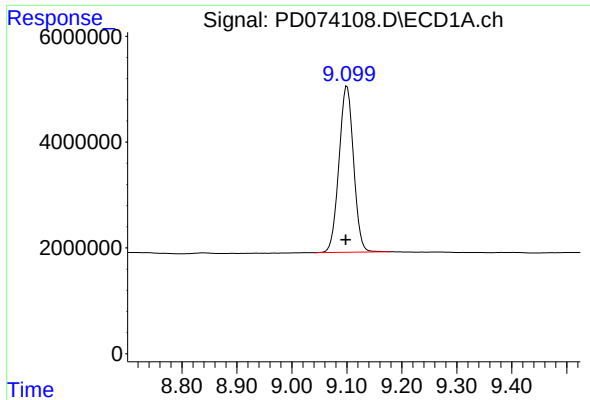

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.002 min
Response: 57912709
Conc: 21.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

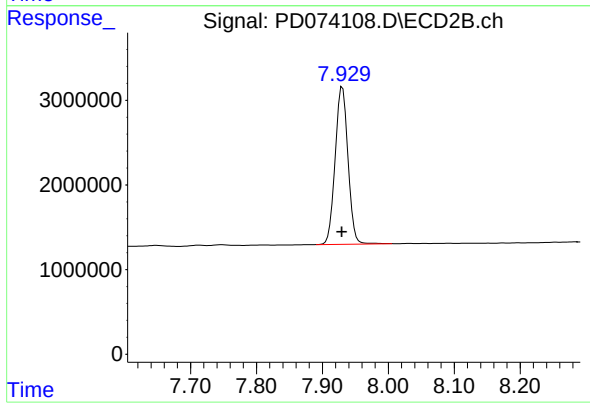

#28 Decachlorobiphenyl

R.T.: 7.930 min
Delta R.T.: 0.001 min
Response: 25179086
Conc: 20.56 ng/ml