

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030323\
 Data File : PD074123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 14:48
 Operator : AR\AJ
 Sample : PB151111TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 21:31:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	46538574	23205033	20.313	19.592
28)	SA Decachlor...	9.101	7.931	55316426	23334654	20.753	19.058
Target Compounds							
4)	MA Heptachlor	4.951f	0.000	539140	0	0.157	N.D. #
5)	MB Aldrin	5.259f	0.000	131294	0	0.039	N.D. #
6)	B beta-BHC	4.555f	0.000	32279	0	0.021	N.D. #
7)	B delta-BHC	4.780	0.000	3892882	0	1.389	N.D. #
8)	B Heptachlo...	5.688f	0.000	1566289	0	0.550	N.D. #
15)	B Endosulfa...	6.841f	0.000	368231	0	0.127	N.D. #
19)	B Endosulfa...	0.000	6.348	0	91516	N.D.	0.075 #
21)	B Endrin ke...	7.700f	0.000	993372	0	0.339	N.D. #
24)	Chlordane-2	5.259	0.000	131294	0	0.972	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030323\
Data File : PD074123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 14:48
Operator : AR\AJ
Sample : PB151111TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 21:31:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

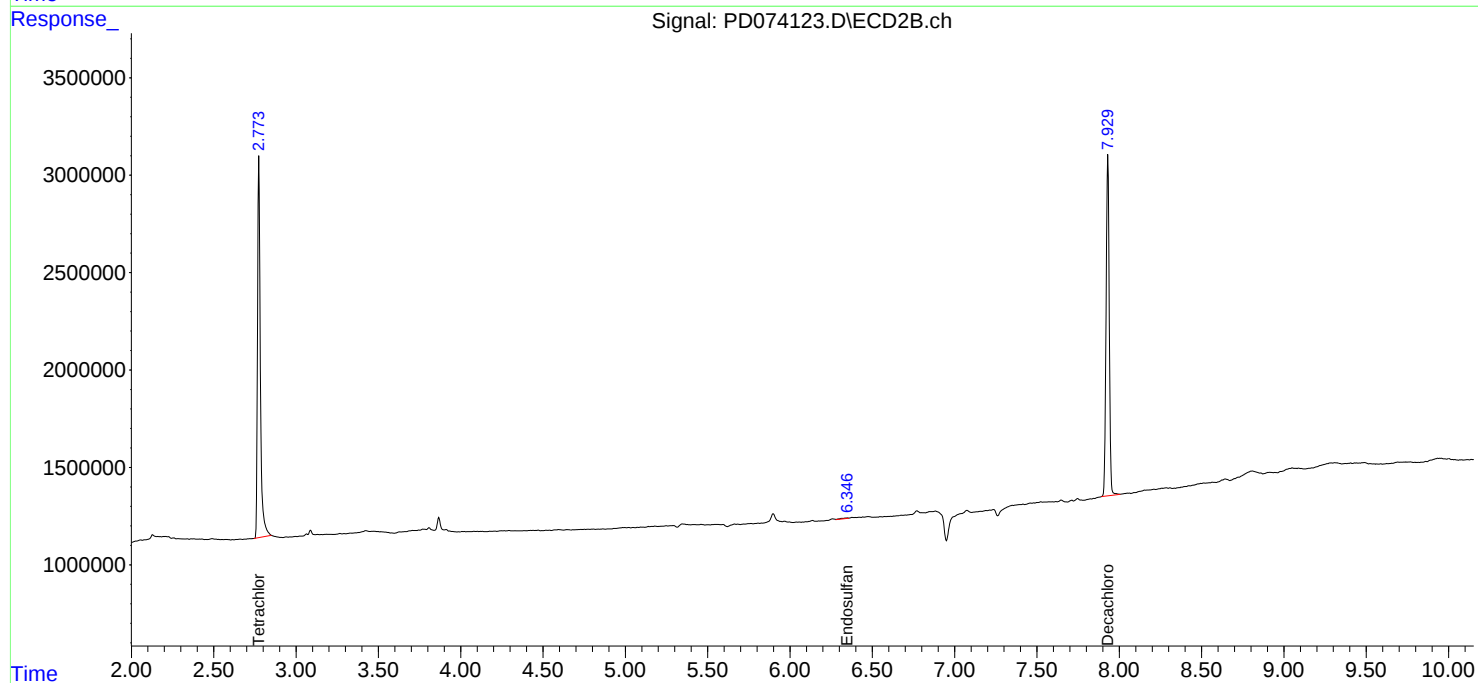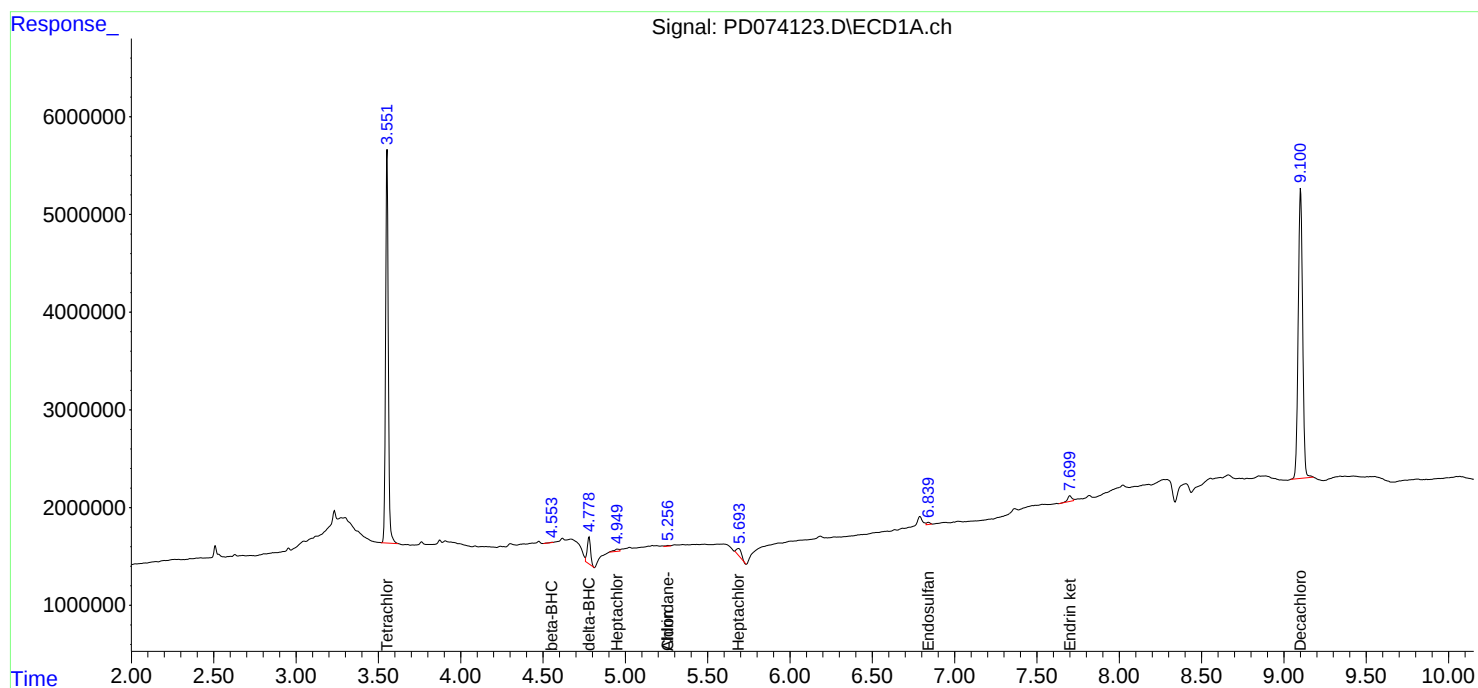


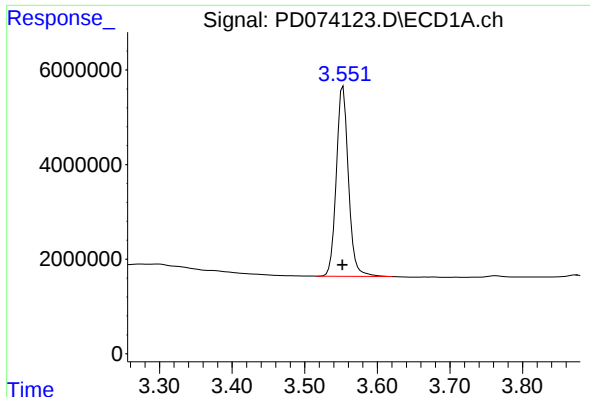

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 46538574
Conc: 20.31 ng/ml

Instrument :
ECD_O
ClientSampleId :

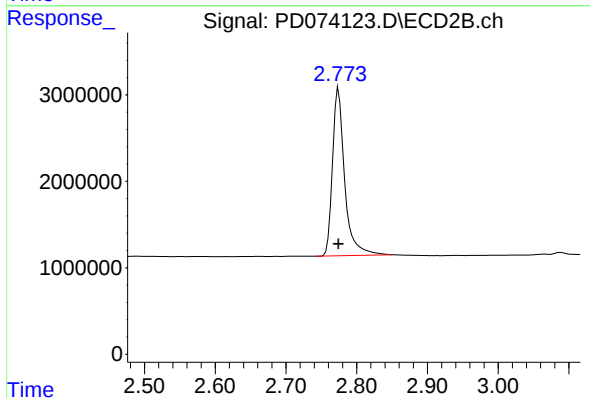


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 23205033
Conc: 19.59 ng/ml

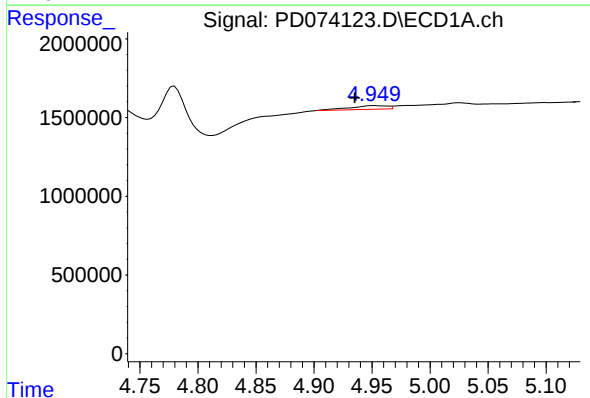


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.016 min
Response: 539140
Conc: 0.16 ng/ml

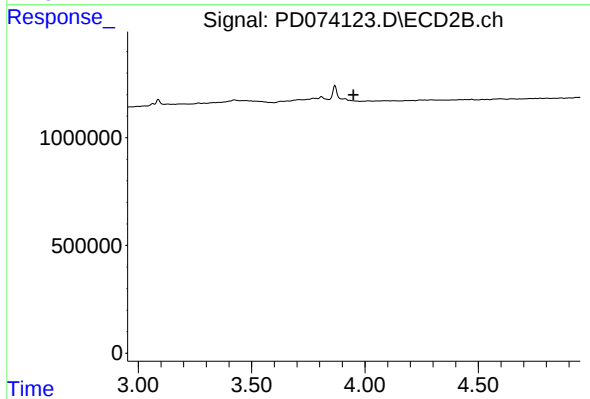

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.950 min
Response: 0
Conc: N.D.

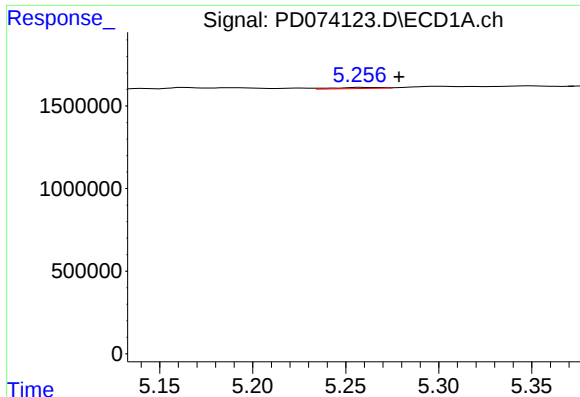

#5 Aldrin


R.T.: 5.259 min
Delta R.T.: -0.020 min
Response: 131294
Conc: 0.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

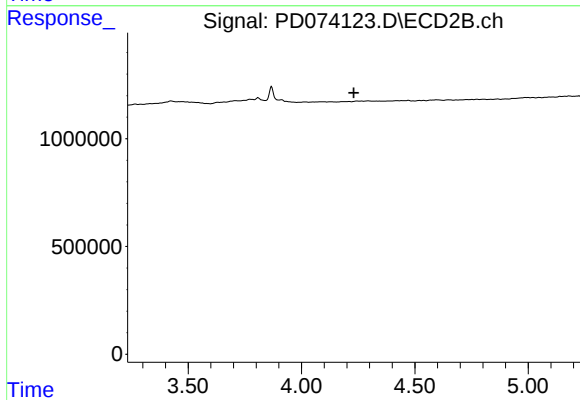


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.231 min
Response: 0
Conc: N.D.

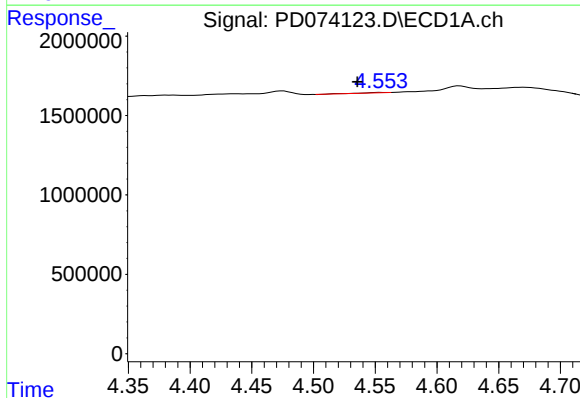


#6 beta-BHC

R.T.: 4.555 min
Delta R.T.: 0.019 min
Response: 32279
Conc: 0.02 ng/ml

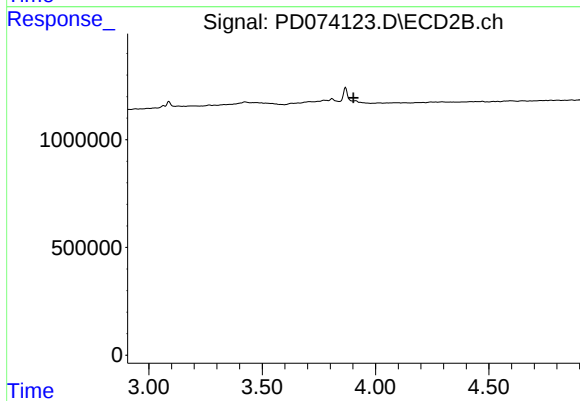

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

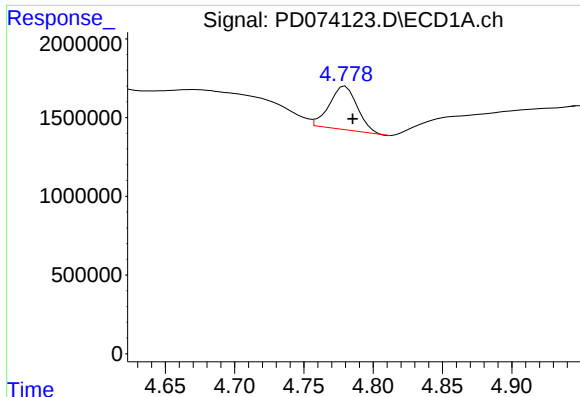

#7 delta-BHC


R.T.: 4.780 min
Delta R.T.: -0.005 min
Response: 3892882
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :

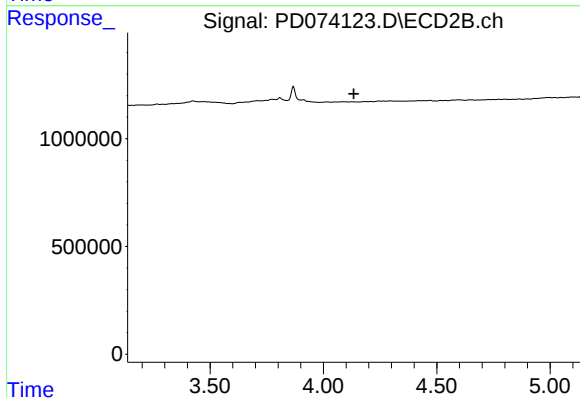


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.135 min
Response: 0
Conc: N.D.

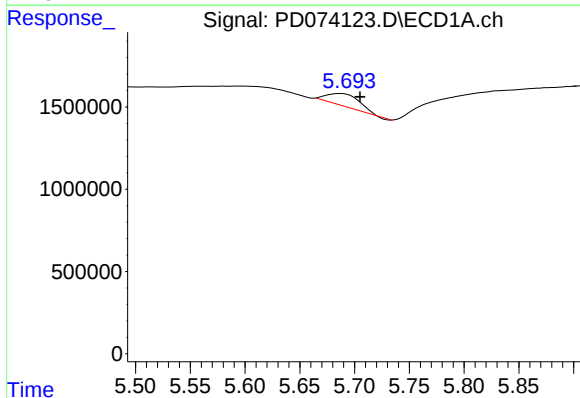


#8 Heptachlor epoxide

R.T.: 5.688 min
Delta R.T.: -0.018 min
Response: 1566289
Conc: 0.55 ng/ml

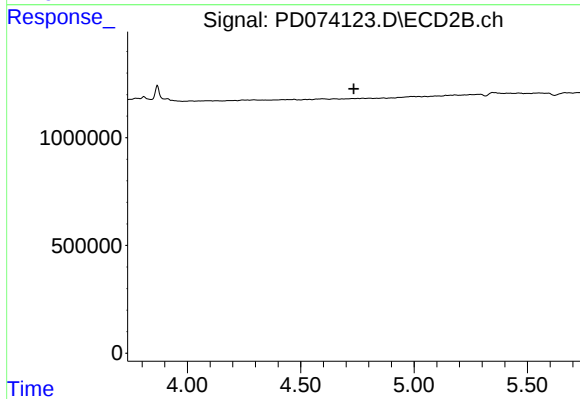

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

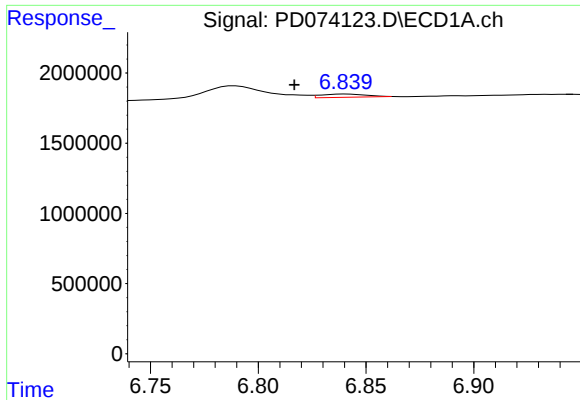

#15 Endosulfan II


R.T.: 6.841 min
Delta R.T.: 0.024 min
Response: 368231
Conc: 0.13 ng/ml

Instrument :
ECD_O
ClientSampleId :

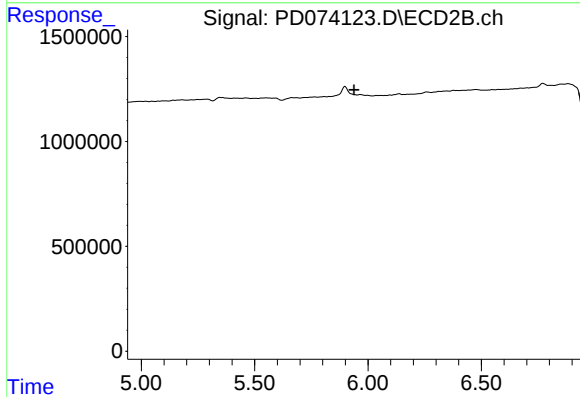


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

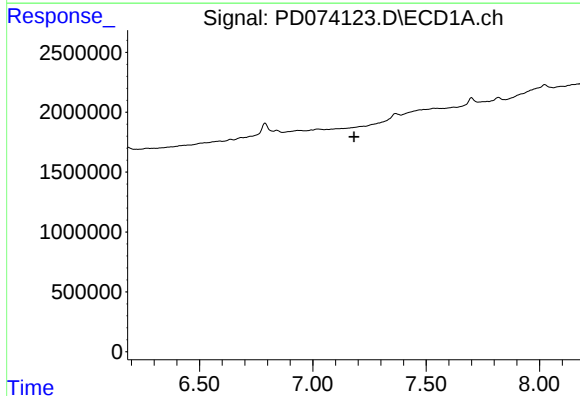


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

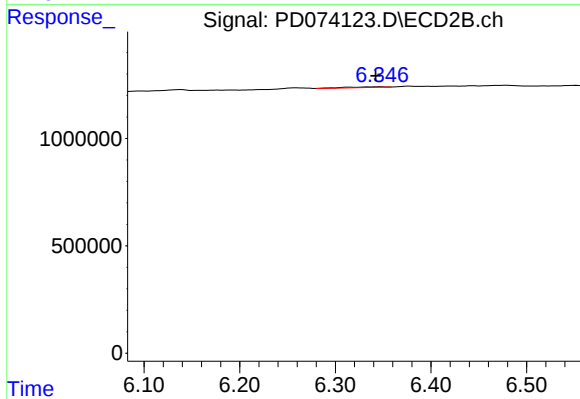

#19 Endosulfan Sulfate


R.T.: 6.348 min
Delta R.T.: 0.005 min
Response: 91516
Conc: 0.08 ng/ml

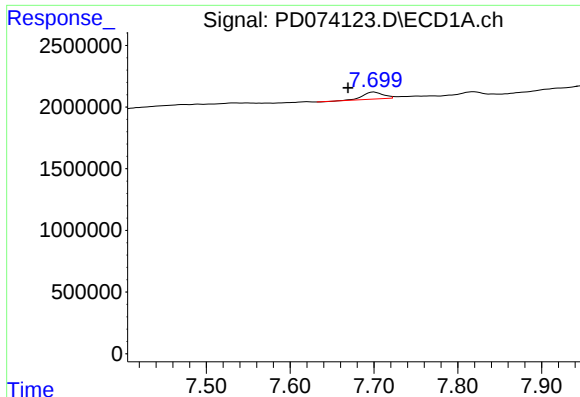

#21 Endrin ketone


R.T.: 7.700 min
Delta R.T.: 0.031 min
Response: 993372
Conc: 0.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

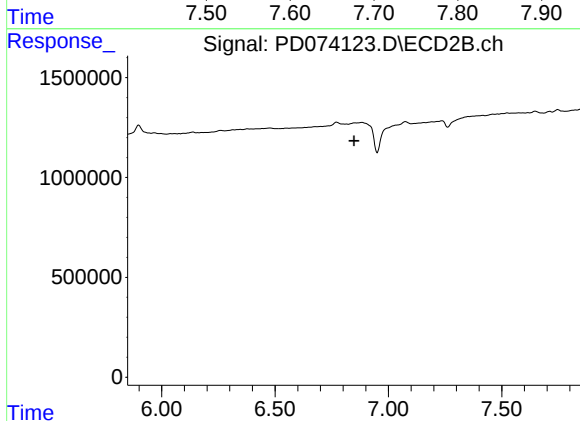


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

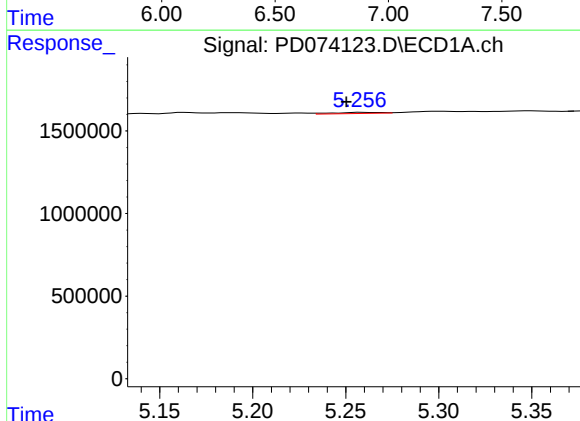


#24 Chlordane-2

R.T.: 5.259 min
Delta R.T.: 0.008 min
Response: 131294
Conc: 0.97 ng/ml

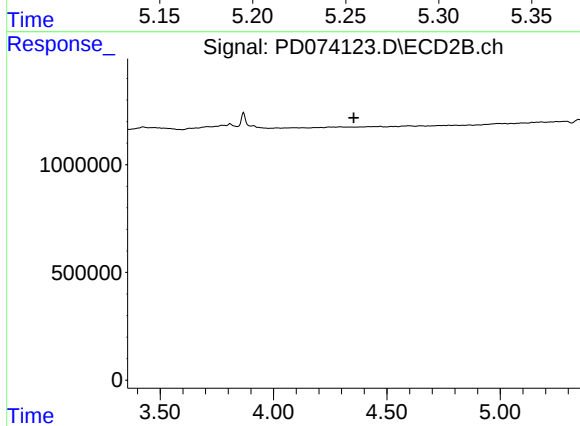

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.353 min
Response: 0
Conc: N.D.

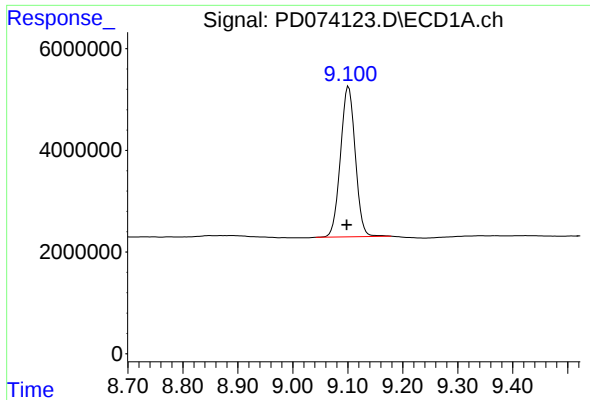

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.003 min
Response: 55316426
Conc: 20.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

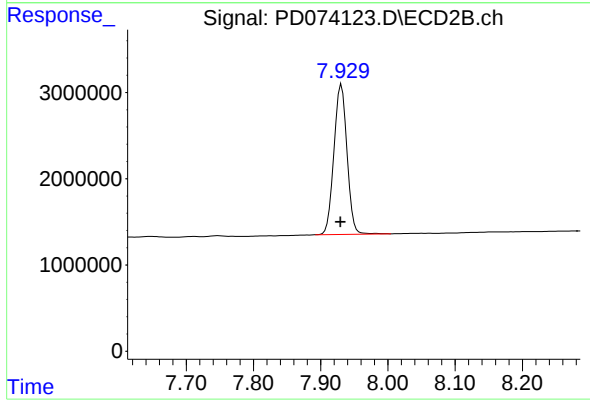

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: 0.001 min
Response: 23334654
Conc: 19.06 ng/ml