

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030321\
 Data File : P0075828.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2021 10:58
 Operator : AJ/MA
 Sample : AR1262CCC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262CCC500

Manual Integrations
 APPROVED

Ankita
 3/4/2021 10:34:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 12:45:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.941	3.954	3475641	2499360	56.859	56.574
2) SA Decachlor...	10.958	9.224	2262978	2060518	49.733	47.482
Target Compounds						
36) L8 AR-1262-1	8.589	7.313	1578037	928699	437.816	443.388
37) L8 AR-1262-2	9.146	7.863	2764545	2993993	422.339	431.937
38) L8 AR-1262-3	9.455	8.149	1866802	1231785	428.200m	433.034
39) L8 AR-1262-4	9.551	8.213	1396594	2192616	414.660m	435.133
40) L8 AR-1262-5	10.213	8.708	993135	1023271	413.332	438.747

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030321\
Data File : PO075828.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2021 10:58
Operator : AJ/MA
Sample : AR1262CCC500
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 12:45:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

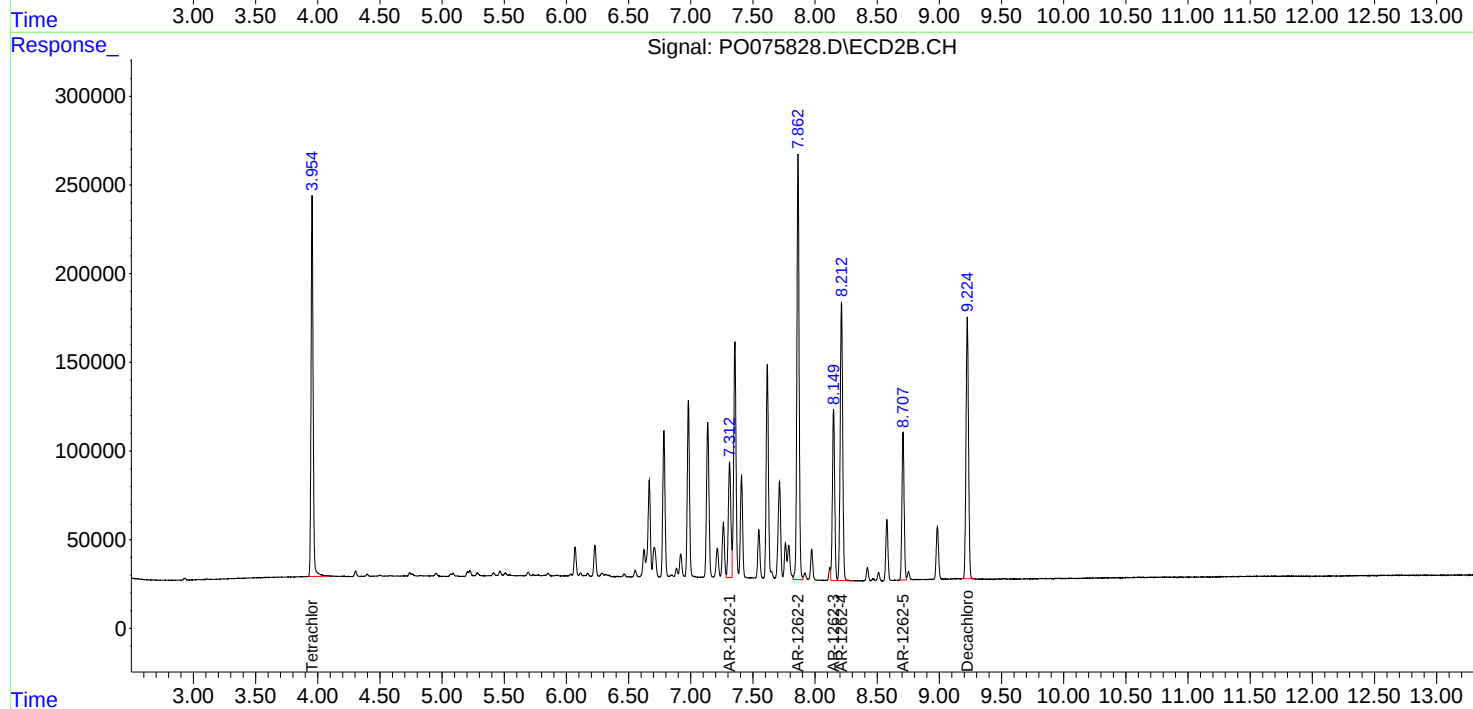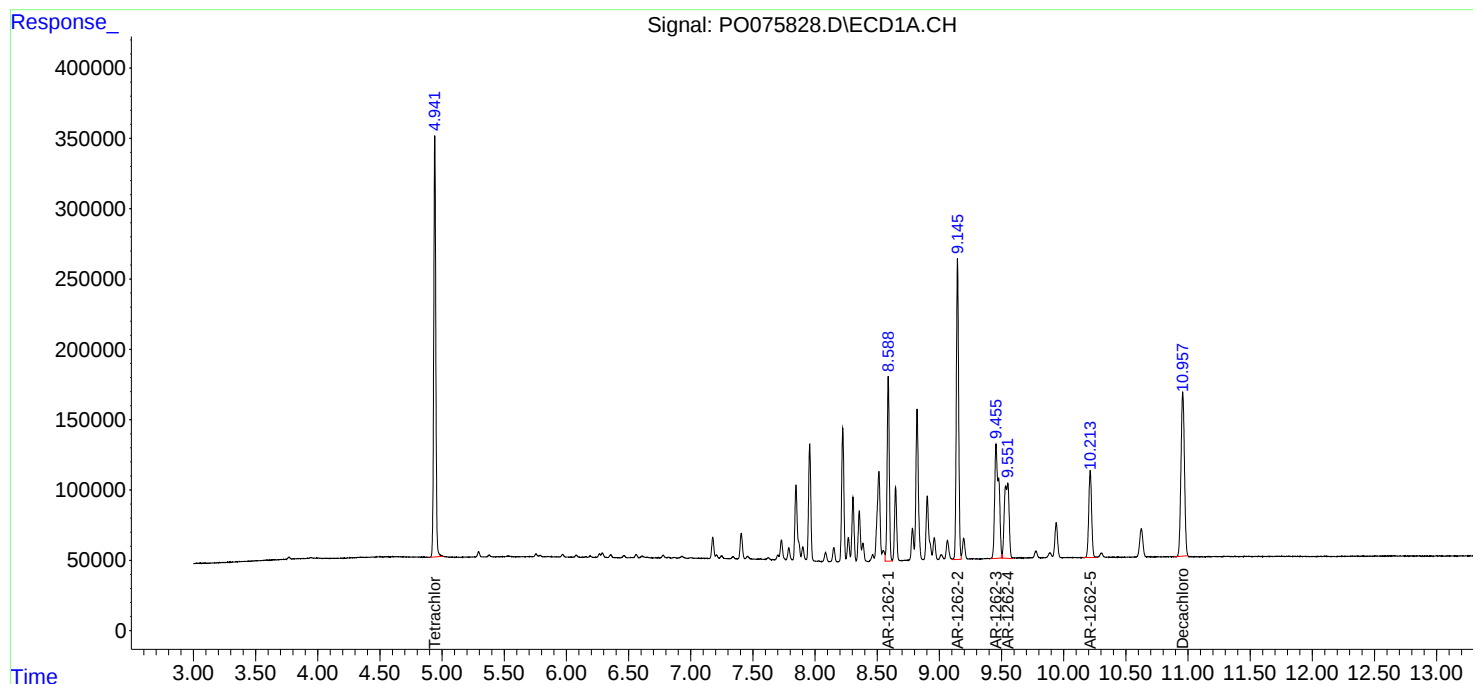

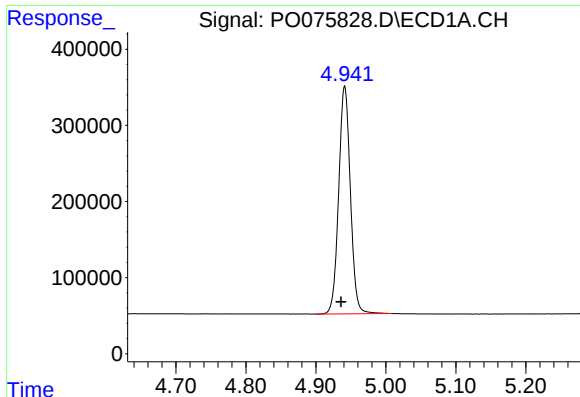


#1 Tetrachloro-m-xylene

R.T.: 4.941 min
Delta R.T.: 0.005 min
Response: 3475641
Conc: 56.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:55 AM

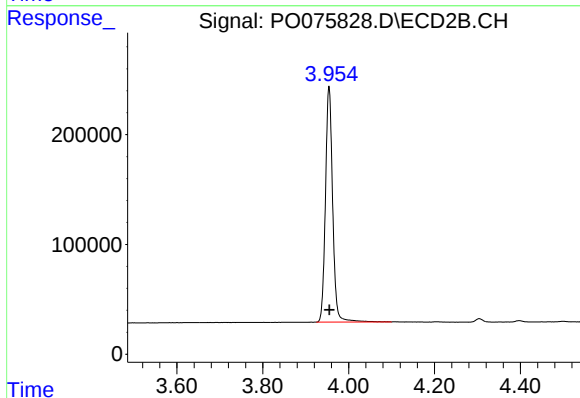


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 2499360
Conc: 56.57 ng/ml

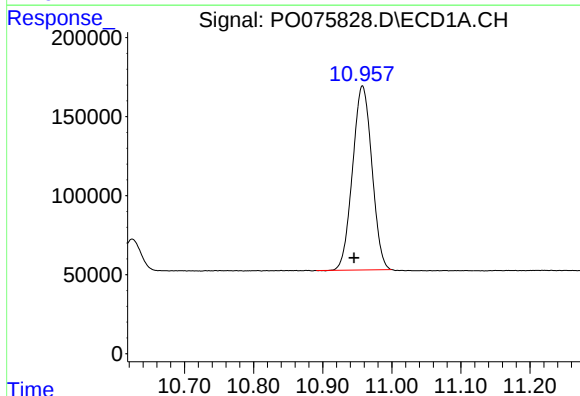


#2 Decachlorobiphenyl

R.T.: 10.958 min
Delta R.T.: 0.012 min
Response: 2262978
Conc: 49.73 ng/ml

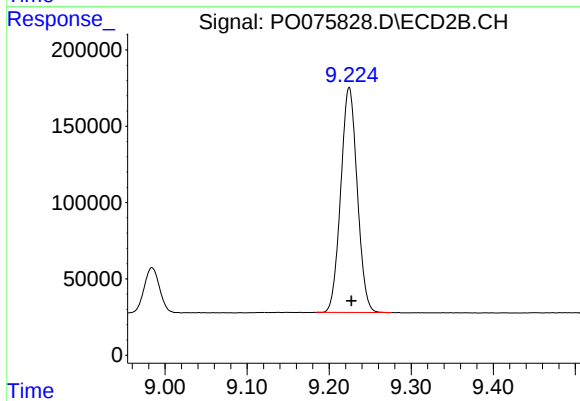

#2 Decachlorobiphenyl

R.T.: 9.224 min
Delta R.T.: -0.003 min
Response: 2060518
Conc: 47.48 ng/ml

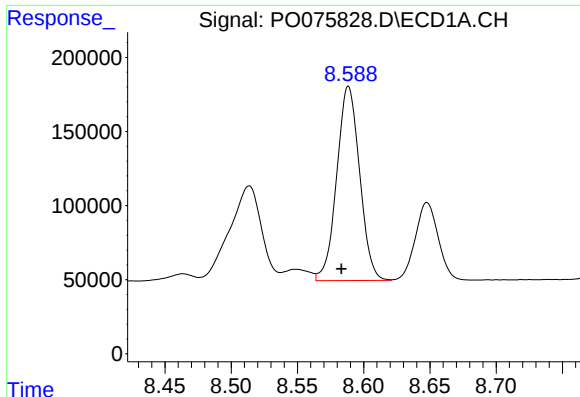


#36 AR-1262-1

R.T.: 8.589 min
Delta R.T.: 0.005 min
Response: 1578037
Conc: 437.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:55 AM

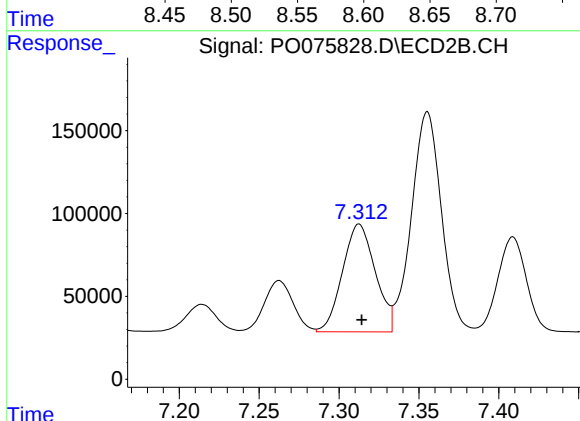


#36 AR-1262-1

R.T.: 7.313 min
Delta R.T.: -0.002 min
Response: 928699
Conc: 443.39 ng/ml

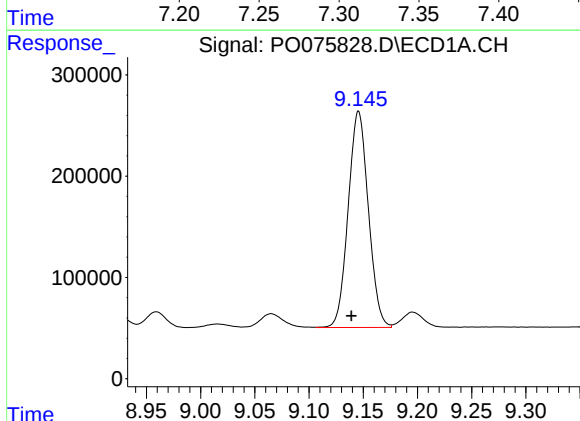


#37 AR-1262-2

R.T.: 9.146 min
Delta R.T.: 0.007 min
Response: 2764545
Conc: 422.34 ng/ml

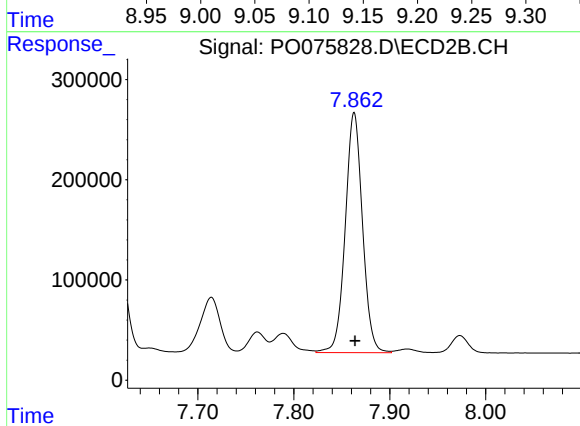

#37 AR-1262-2

R.T.: 7.863 min
Delta R.T.: -0.001 min
Response: 2993993
Conc: 431.94 ng/ml

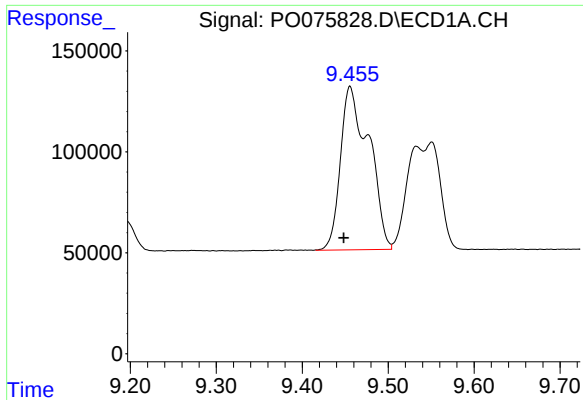


#38 AR-1262-3

R.T.: 9.455 min
Delta R.T.: 0.007 min
Response: 1866802
Conc: 428.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:55 AM

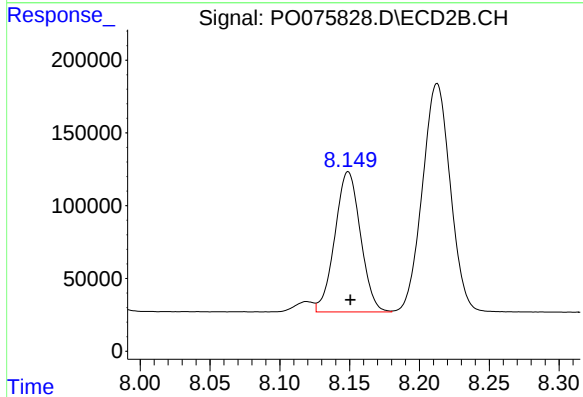


#38 AR-1262-3

R.T.: 8.149 min
Delta R.T.: -0.002 min
Response: 1231785
Conc: 433.03 ng/ml

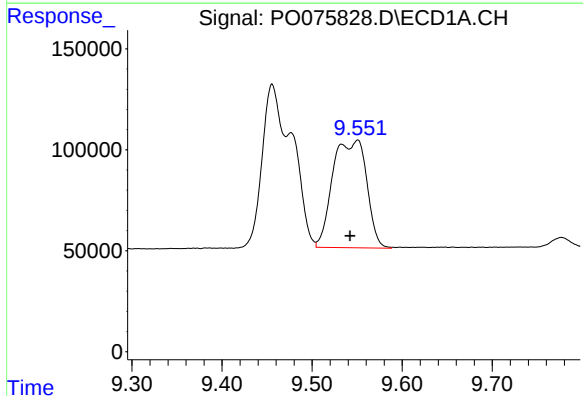


#39 AR-1262-4

R.T.: 9.551 min
Delta R.T.: 0.008 min
Response: 1396594
Conc: 414.66 ng/ml m

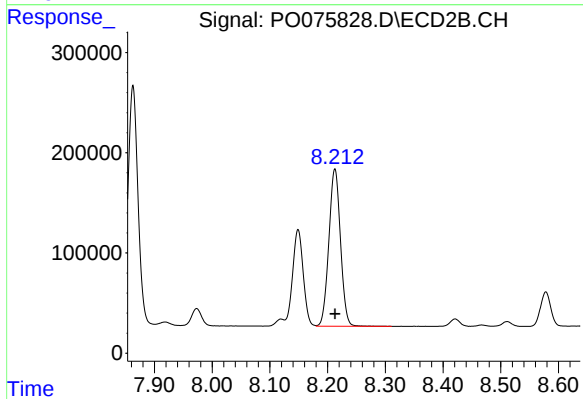

#39 AR-1262-4

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 2192616
Conc: 435.13 ng/ml

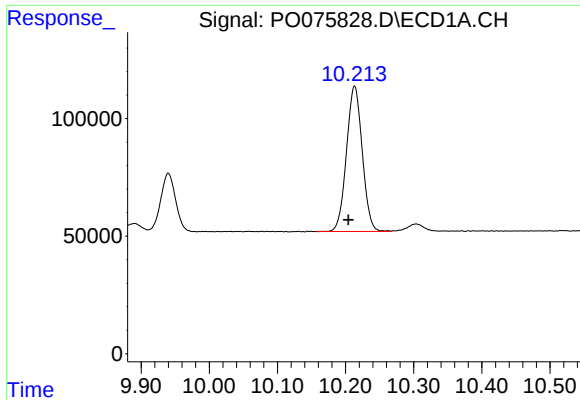


#40 AR-1262-5

R.T.: 10.213 min
Delta R.T.: 0.009 min
Response: 993135
Conc: 413.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500

Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:55 AM

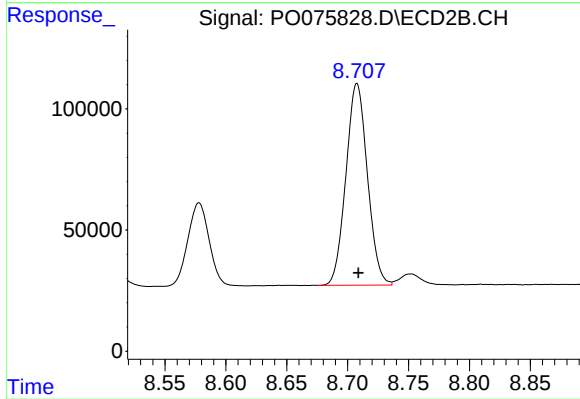

#40 AR-1262-5

R.T.: 8.708 min
Delta R.T.: -0.001 min
Response: 1023271
Conc: 438.75 ng/ml