

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030321\
 Data File : P0075831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2021 12:06
 Operator : AJ/MA
 Sample : M1530-03 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF265P-2-2

Manual Integrations
 APPROVED

Ankita
 3/4/2021 10:34:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 12:46:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.952	138234	109444	2.261	2.477
2) SA Decachlor...	10.955	9.223	108357	111437	2.381m	2.568
Target Compounds						
36) L8 AR-1262-1	8.586	7.311	132611	38776	36.792	18.513 #
37) L8 AR-1262-2	9.143	7.861	159857	186429	24.421m	26.896
38) L8 AR-1262-3	9.454	8.147	239801	225358	55.005	79.225 #
39) L8 AR-1262-4	9.548	8.211	344679	307965	102.338	61.117 #
40) L8 AR-1262-5	10.211	8.706	135892	144931	56.557	62.142

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030321\
Data File : PO075831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2021 12:06
Operator : AJ/MA
Sample : M1530-03 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HEF265P-2-2


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 12:46:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

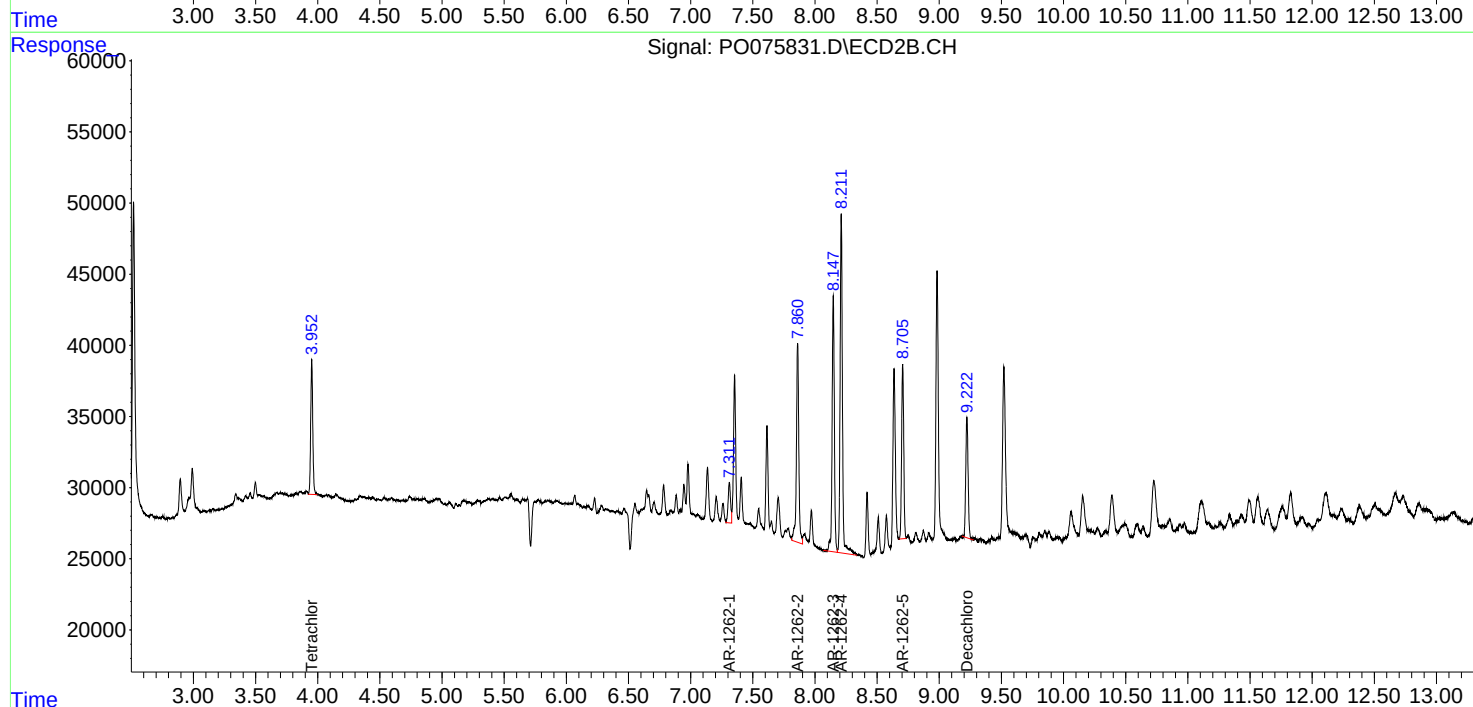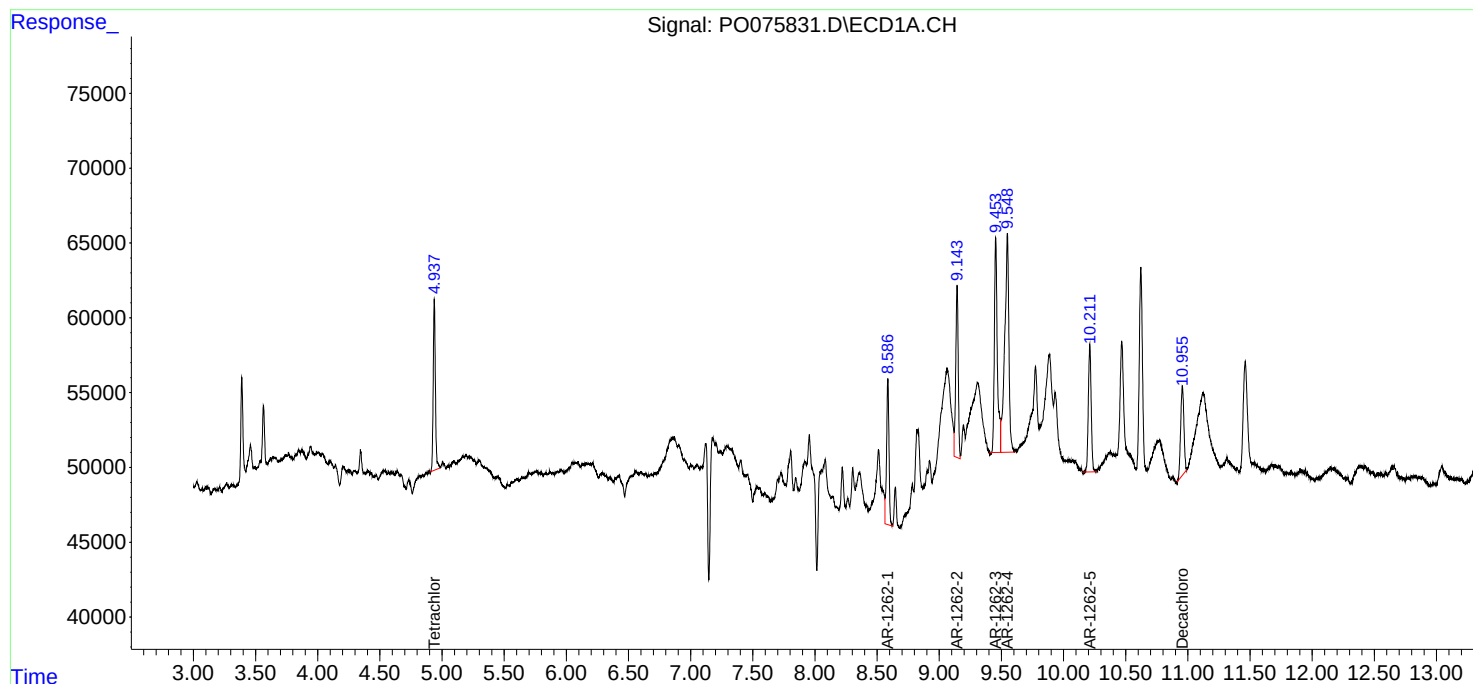

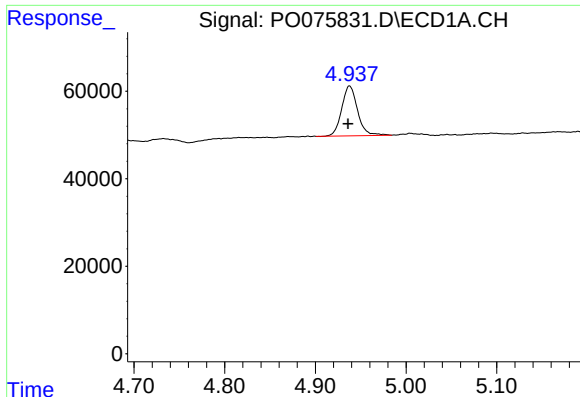


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: 0.002 min
Response: 138234
Conc: 2.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF265P-2-2


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:59 AM

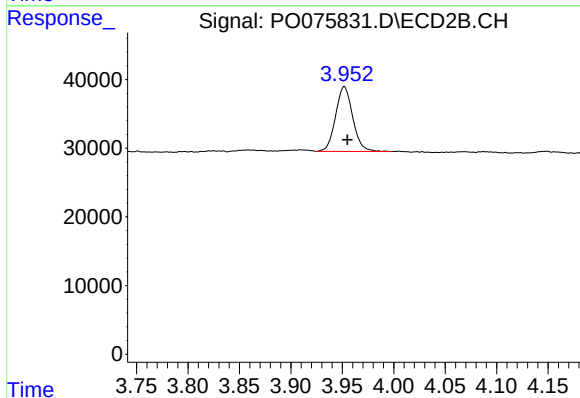


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: -0.003 min
Response: 109444
Conc: 2.48 ng/ml

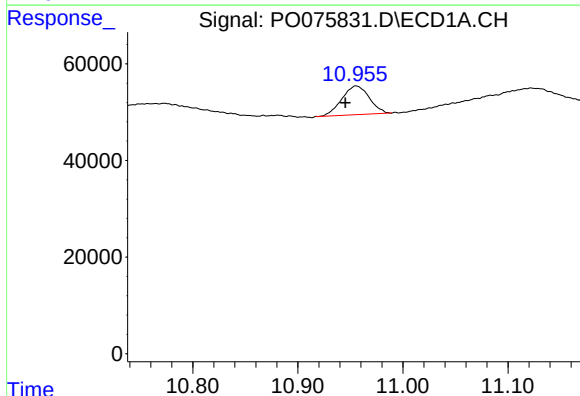


#2 Decachlorobiphenyl

R.T.: 10.955 min
Delta R.T.: 0.009 min
Response: 108357
Conc: 2.38 ng/ml m

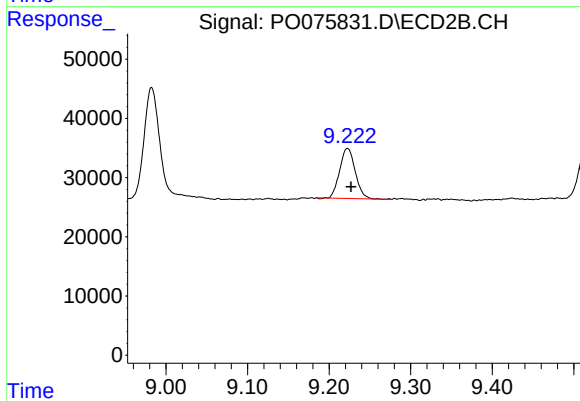

#2 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 111437
Conc: 2.57 ng/ml

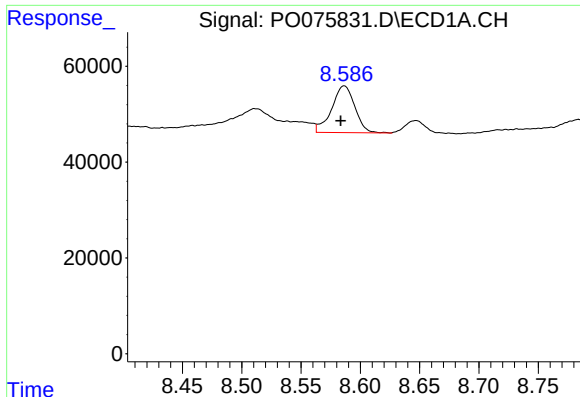


#36 AR-1262-1

R.T.: 8.586 min
Delta R.T.: 0.003 min
Response: 132611
Conc: 36.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF265P-2-2


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:59 AM

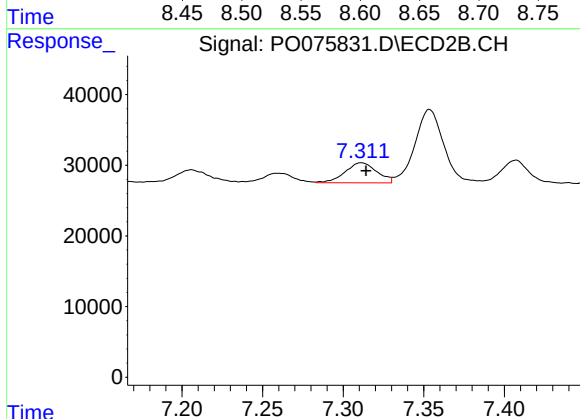


#36 AR-1262-1

R.T.: 7.311 min
Delta R.T.: -0.003 min
Response: 38776
Conc: 18.51 ng/ml

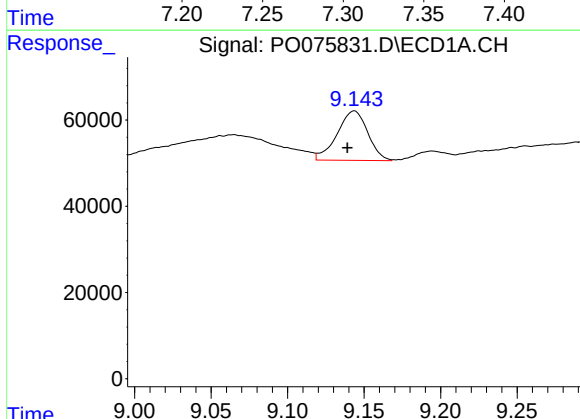


#37 AR-1262-2

R.T.: 9.143 min
Delta R.T.: 0.004 min
Response: 159857
Conc: 24.42 ng/ml m

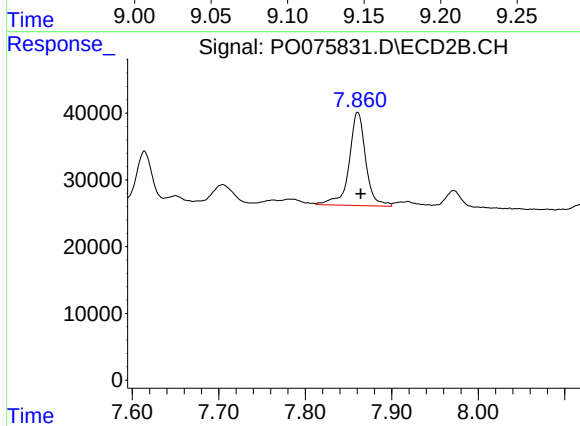

#37 AR-1262-2

R.T.: 7.861 min
Delta R.T.: -0.003 min
Response: 186429
Conc: 26.90 ng/ml

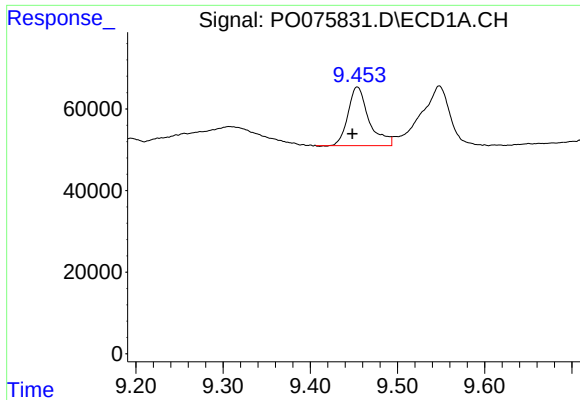


#38 AR-1262-3

R.T.: 9.454 min
Delta R.T.: 0.006 min
Response: 239801
Conc: 55.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF265P-2-2


Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:59 AM

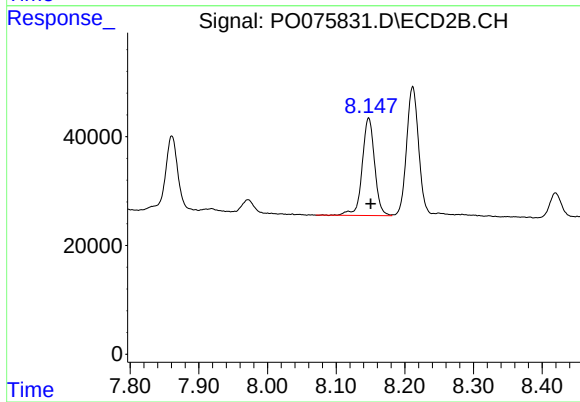


#38 AR-1262-3

R.T.: 8.147 min
Delta R.T.: -0.003 min
Response: 225358
Conc: 79.22 ng/ml

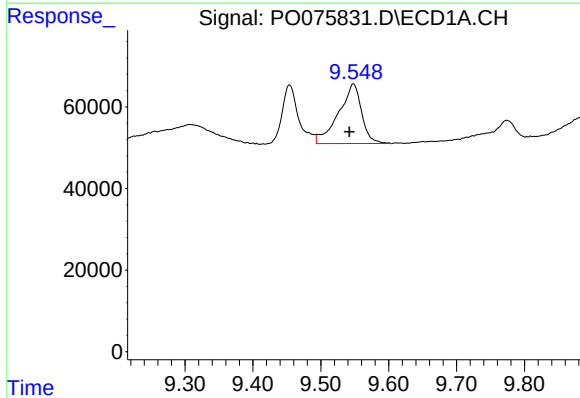


#39 AR-1262-4

R.T.: 9.548 min
Delta R.T.: 0.006 min
Response: 344679
Conc: 102.34 ng/ml

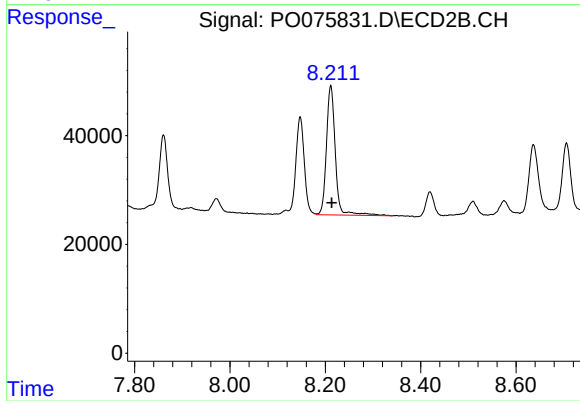

#39 AR-1262-4

R.T.: 8.211 min
Delta R.T.: -0.002 min
Response: 307965
Conc: 61.12 ng/ml

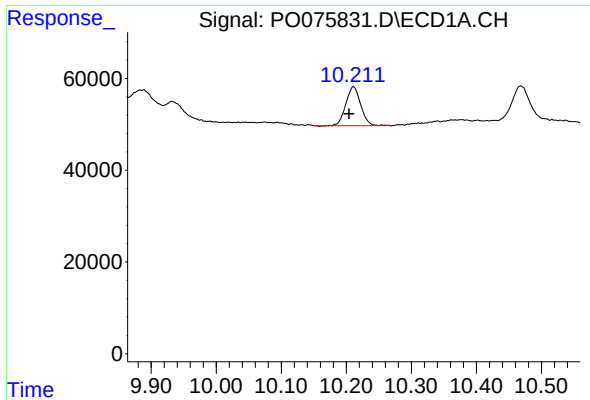


#40 AR-1262-5

R.T.: 10.211 min
Delta R.T.: 0.007 min
Response: 135892
Conc: 56.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF265P-2-2

Manual Integrations
APPROVED

Ankita
3/4/2021 10:34:59 AM

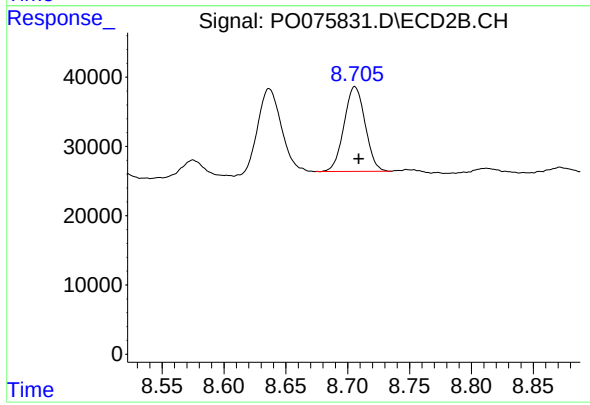

#40 AR-1262-5

R.T.: 8.706 min
Delta R.T.: -0.003 min
Response: 144931
Conc: 62.14 ng/ml