

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030321\
 Data File : P0075839.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2021 14:23
 Operator : AJ/MA
 Sample : M1528-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-CON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 15:19:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.952	1472188	1086733	24.084	24.599
2) SA Decachlor...	10.954	9.222	875177	823467	19.234	18.976

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030321\
Data File : P0075839.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2021 14:23
Operator : AJ/MA
Sample : M1528-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MW-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 15:19:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

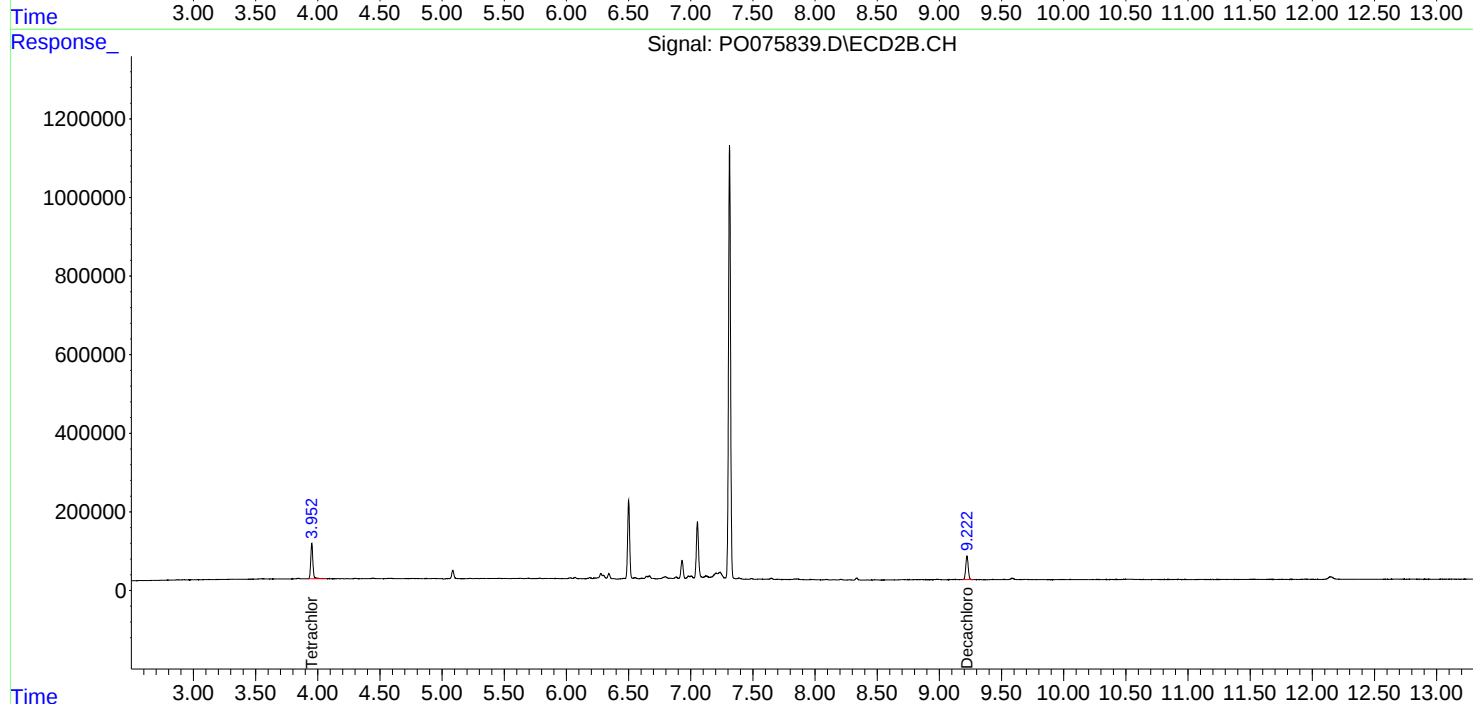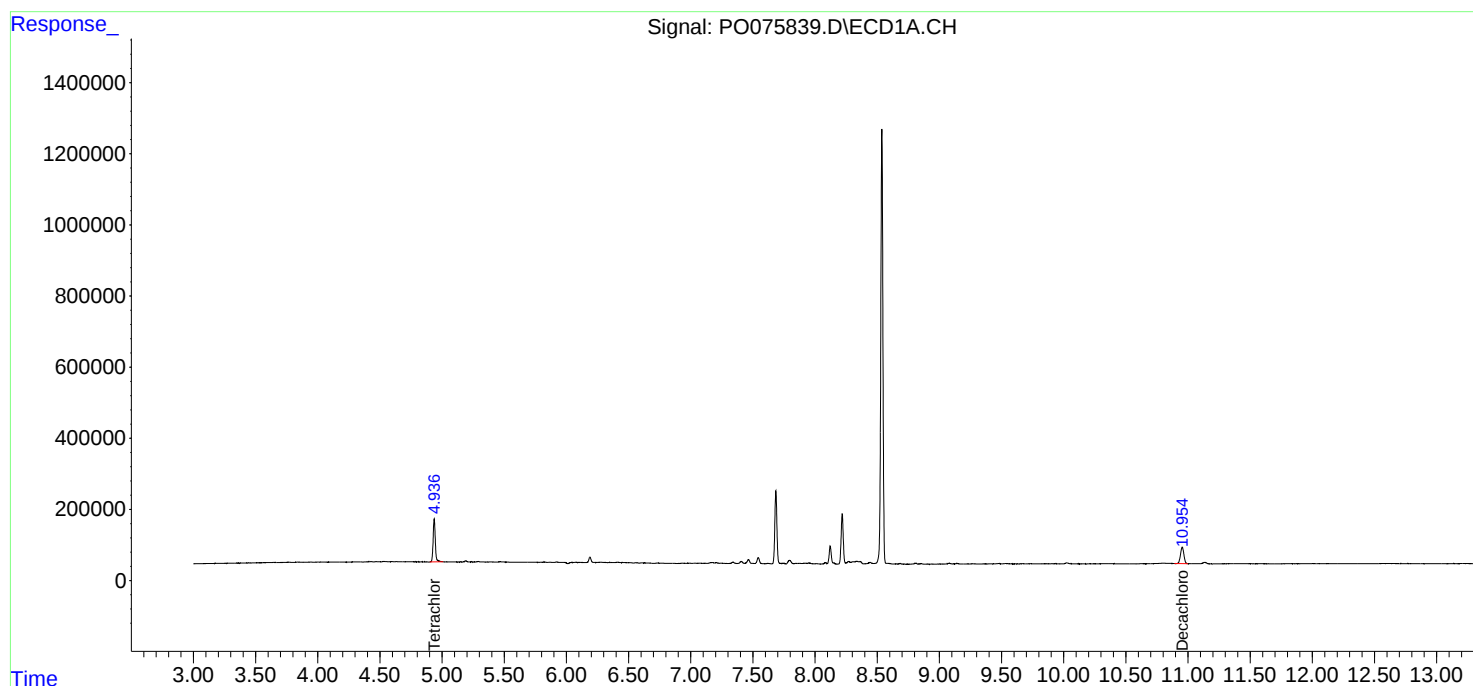


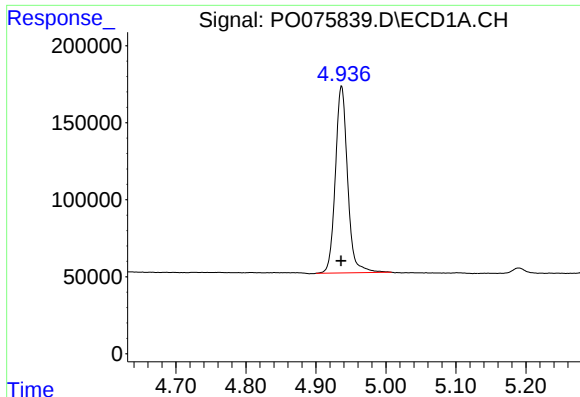

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 1472188
Conc: 24.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-CON

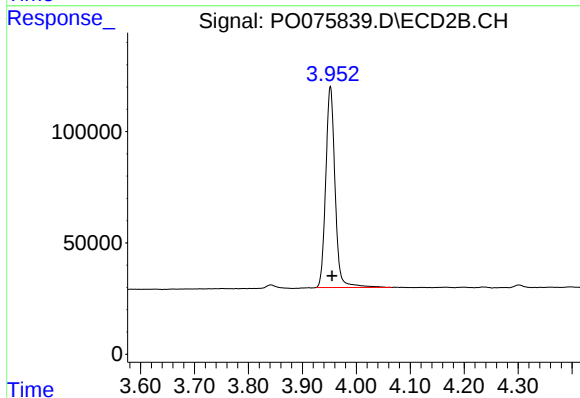


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: -0.003 min
Response: 1086733
Conc: 24.60 ng/ml

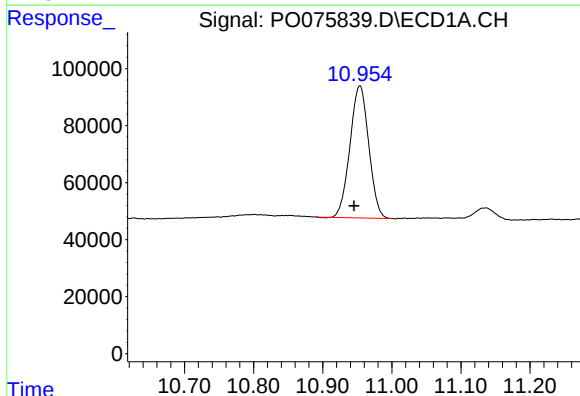

#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: 0.008 min
Response: 875177
Conc: 19.23 ng/ml

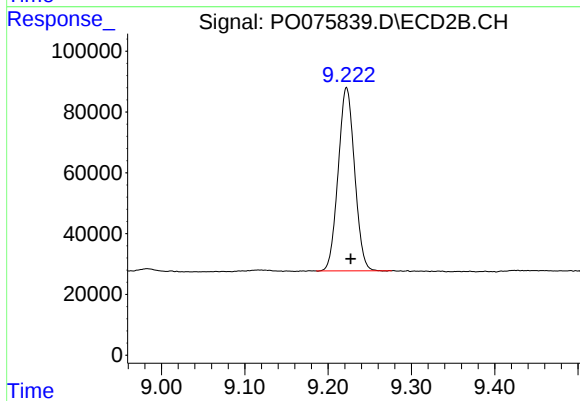

#2 Decachlorobiphenyl

R.T.: 9.222 min
Delta R.T.: -0.005 min
Response: 823467
Conc: 18.98 ng/ml