

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030322\
 Data File : P0085059.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 16:30
 Operator : YP\AJ
 Sample : N1727-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220215-096-21-03-ELUTRIATE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:20:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.510	3.597	4857721	933073	17.374	20.748
2) SA Decachlor...	10.433	8.621	2297862	547609	13.109	14.903

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030322\
Data File : P0085059.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 16:30
Operator : YP\AJ
Sample : N1727-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220215-096-21-03-ELUTRIATE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:20:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

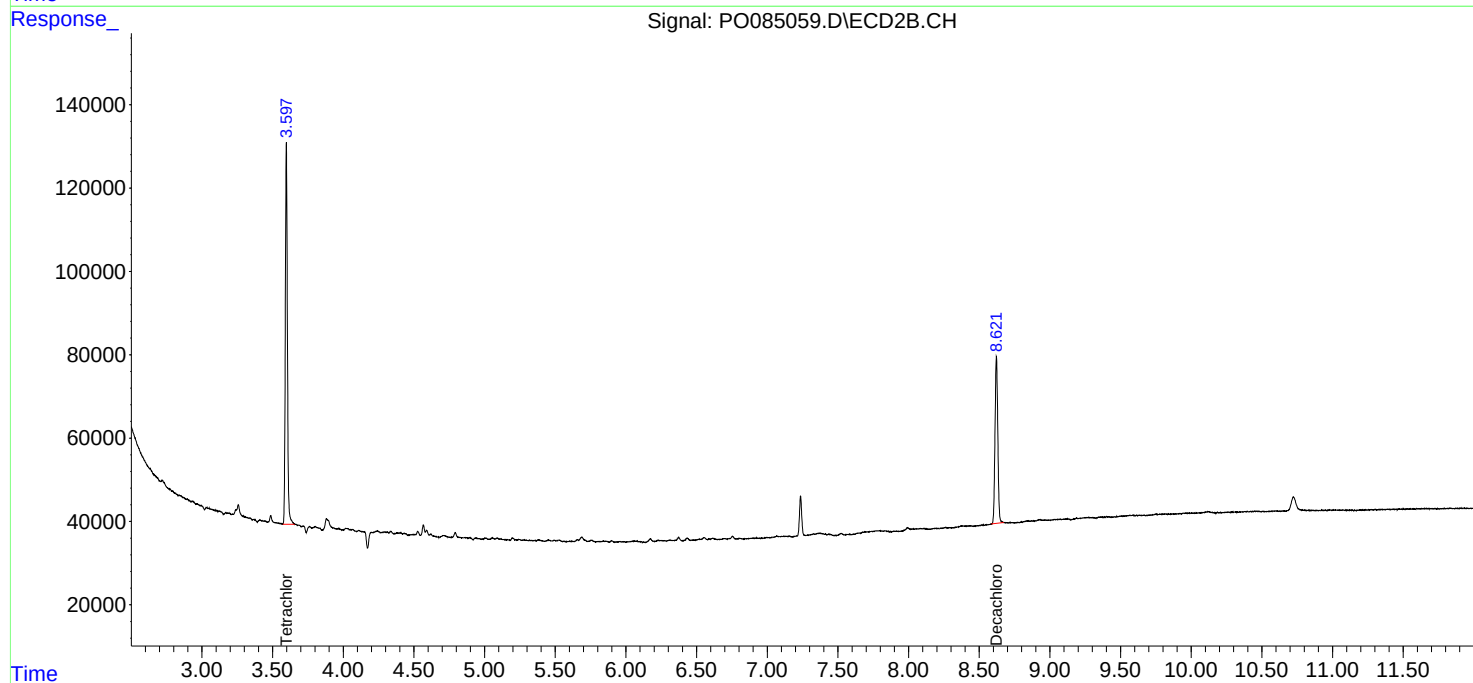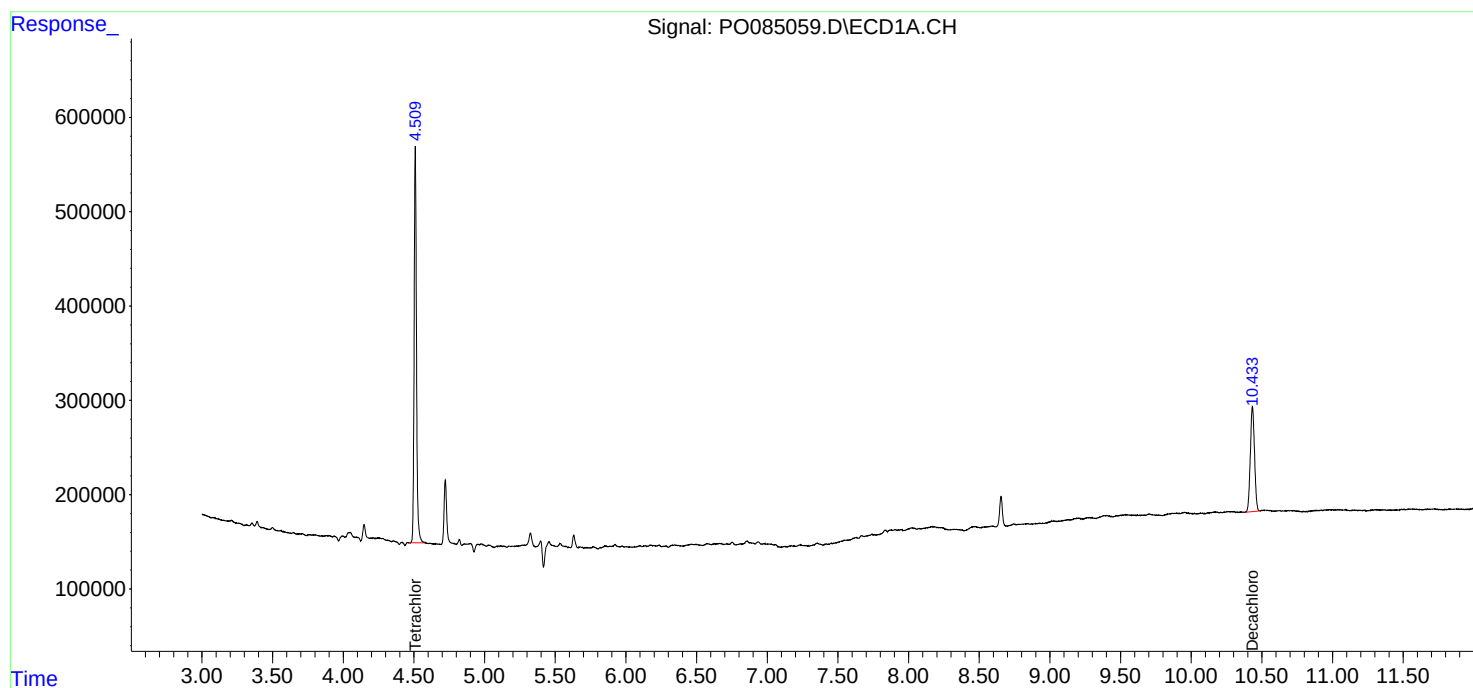


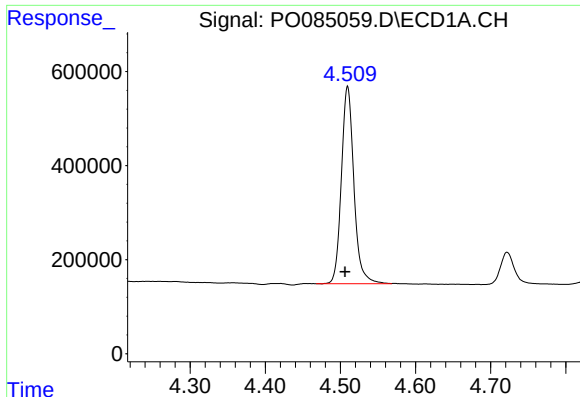

#1 Tetrachloro-m-xylene


R.T.: 4.510 min
Delta R.T.: 0.004 min
Response: 4857721
Conc: 17.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220215-096-21-03-ELUTRIATE

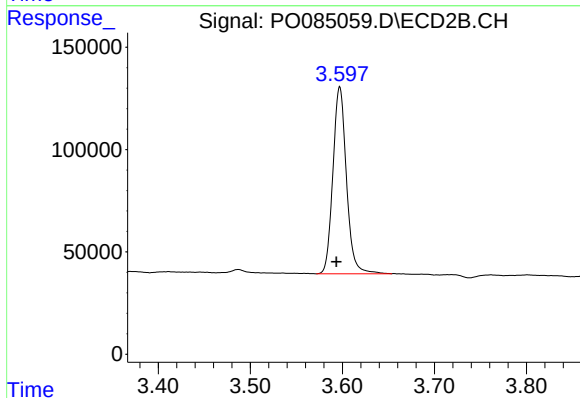


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.004 min
Response: 933073
Conc: 20.75 ng/ml

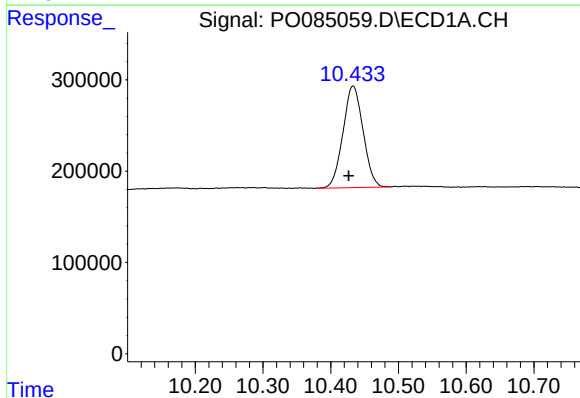

#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.006 min
Response: 2297862
Conc: 13.11 ng/ml

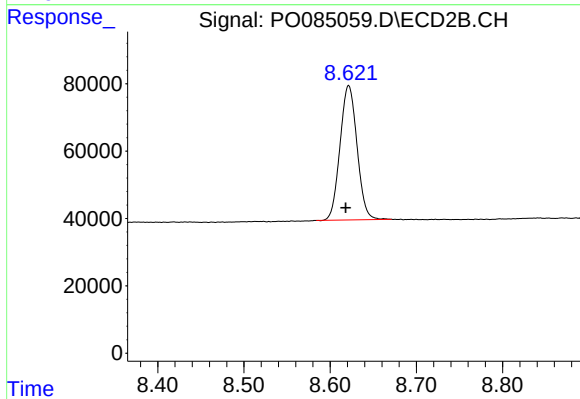

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: 0.003 min
Response: 547609
Conc: 14.90 ng/ml