

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030323\
 Data File : P0092927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 11:00
 Operator : YP/AJ
 Sample : PB151157BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB151157BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 16:47:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.443	3.638	56698571	20955182	18.882	16.440
2) SA Decachlor...	10.288	8.679	52746544	22786125	27.422m	19.552 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030323\
Data File : PO092927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 11:00
Operator : YP/AJ
Sample : PB151157BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB151157BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 16:47:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

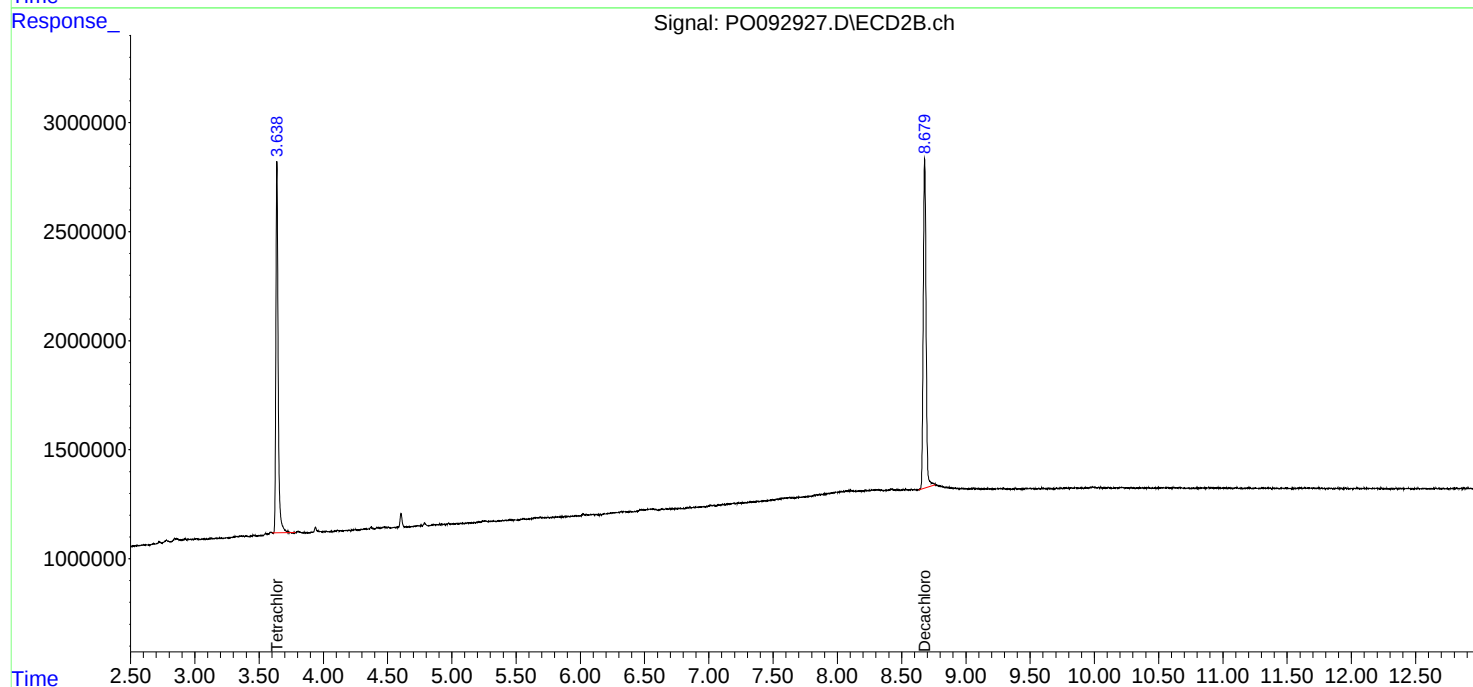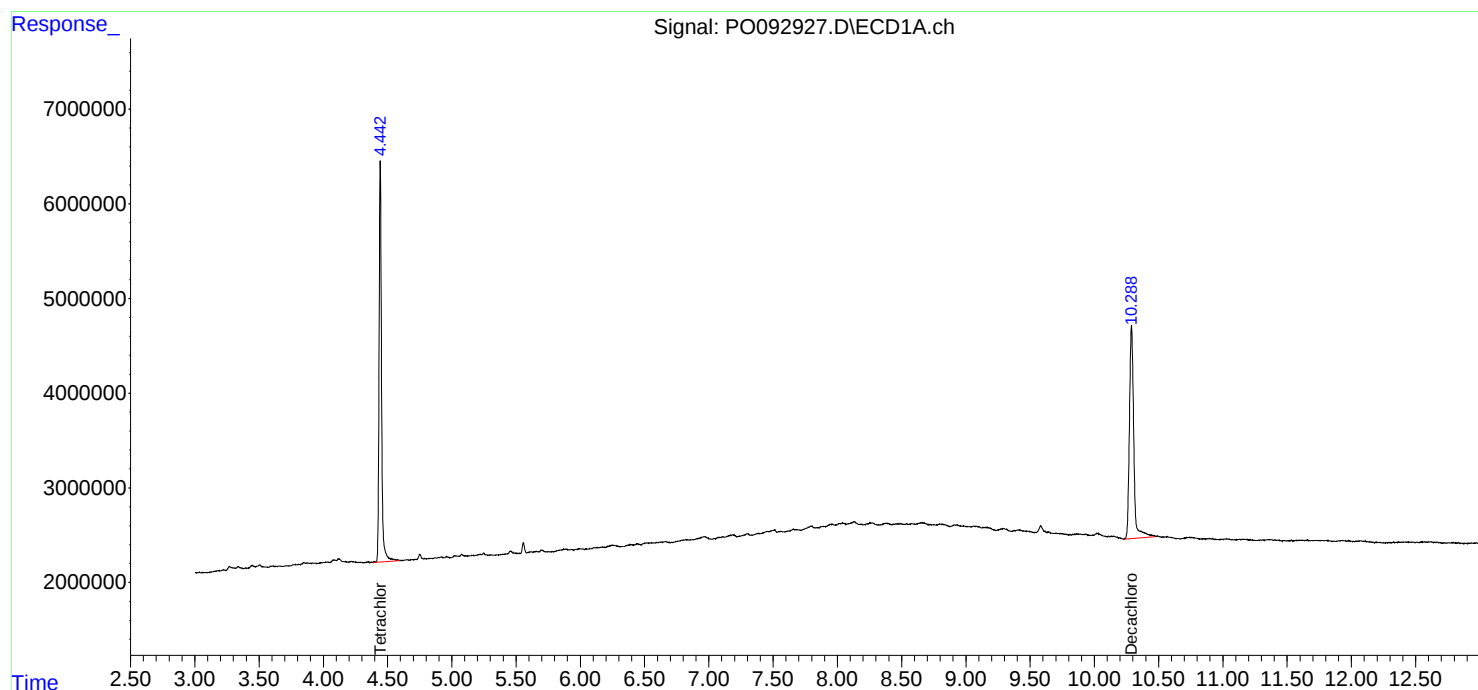

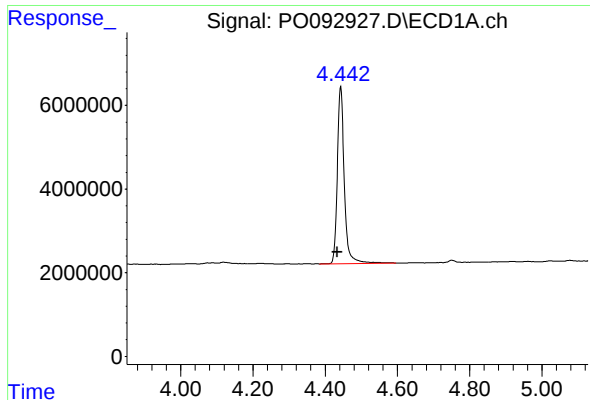


#1 Tetrachloro-m-xylene

R.T.: 4.443 min
Delta R.T.: 0.009 min
Response: 56698571
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB151157BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

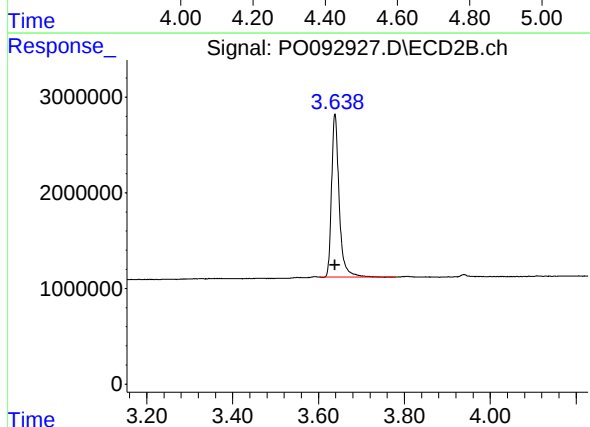


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 20955182
Conc: 16.44 ng/ml

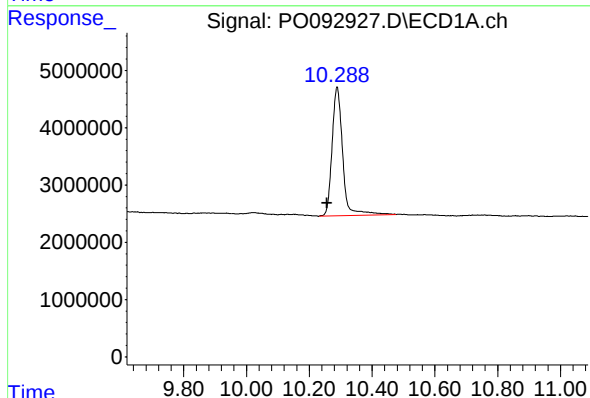

#2 Decachlorobiphenyl

R.T.: 10.288 min
Delta R.T.: 0.032 min
Response: 52746544
Conc: 27.42 ng/ml m

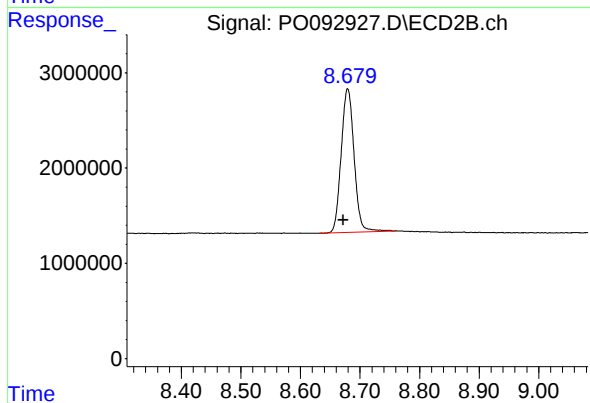

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: 0.007 min
Response: 22786125
Conc: 19.55 ng/ml