

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030323\
 Data File : P0092932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 12:26
 Operator : YP/AJ
 Sample : 01747-04 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF461Z-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 16:48:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.430	3.635	5489540	2076988	1.828m	1.629m
2) SA Decachlor...	10.265	8.669	4498885	2043628	2.339m	1.754m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030323\
Data File : PO092932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 12:26
Operator : YP/AJ
Sample : 01747-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEF461Z-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 16:48:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

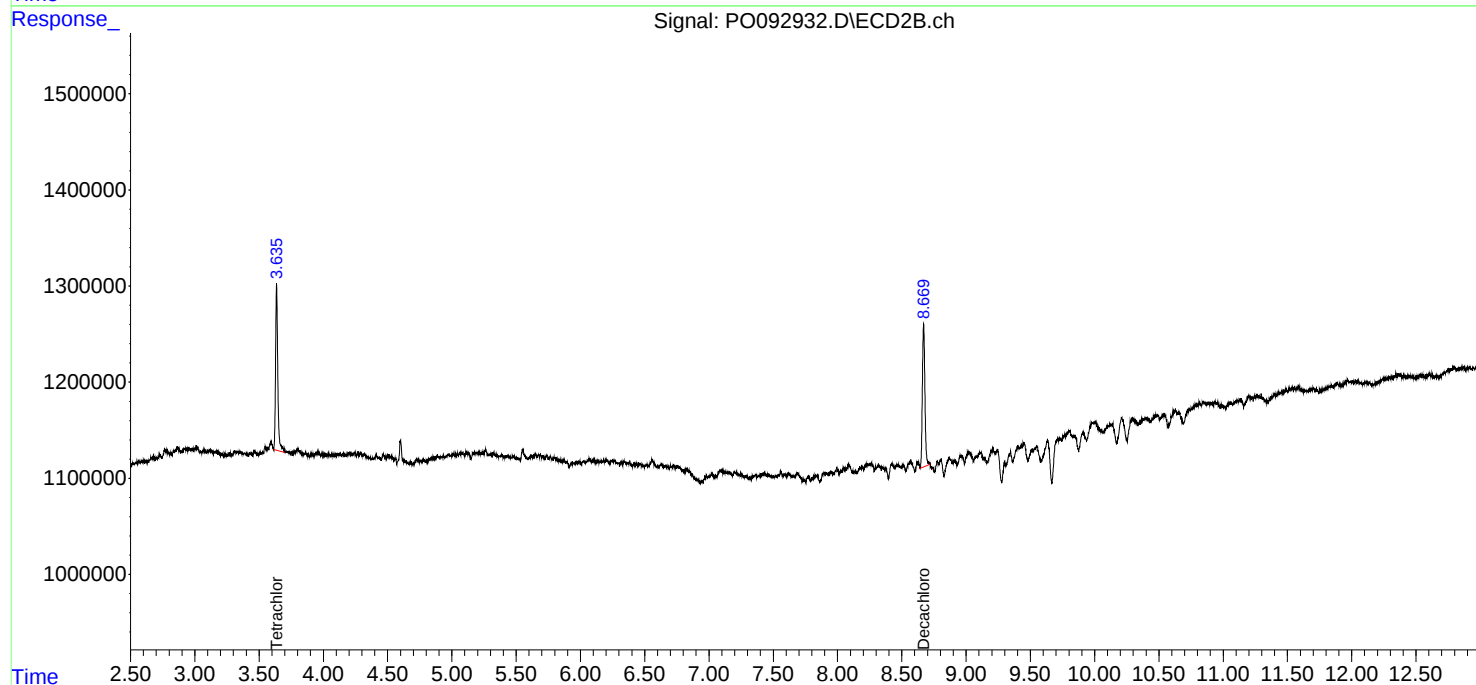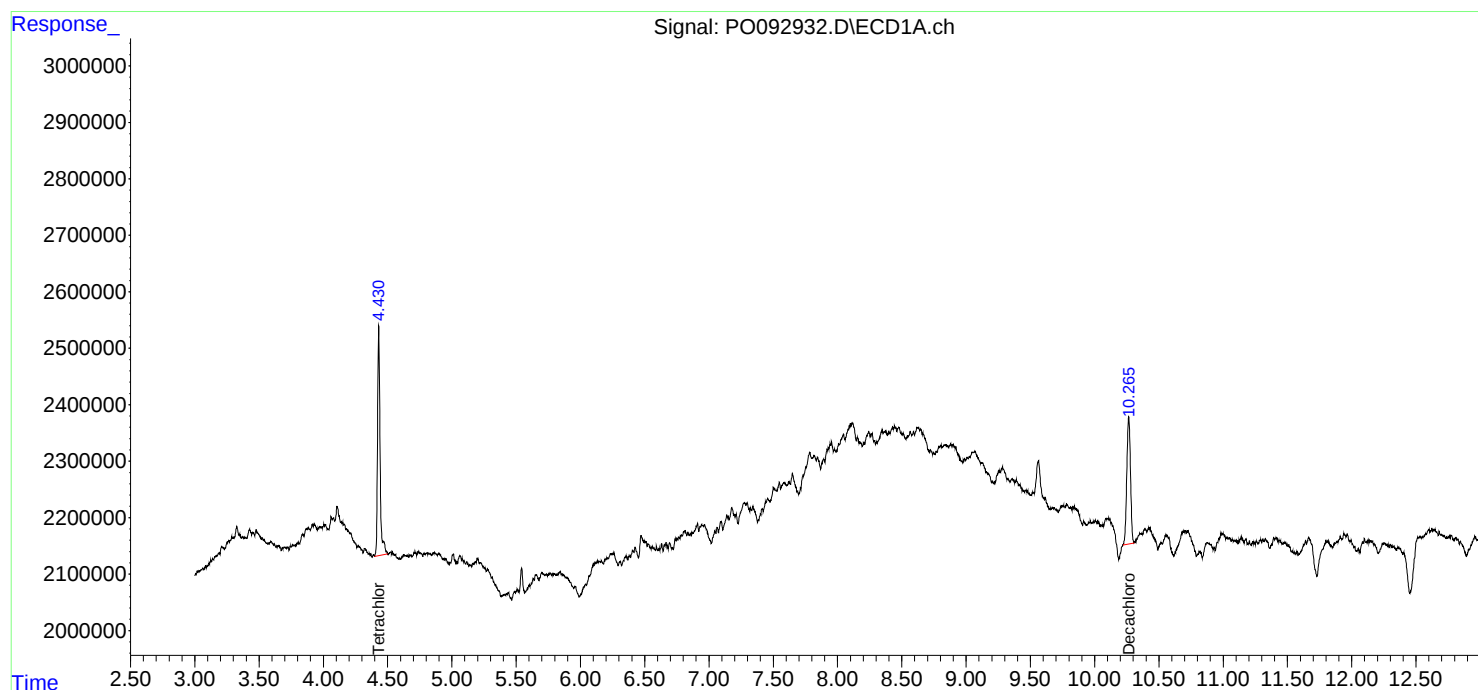

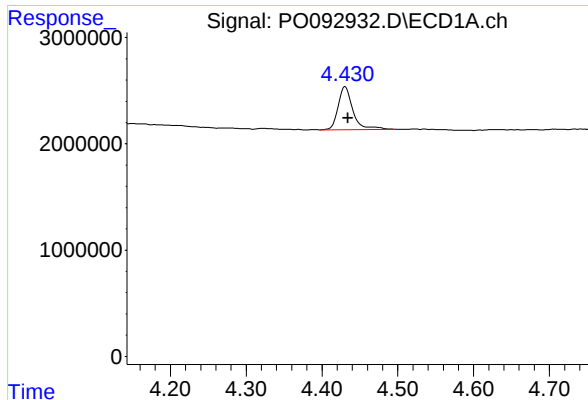


#1 Tetrachloro-m-xylene

R.T.: 4.430 min
Delta R.T.: -0.004 min
Response: 5489540
Conc: 1.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF461Z-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

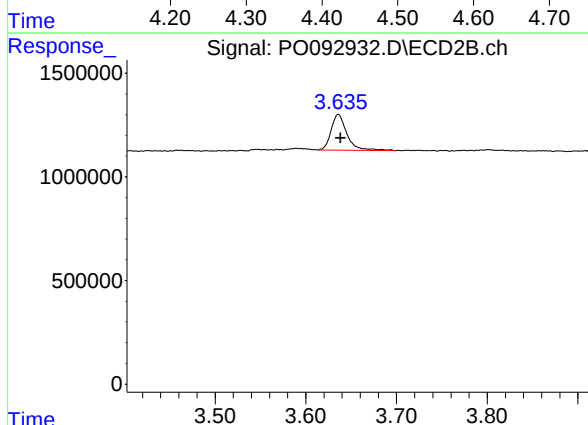


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.003 min
Response: 2076988
Conc: 1.63 ng/ml

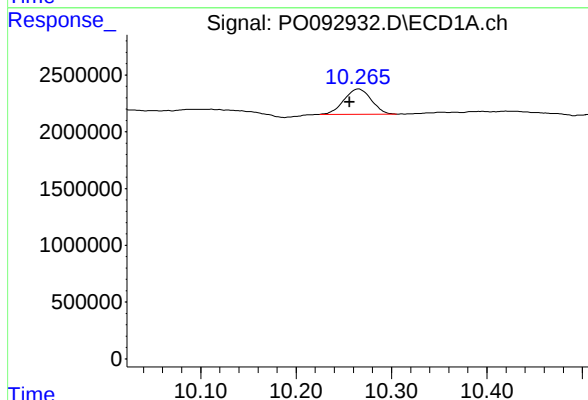

#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: 0.009 min
Response: 4498885
Conc: 2.34 ng/ml

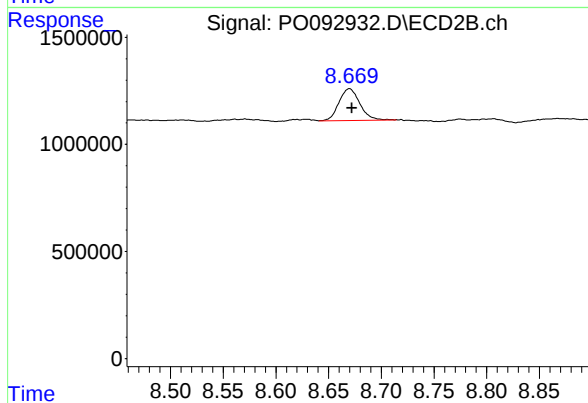

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 2043628
Conc: 1.75 ng/ml