

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030323\
 Data File : P0092933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 12:43
 Operator : YP/AJ
 Sample : 01747-05 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC226596-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 16:48:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.431	3.636	5629720	2141056	1.875	1.680
2) SA Decachlor...	10.265	8.670	4691879	2038654	2.439m	1.749m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030323\
Data File : PO092933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 12:43
Operator : YP/AJ
Sample : 01747-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC226596-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 16:48:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

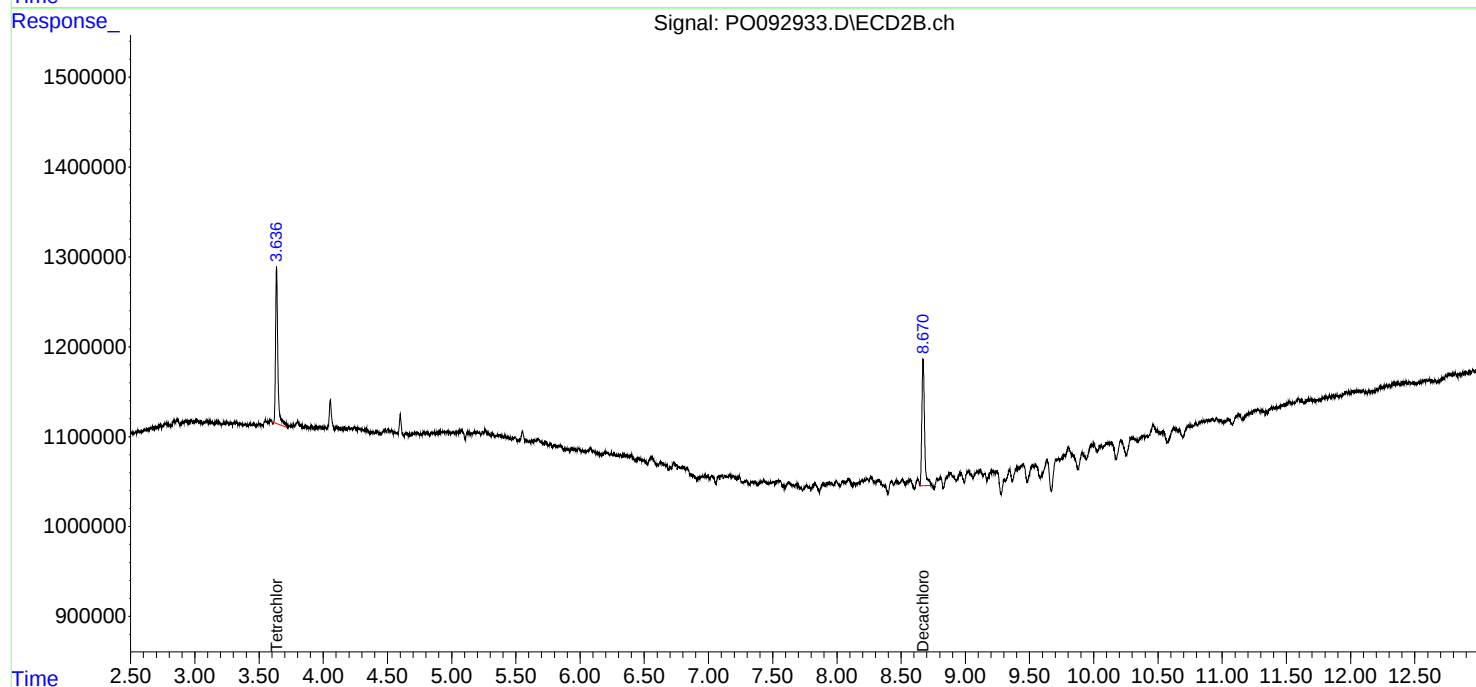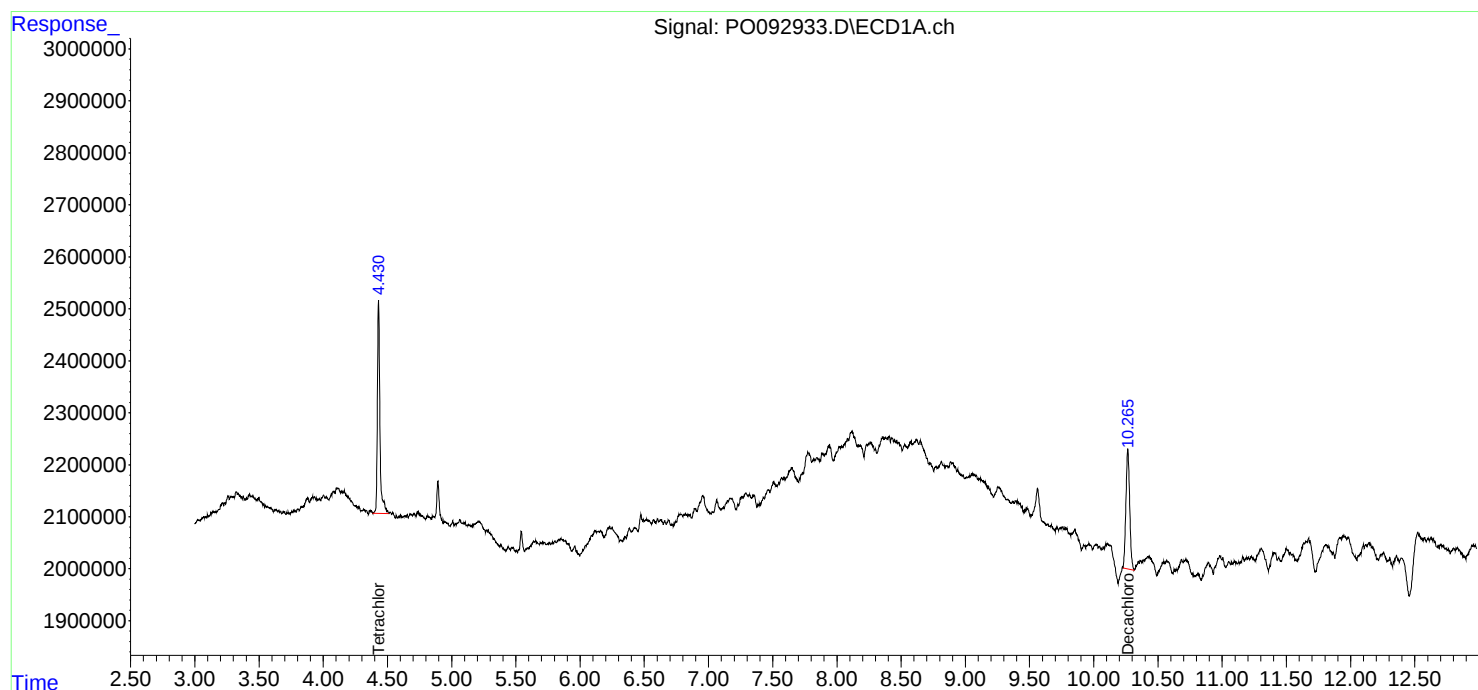

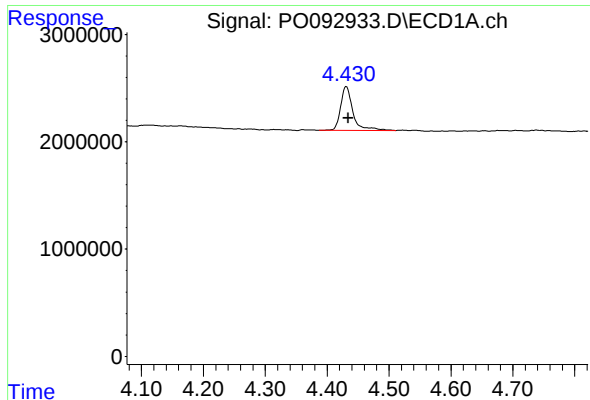


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 5629720
Conc: 1.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226596-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

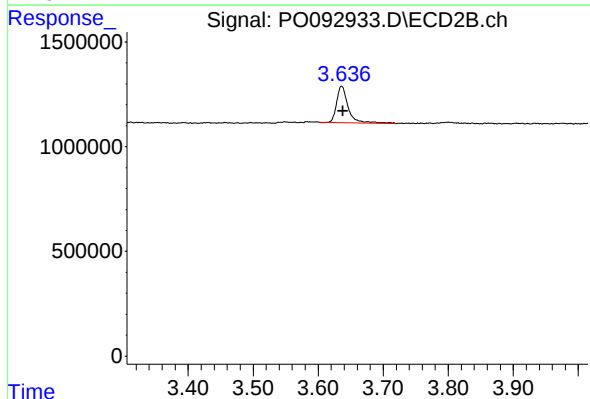


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 2141056
Conc: 1.68 ng/ml

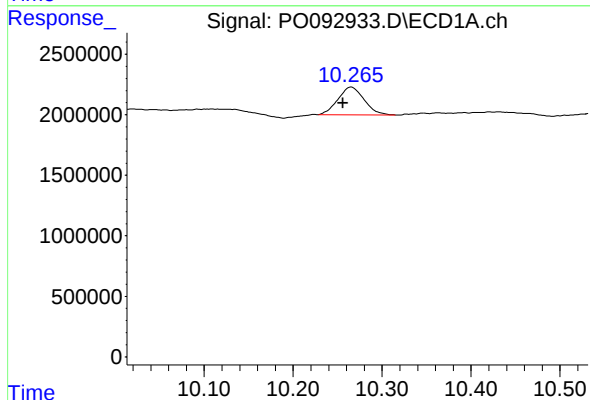

#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: 0.008 min
Response: 4691879
Conc: 2.44 ng/ml m

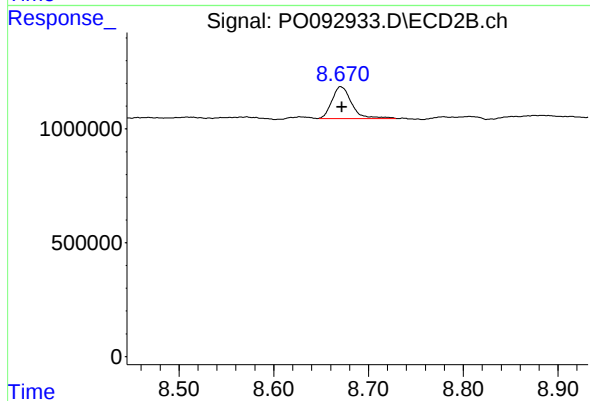

#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 2038654
Conc: 1.75 ng/ml m