

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030325\
 Data File : P0109637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2025 16:00
 Operator : YP/AJ
 Sample : Q1470-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 12925-DRIP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 16:13:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.696	3.694	174.9E6	100.0E6	18.482	19.113
2) SA Decachlor...	8.751	8.701	122.7E6	48553494	14.266	15.248

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030325\
Data File : PO109637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2025 16:00
Operator : YP/AJ
Sample : Q1470-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
12925-DRIP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 16:13:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

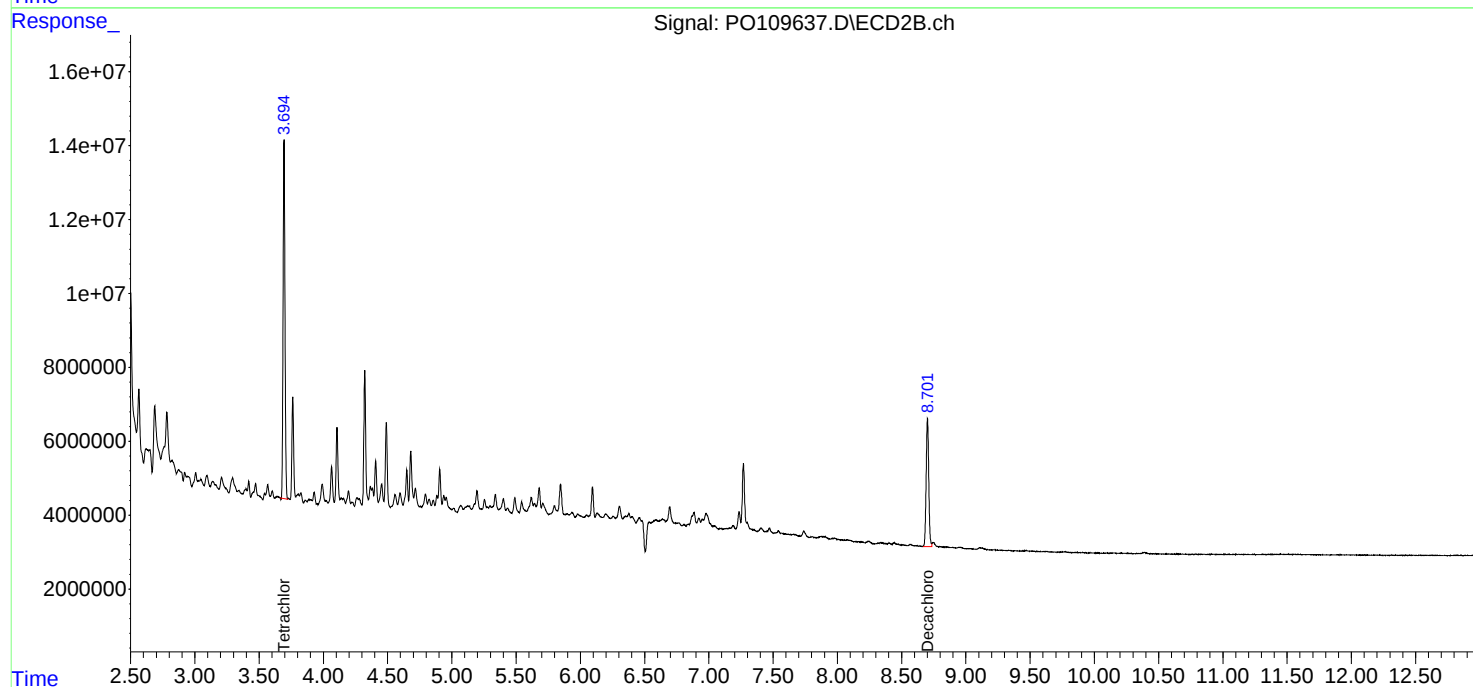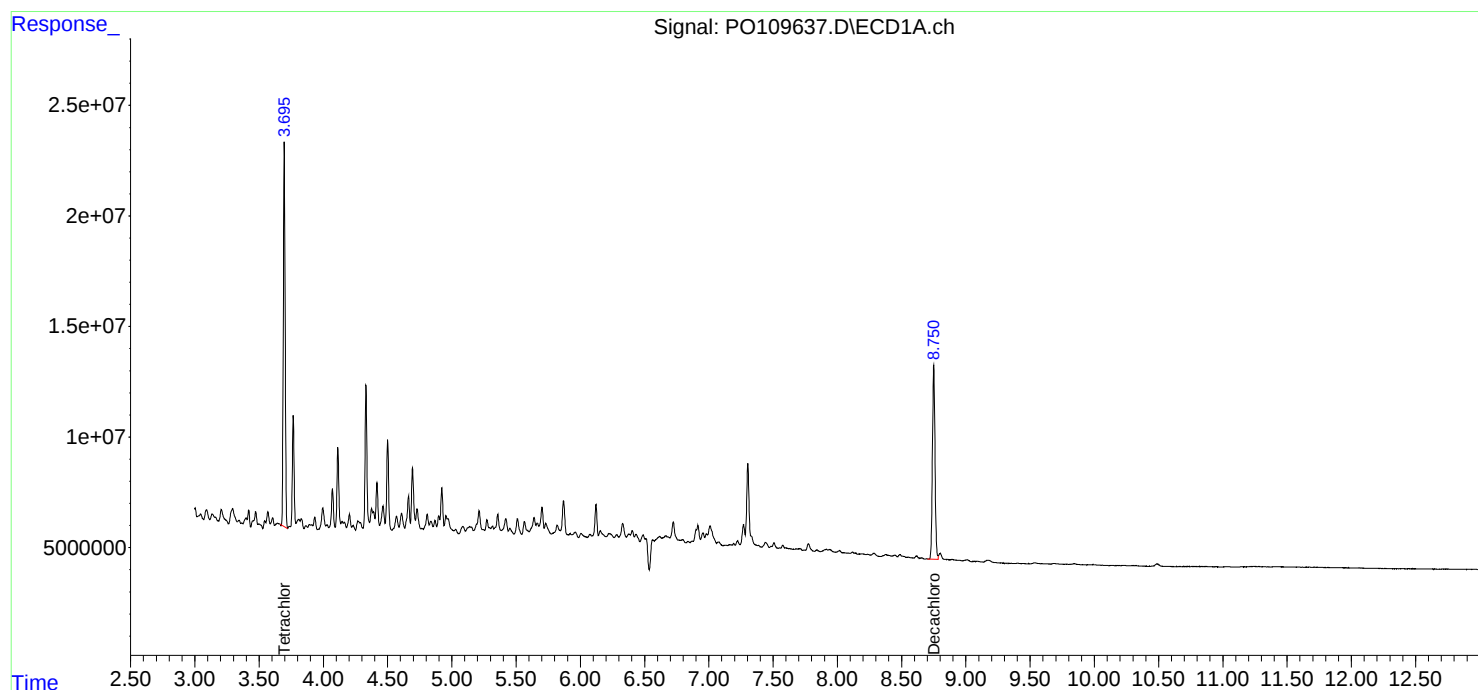


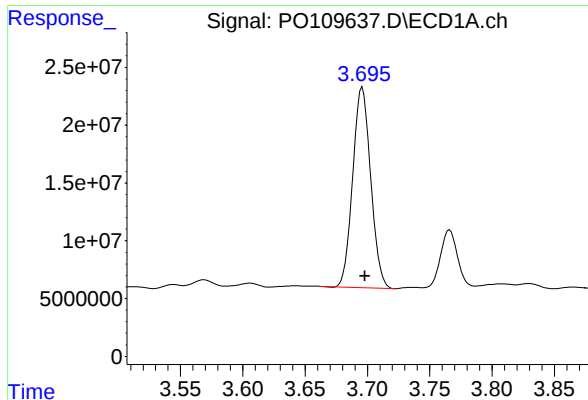

#1 Tetrachloro-m-xylene


R.T.: 3.696 min
Delta R.T.: -0.002 min
Response: 174931999
Conc: 18.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
12925-DRIP

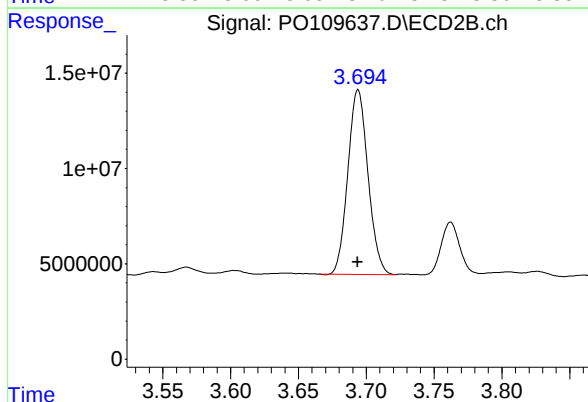


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 100042605
Conc: 19.11 ng/ml

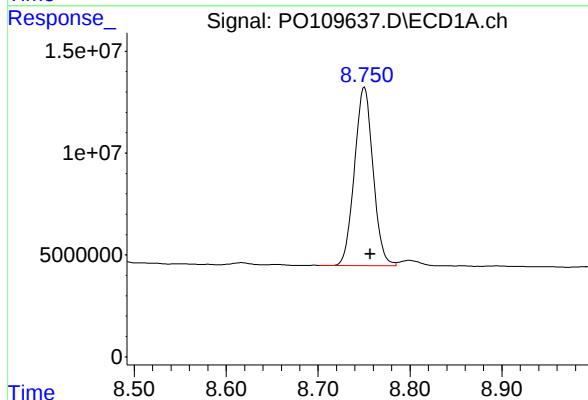

#2 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.006 min
Response: 122715682
Conc: 14.27 ng/ml

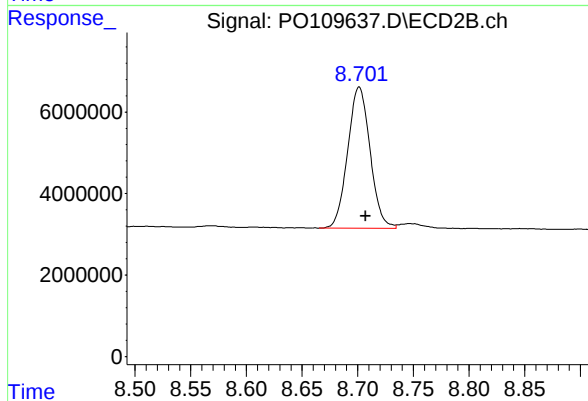

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.006 min
Response: 48553494
Conc: 15.25 ng/ml