

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030325\
 Data File : P0109641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2025 17:14
 Operator : YP/AJ
 Sample : Q1467-02 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 50607

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2025
 Supervised By :Ankita Jodhani 03/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 07:27:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.694	3.692	15685298	8824326	1.657m	1.686m
2) SA Decachlor...	8.750	8.701	5343165	2233717	0.621m	0.701m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030325\
Data File : PO109641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2025 17:14
Operator : YP/AJ
Sample : Q1467-02 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
50607


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2025
Supervised By :Ankita Jodhani 03/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 07:27:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

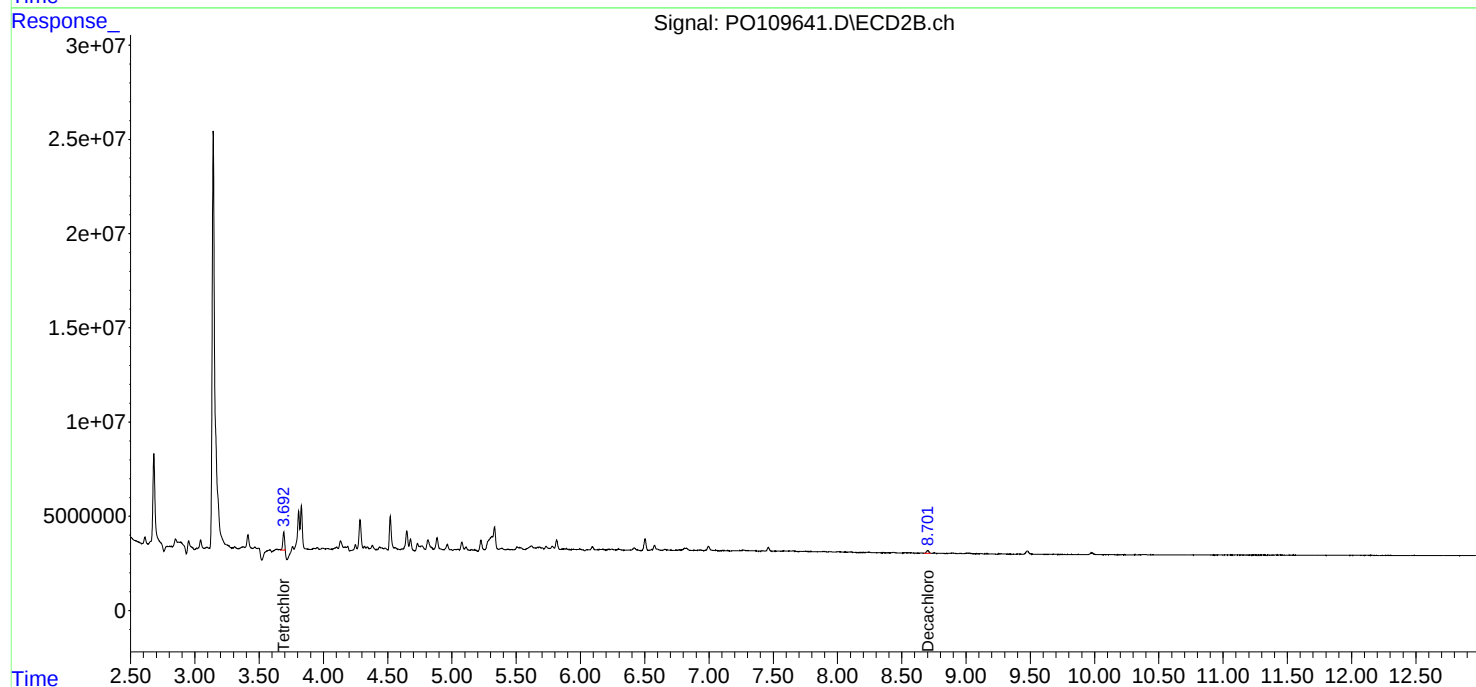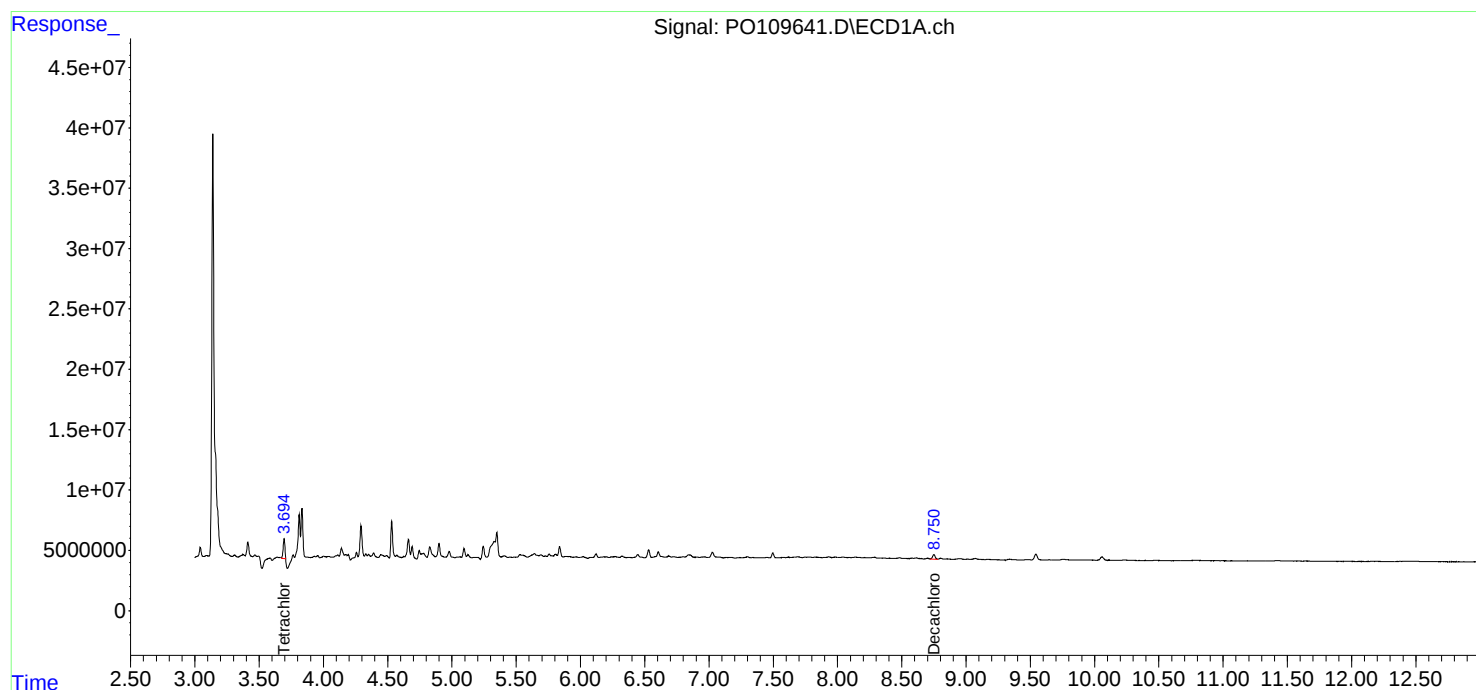

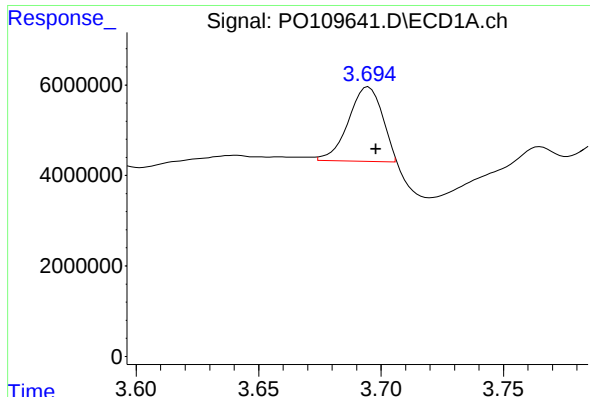


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: -0.004 min
Response: 15685298
Conc: 1.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
50607


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2025
Supervised By :Ankita Jodhani 03/04/2025

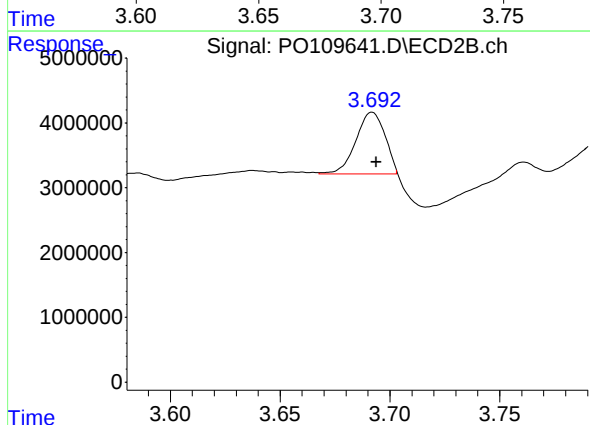


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: -0.002 min
Response: 8824326
Conc: 1.69 ng/ml m

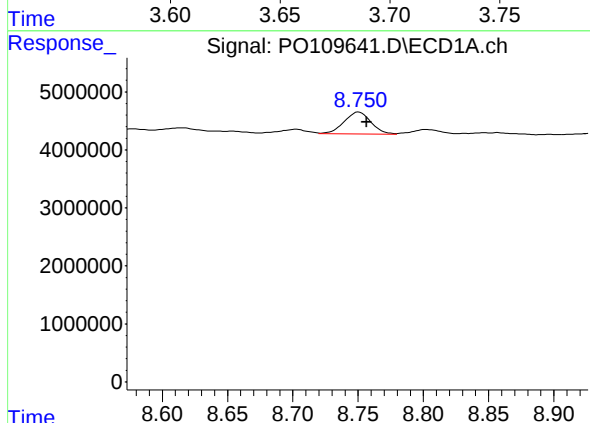

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.007 min
Response: 5343165
Conc: 0.62 ng/ml m

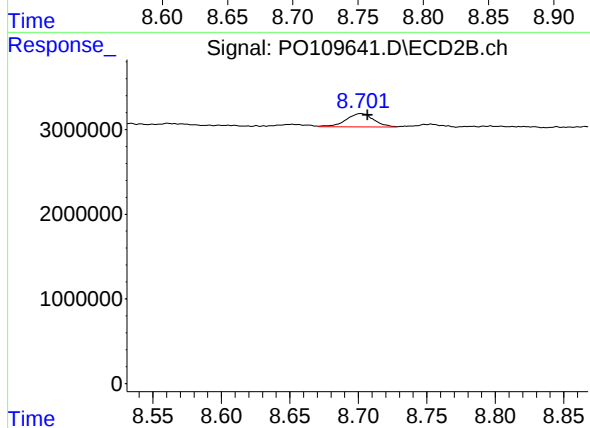

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.005 min
Response: 2233717
Conc: 0.70 ng/ml m