

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030421\
 Data File : P0075846.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2021 16:18
 Operator : AJ/MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 08:10:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds							
2) SA Decachlor...	10.948	0.000	4414	0	0.134	N.D.	#
Target Compounds							
29) L6 AR-1254-4	8.073	0.000	8612	0	3.939	N.D.	#
30) L6 AR-1254-5	8.508	0.000	17009	0	7.473	N.D.	#
34) L7 AR-1260-4	8.831f	0.000	58822	0	27.059	N.D.	#
39) L8 AR-1262-4	9.551	0.000	3695	0	1.617	N.D.	#
40) L8 AR-1262-5	10.192	0.000	4184	0	2.762	N.D.	#
42) L9 AR-1268-2	9.551	0.000	3695	0	0.791	N.D.	#
43) L9 AR-1268-3	9.771	0.000	4092	0	0.982	N.D.	#
44) L9 AR-1268-4	10.192	0.000	4184	0	2.669	N.D.	#
45) L9 AR-1268-5	10.610	0.000	3643	0	0.288	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030421\
Data File : P0075846.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2021 16:18
Operator : AJ/MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 08:10:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

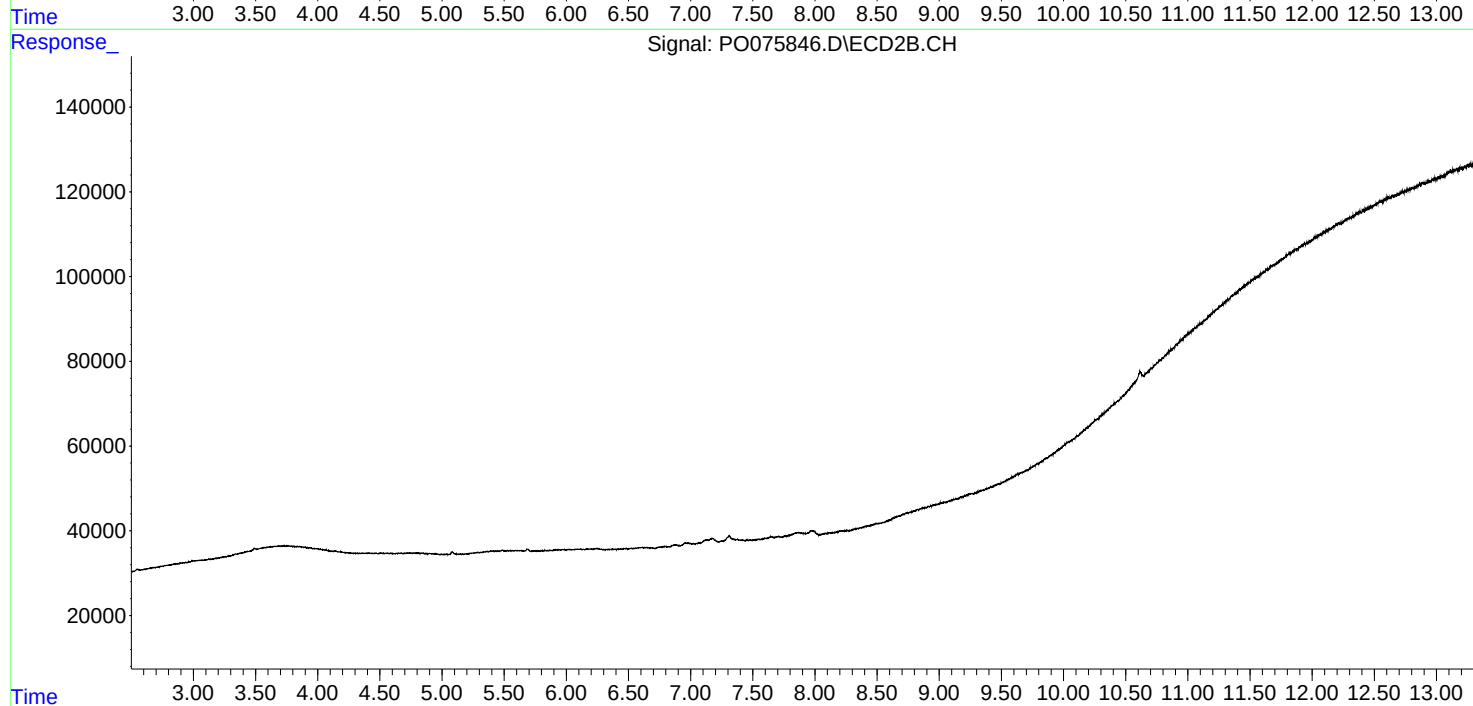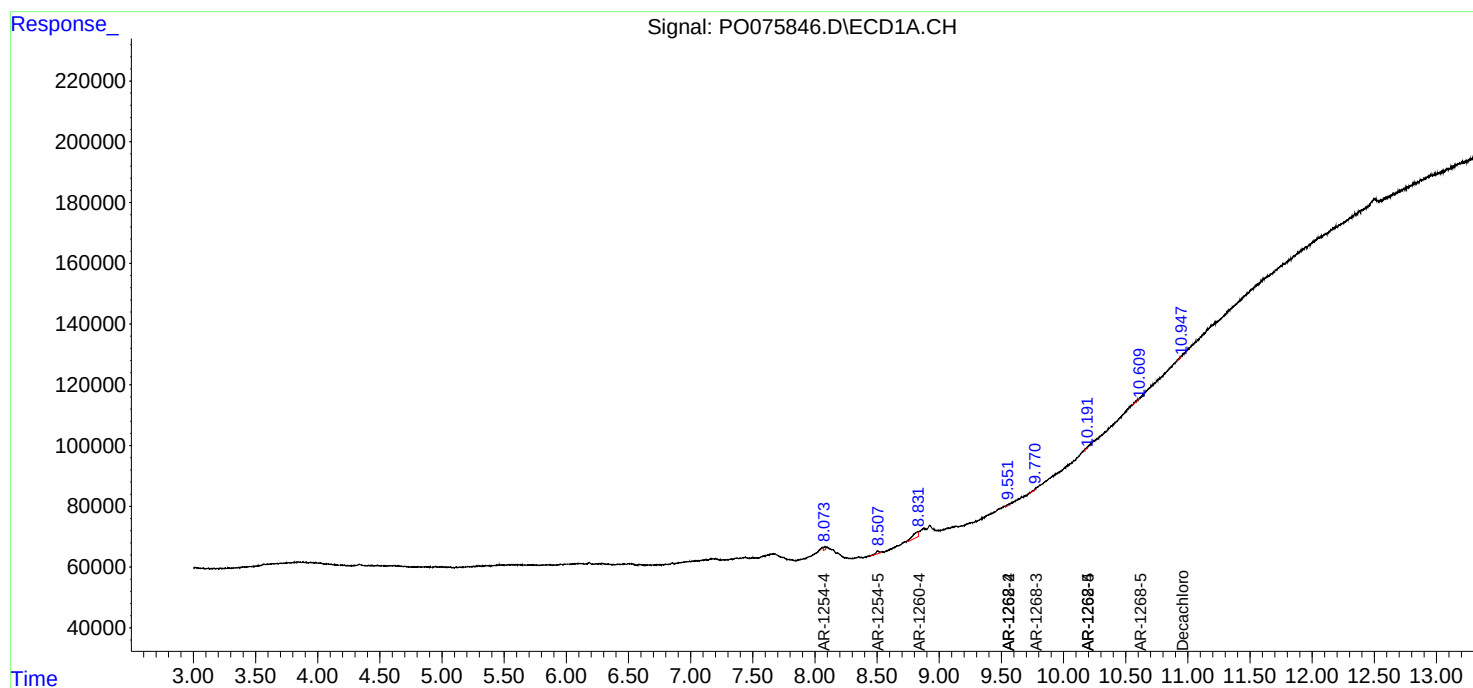


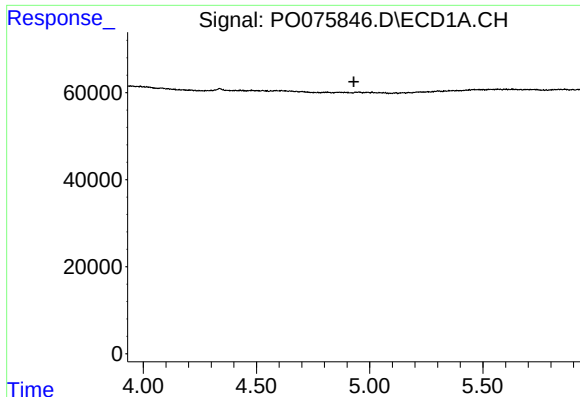

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.930 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

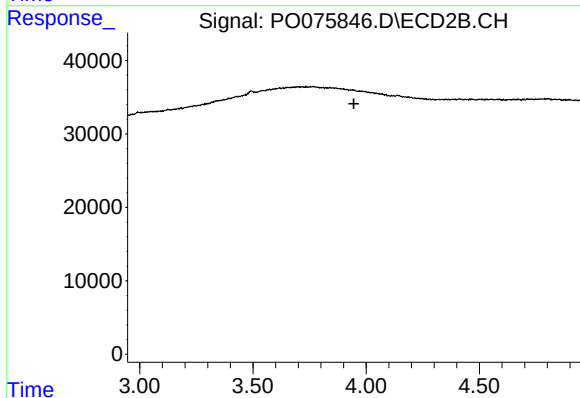


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.946 min
Response: 0
Conc: N.D.

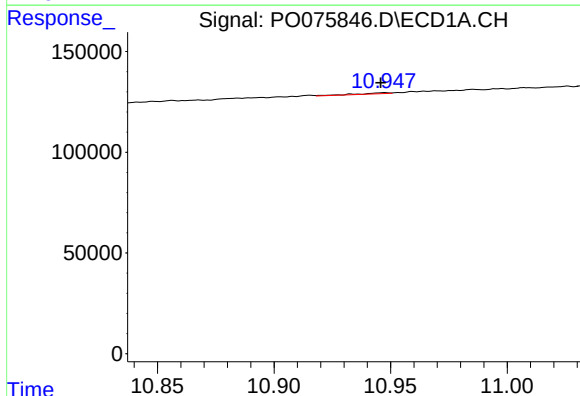


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.002 min
Response: 4414
Conc: 0.13 ng/ml

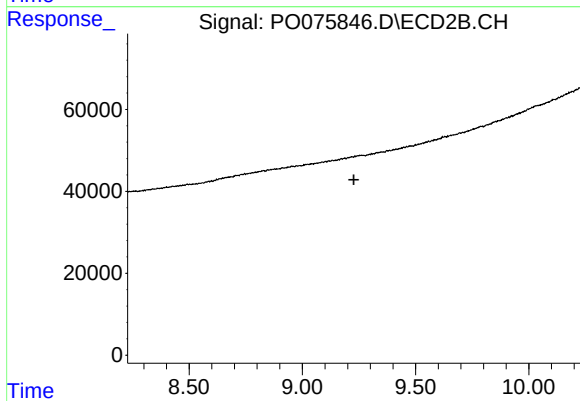

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

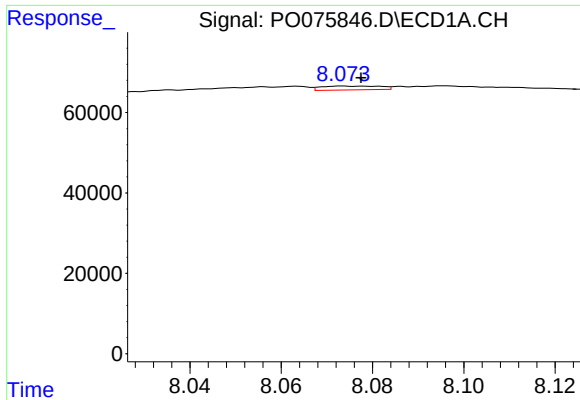

#29 AR-1254-4


R.T.: 8.073 min
Delta R.T.: -0.004 min
Response: 8612
Conc: 3.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

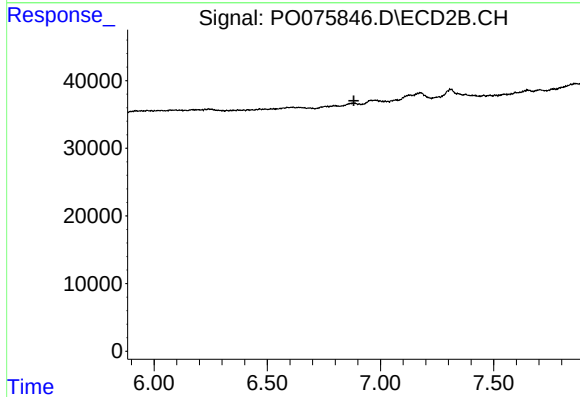


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.883 min
Response: 0
Conc: N.D.

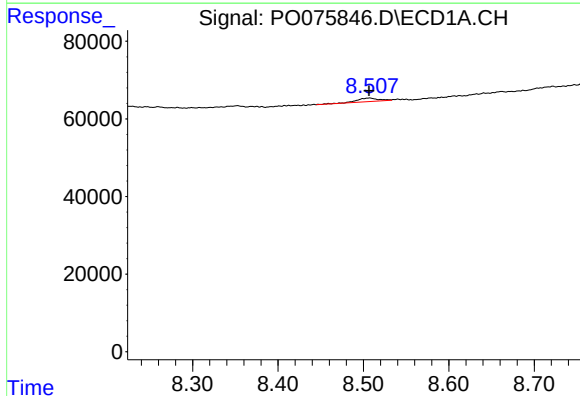


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: 0.001 min
Response: 17009
Conc: 7.47 ng/ml

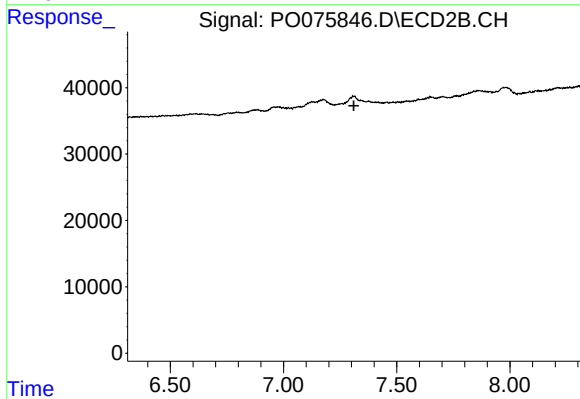

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.311 min
Response: 0
Conc: N.D.

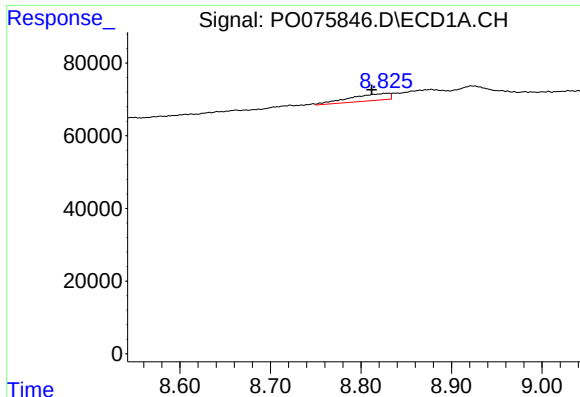

#34 AR-1260-4


R.T.: 8.831 min
Delta R.T.: 0.019 min
Response: 58822
Conc: 27.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

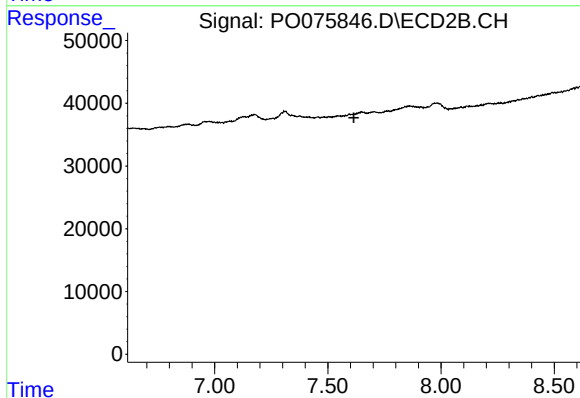


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

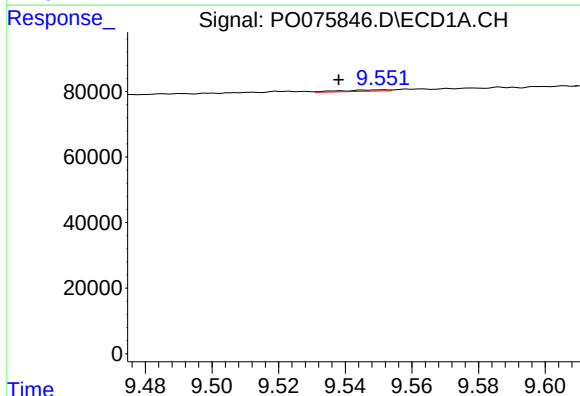


#39 AR-1262-4

R.T.: 9.551 min
Delta R.T.: 0.013 min
Response: 3695
Conc: 1.62 ng/ml

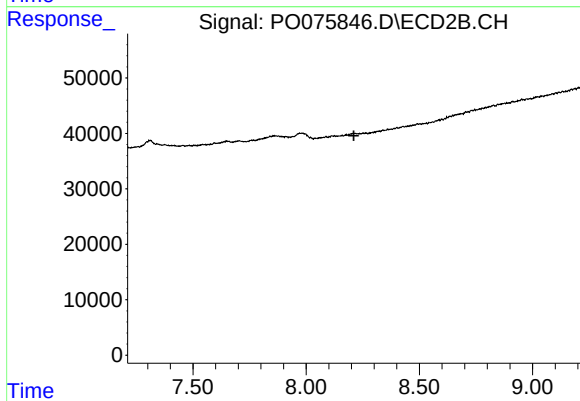

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.211 min
Response: 0
Conc: N.D.

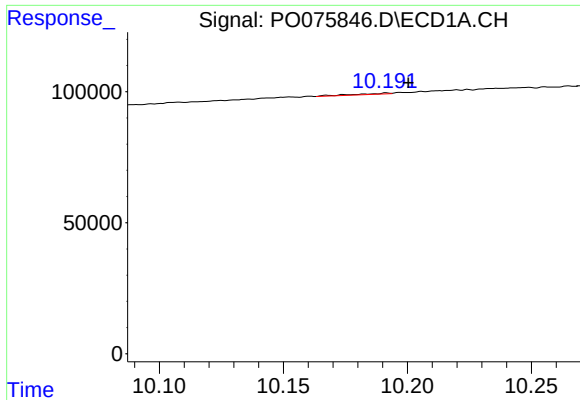

#40 AR-1262-5


R.T.: 10.192 min
Delta R.T.: -0.009 min
Response: 4184
Conc: 2.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

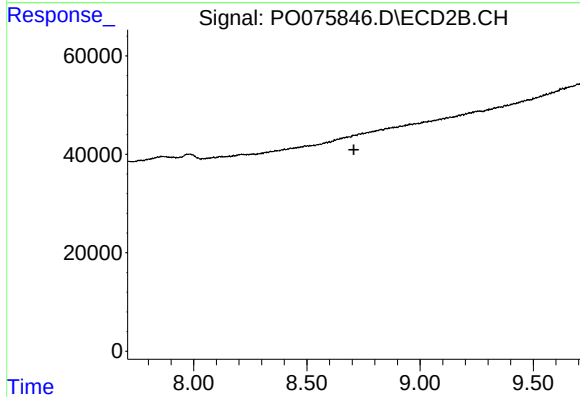


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.708 min
Response: 0
Conc: N.D.

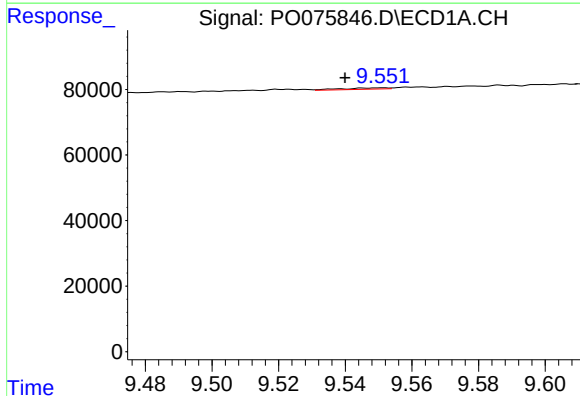


#42 AR-1268-2

R.T.: 9.551 min
Delta R.T.: 0.011 min
Response: 3695
Conc: 0.79 ng/ml

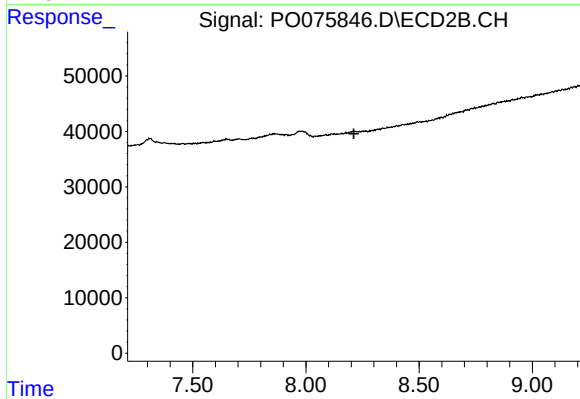

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.211 min
Response: 0
Conc: N.D.

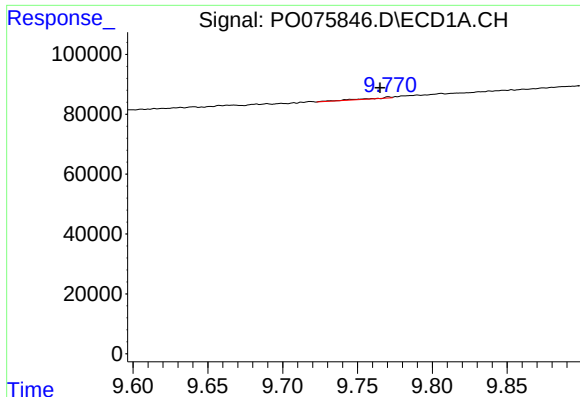

#43 AR-1268-3


R.T.: 9.771 min
Delta R.T.: 0.006 min
Response: 4092
Conc: 0.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

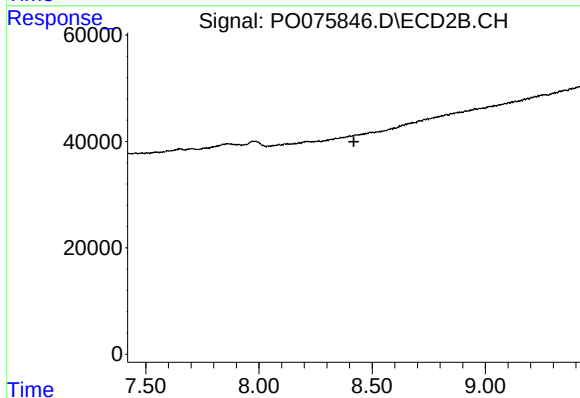


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.419 min
Response: 0
Conc: N.D.

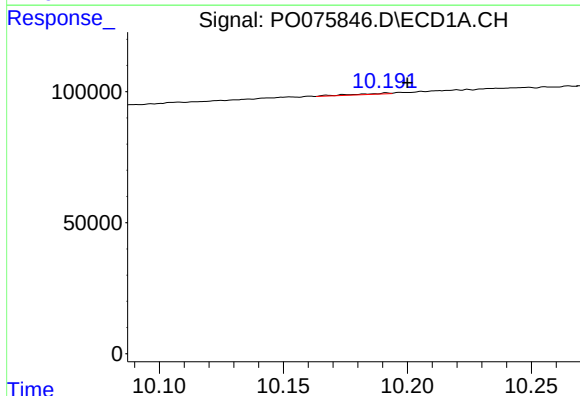


#44 AR-1268-4

R.T.: 10.192 min
Delta R.T.: -0.008 min
Response: 4184
Conc: 2.67 ng/ml

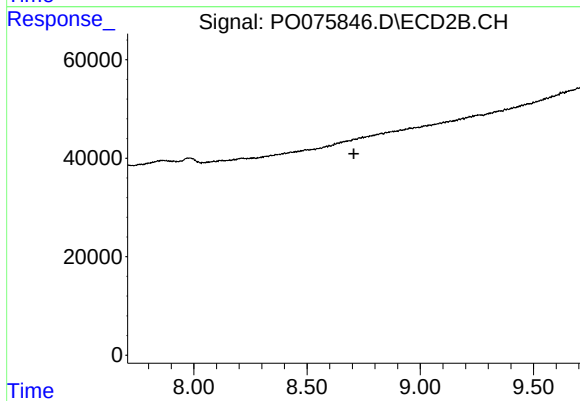

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.707 min
Response: 0
Conc: N.D.

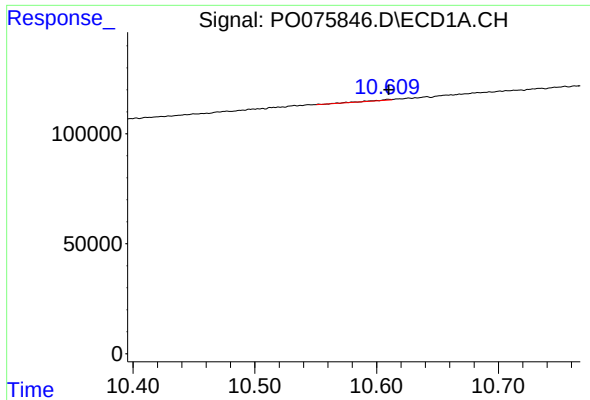

#45 AR-1268-5

R.T.: 10.610 min
Delta R.T.: 0.000 min
Response: 3643
Conc: 0.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

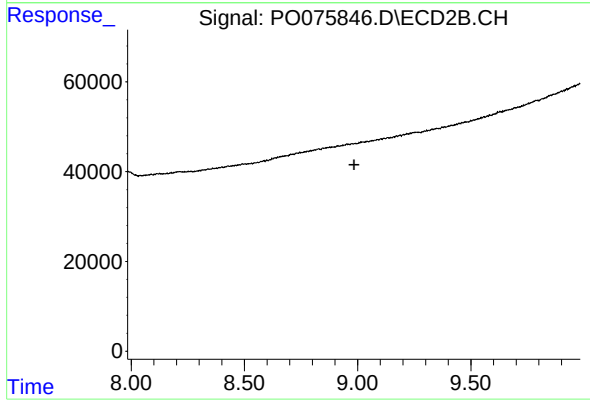

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.984 min
Response: 0
Conc: N.D.