

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030421\
 Data File : P0075864.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2021 21:27
 Operator : AJ/MA
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Ankita
 3/5/2021 1:35:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 07:09:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 07:07:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	3.944	304512	240263	4.924	5.310
2) SA Decachlor...	10.945	9.225	170640	209167	5.113	5.696
Target Compounds						
21) L5 AR-1248-1	6.253	5.195	58527	50393	54.265	54.642m
22) L5 AR-1248-2	6.548	5.457	84500	82388	54.208m	59.110
23) L5 AR-1248-3	6.767	5.501	90939	87880	50.292	61.724
24) L5 AR-1248-4	7.197	5.685	102261	95795	53.830	57.692
25) L5 AR-1248-5	7.237	6.107	96033	93814	50.019	57.554

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030421\
Data File : PO075864.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2021 21:27
Operator : AJ/MA
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 07:09:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 07:07:25 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

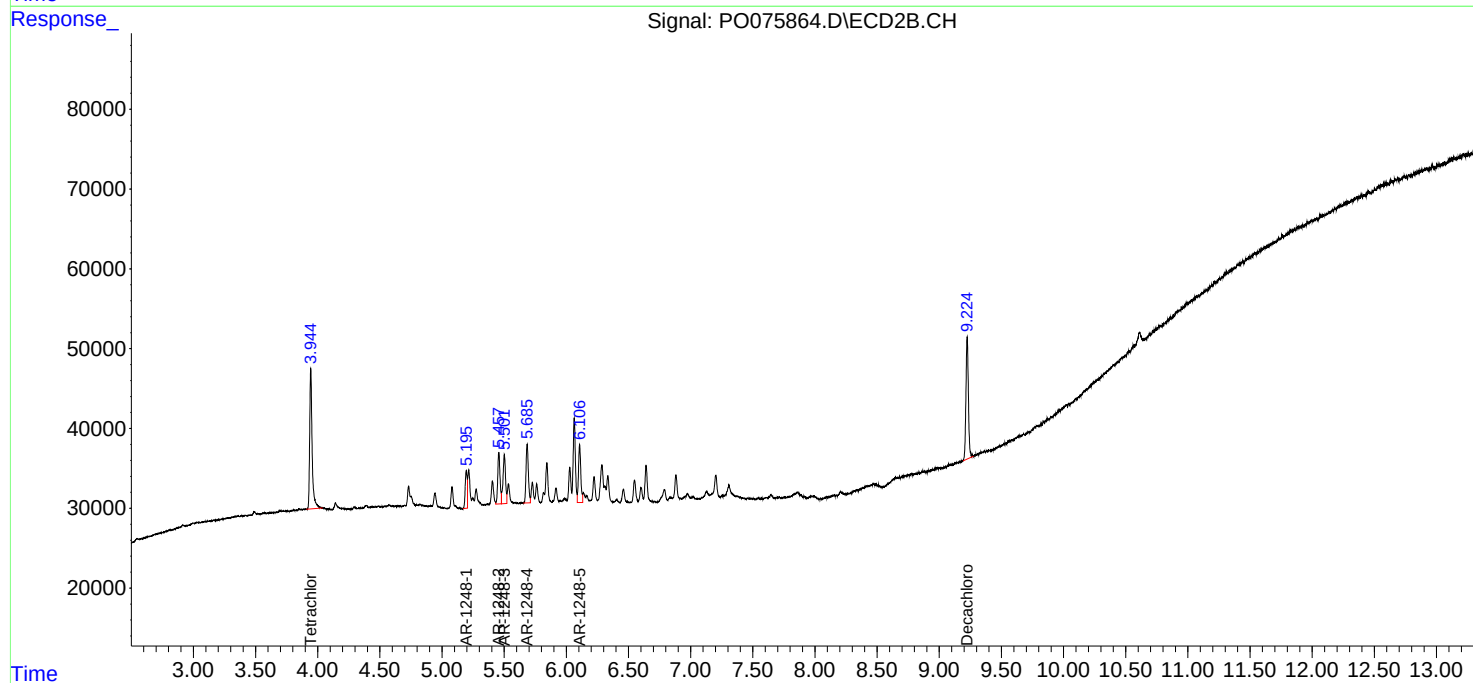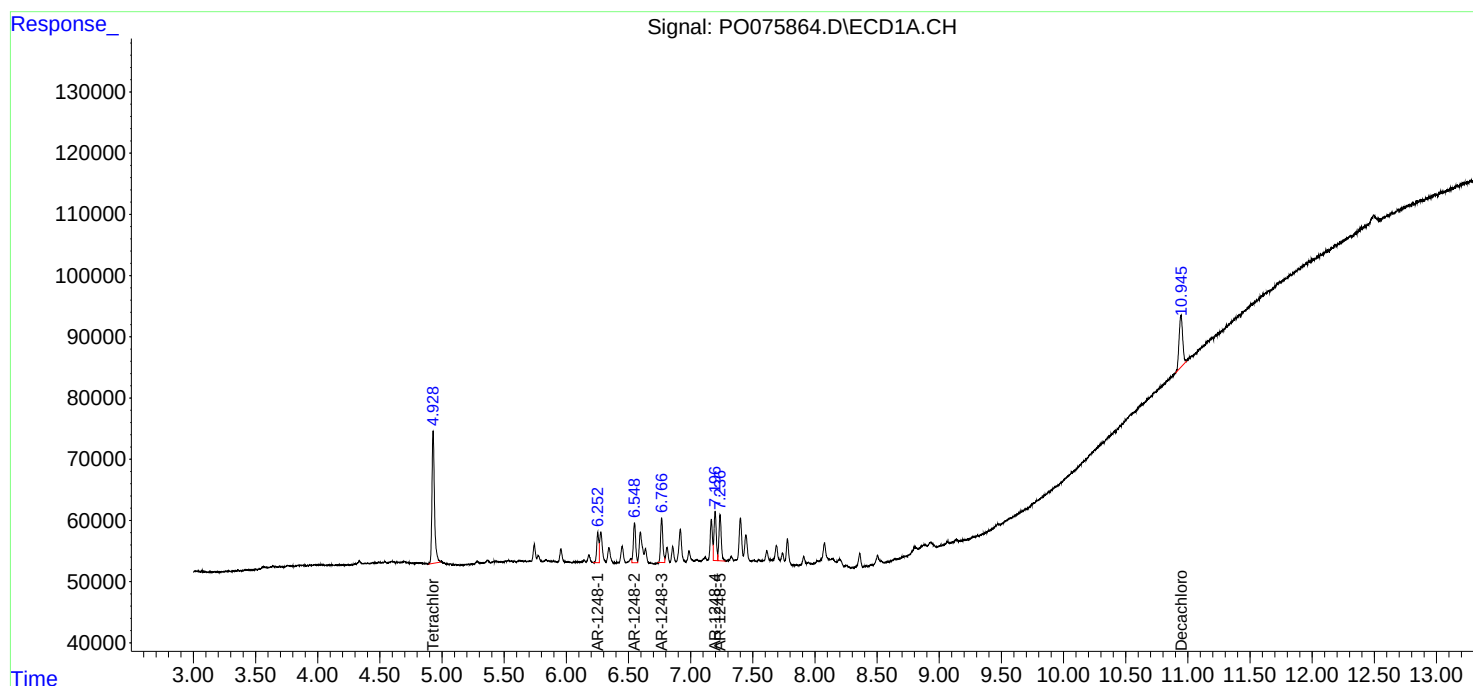

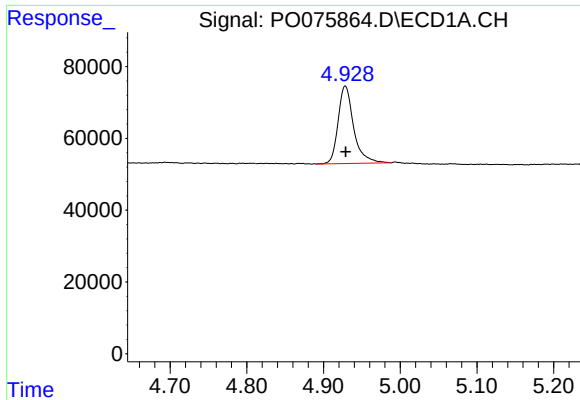


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 304512
Conc: 4.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:25 PM

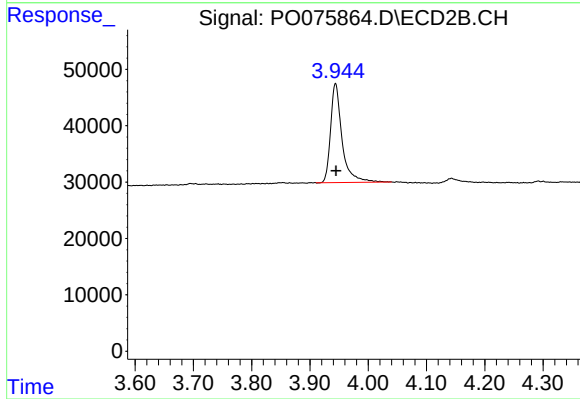


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 240263
Conc: 5.31 ng/ml

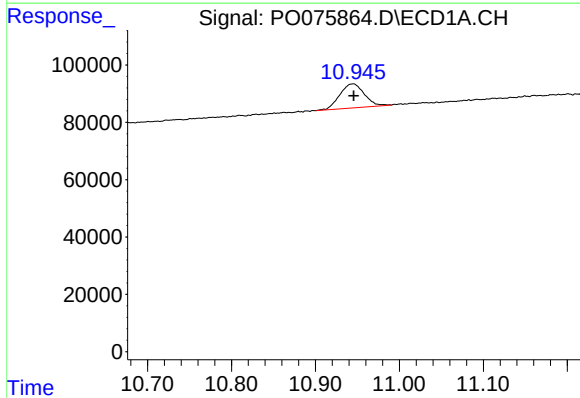


#2 Decachlorobiphenyl

R.T.: 10.945 min
Delta R.T.: -0.001 min
Response: 170640
Conc: 5.11 ng/ml

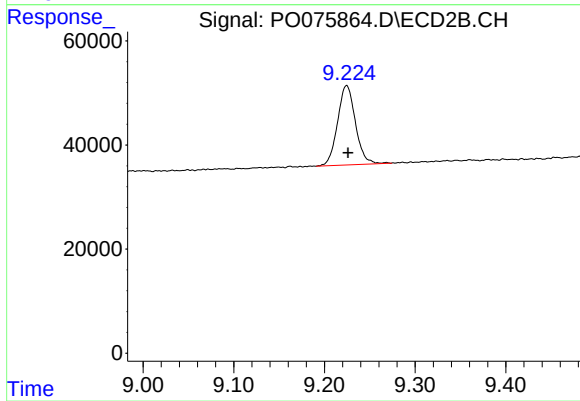

#2 Decachlorobiphenyl

R.T.: 9.225 min
Delta R.T.: -0.001 min
Response: 209167
Conc: 5.70 ng/ml

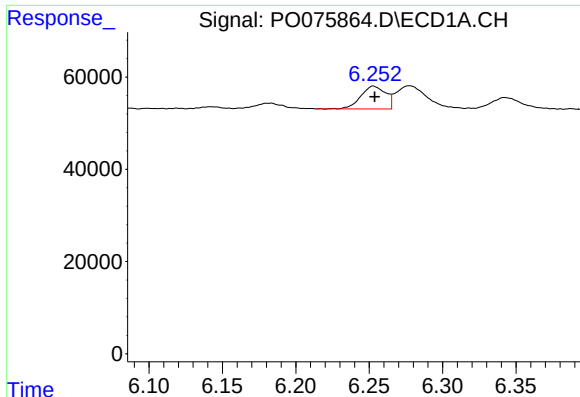


#21 AR-1248-1

R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 58527
Conc: 54.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:25 PM

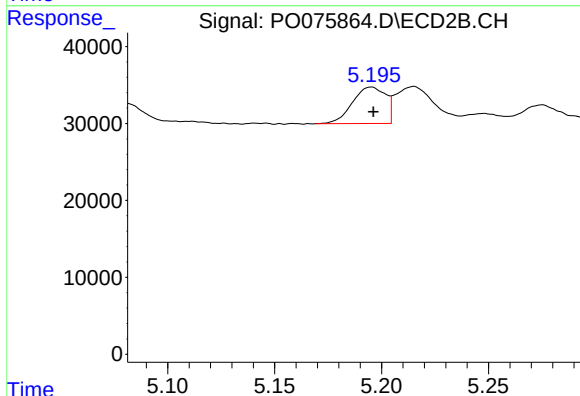


#21 AR-1248-1

R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 50393
Conc: 54.64 ng/ml m

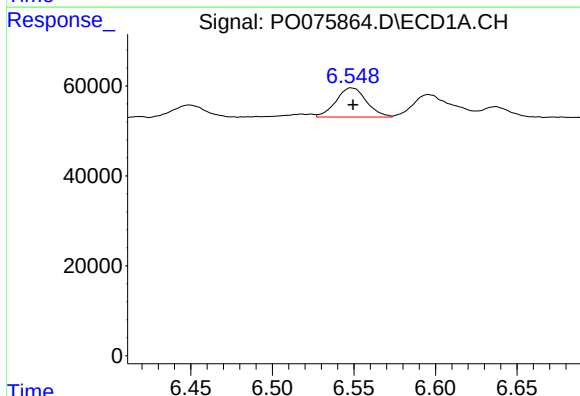


#22 AR-1248-2

R.T.: 6.548 min
Delta R.T.: -0.002 min
Response: 84500
Conc: 54.21 ng/ml m

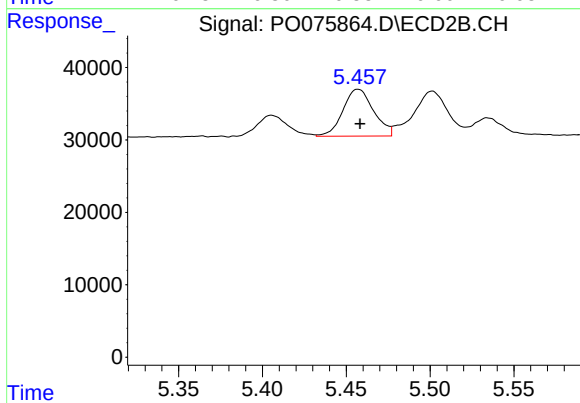

#22 AR-1248-2

R.T.: 5.457 min
Delta R.T.: -0.001 min
Response: 82388
Conc: 59.11 ng/ml

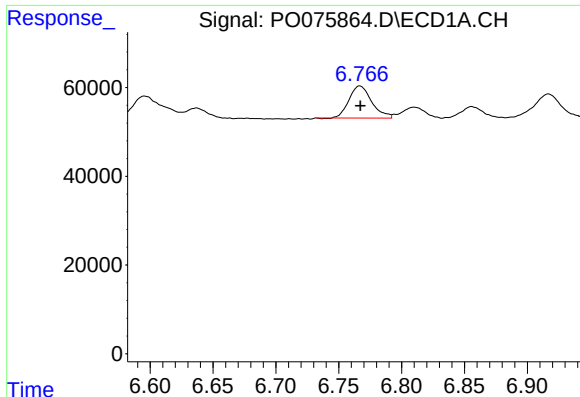


#23 AR-1248-3

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 90939
Conc: 50.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:25 PM

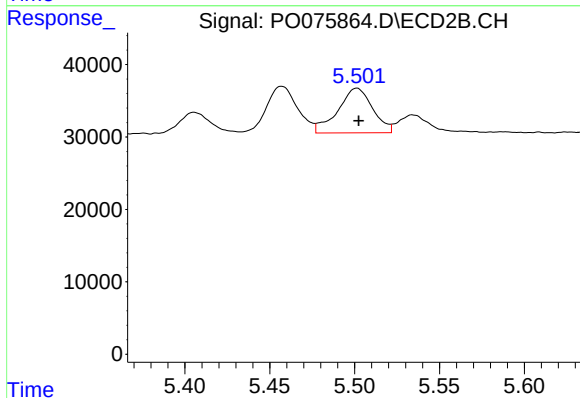


#23 AR-1248-3

R.T.: 5.501 min
Delta R.T.: -0.001 min
Response: 87880
Conc: 61.72 ng/ml

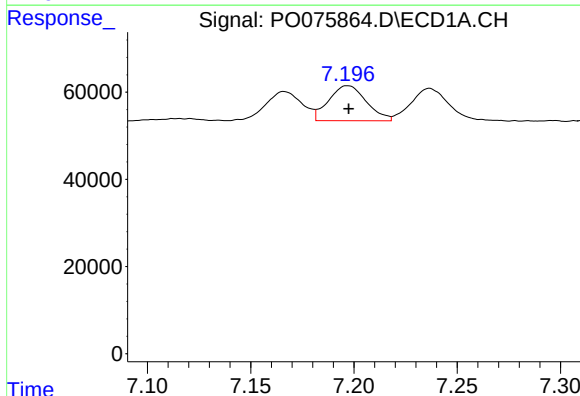


#24 AR-1248-4

R.T.: 7.197 min
Delta R.T.: 0.000 min
Response: 102261
Conc: 53.83 ng/ml

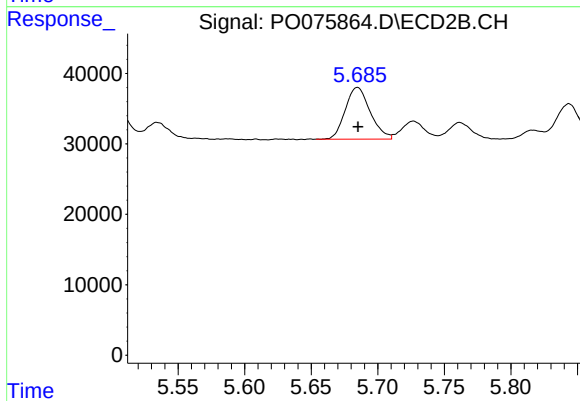

#24 AR-1248-4

R.T.: 5.685 min
Delta R.T.: 0.000 min
Response: 95795
Conc: 57.69 ng/ml

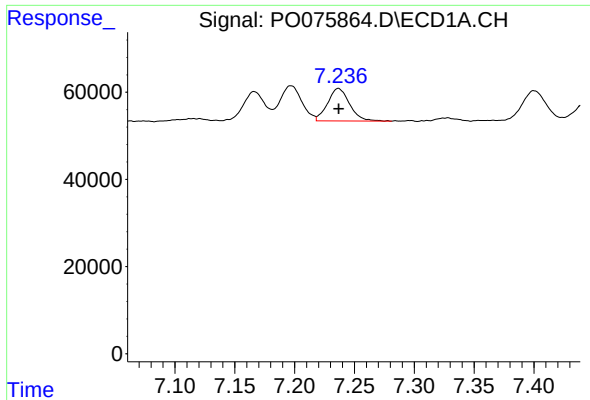


#25 AR-1248-5

R.T.: 7.237 min
Delta R.T.: 0.000 min
Response: 96033
Conc: 50.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:25 PM

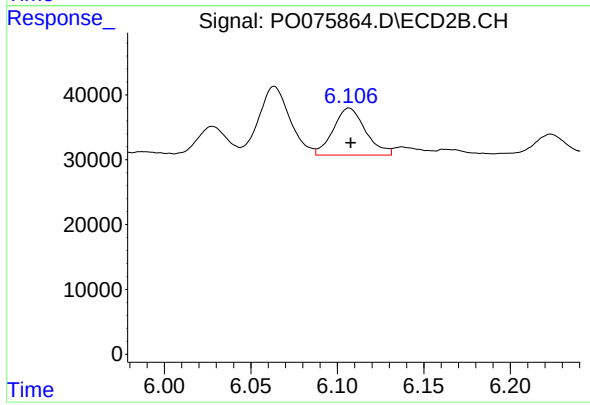

#25 AR-1248-5

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 93814
Conc: 57.55 ng/ml