

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030421\
 Data File : P0075884.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 3:09
 Operator : AJ/MA
 Sample : AR1262ICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO030421AR1262

Manual Integrations
 APPROVED

Ankita
 3/5/2021 1:35:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 08:14:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	3.944	3303952	2436609	55.429	54.623
2) SA Decachlor...	10.941	9.225	1789356	1980445	54.468	54.466
Target Compounds						
36) L8 AR-1262-1	8.579	7.309	1433423	834867	503.512	485.048
37) L8 AR-1262-2	9.136	7.861	2296715	2762173	503.997	495.585
38) L8 AR-1262-3	9.445	8.147	1544357	1152662	510.732	496.722
39) L8 AR-1262-4	9.540	8.211	1170673	2045232	512.422m	486.577
40) L8 AR-1262-5	10.200	8.708	766231	933578	505.829	516.576

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030421\
Data File : PO075884.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 3:09
Operator : AJ/MA
Sample : AR1262ICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ICVPO030421AR1262


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 08:14:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

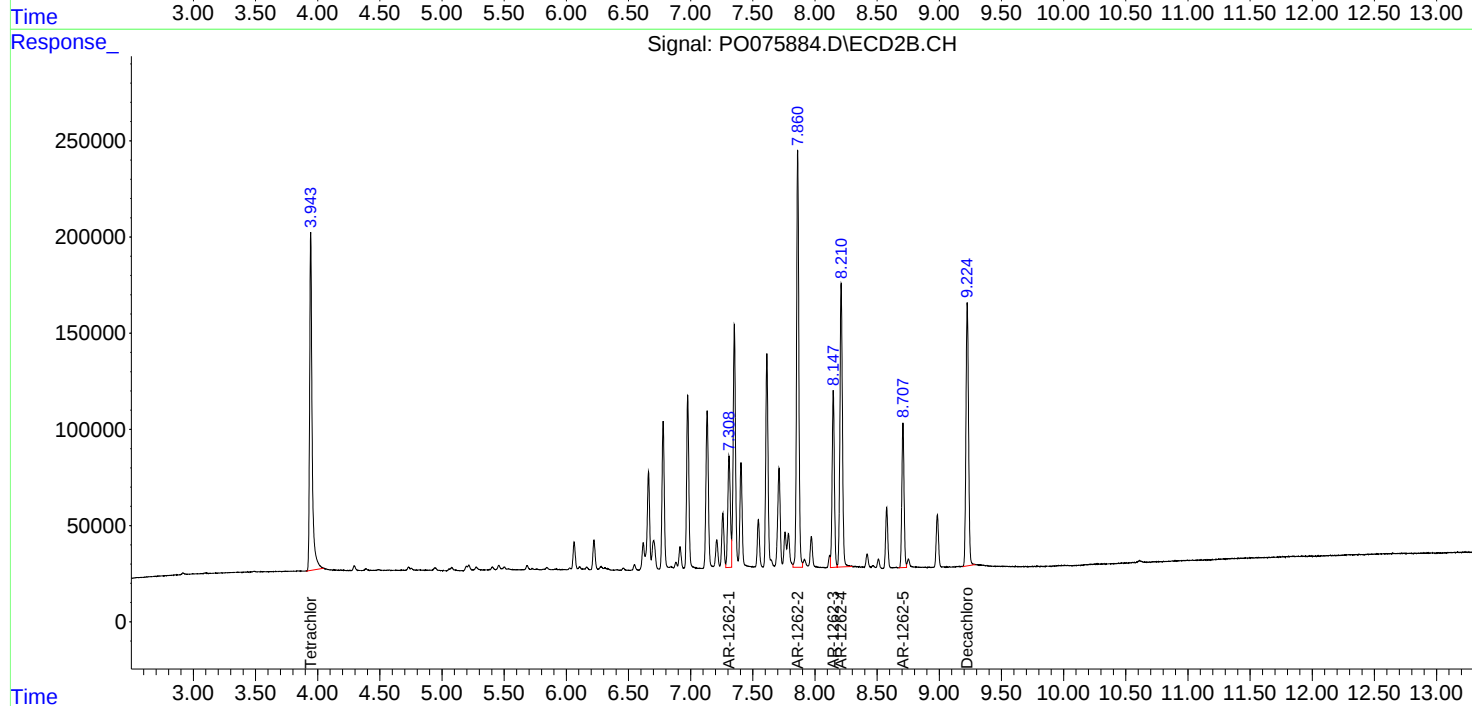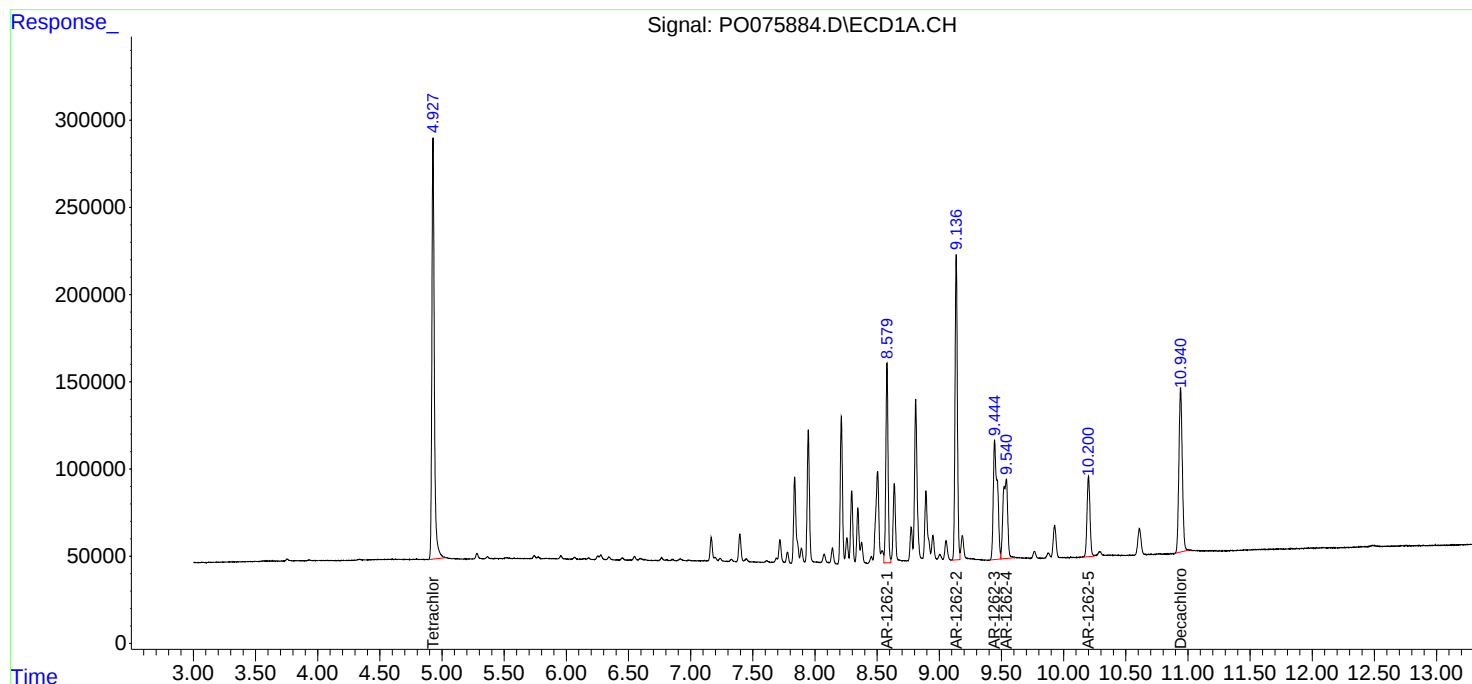

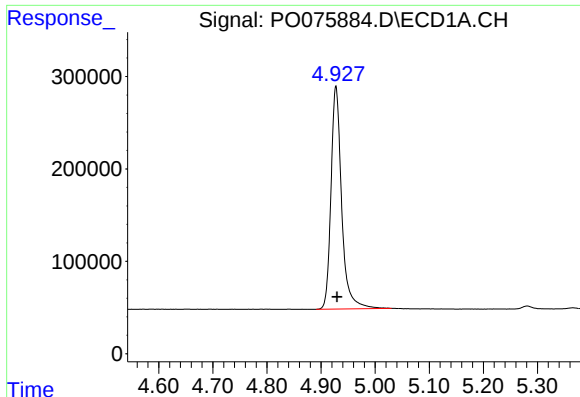


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 3303952
Conc: 55.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO030421AR1262


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:31 PM

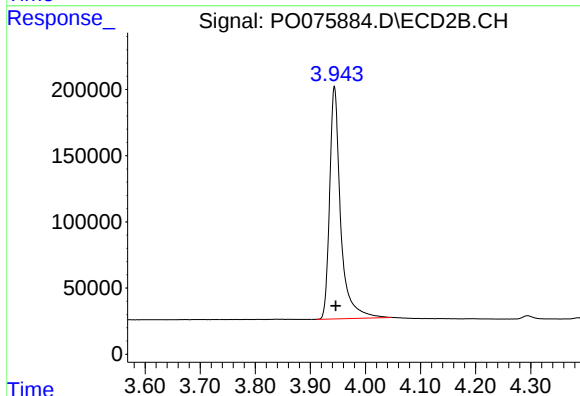


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.002 min
Response: 2436609
Conc: 54.62 ng/ml

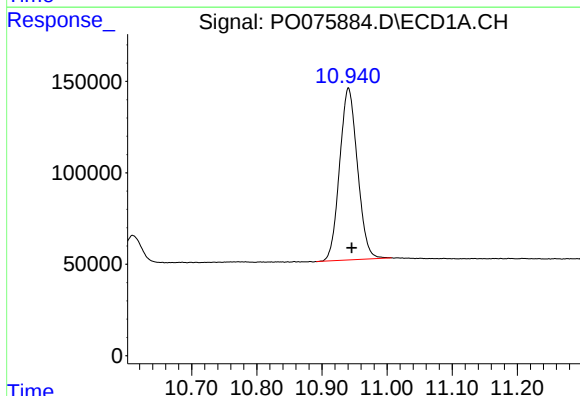


#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: -0.005 min
Response: 1789356
Conc: 54.47 ng/ml

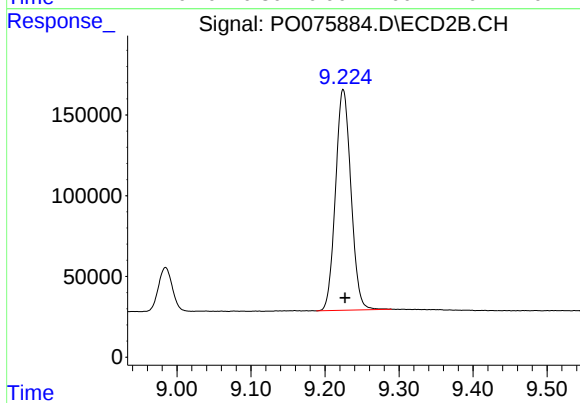

#2 Decachlorobiphenyl

R.T.: 9.225 min
Delta R.T.: -0.003 min
Response: 1980445
Conc: 54.47 ng/ml

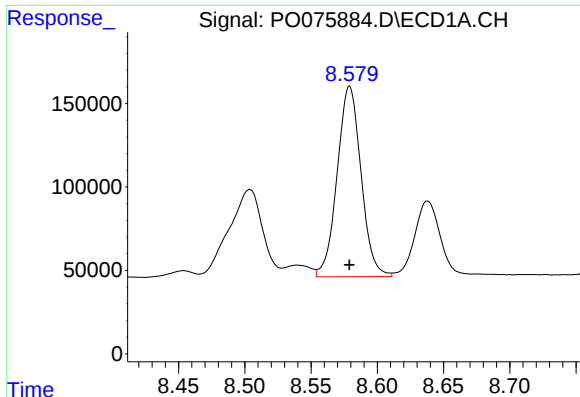


#36 AR-1262-1

R.T.: 8.579 min
Delta R.T.: 0.000 min
Response: 1433423
Conc: 503.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO030421AR1262


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:31 PM

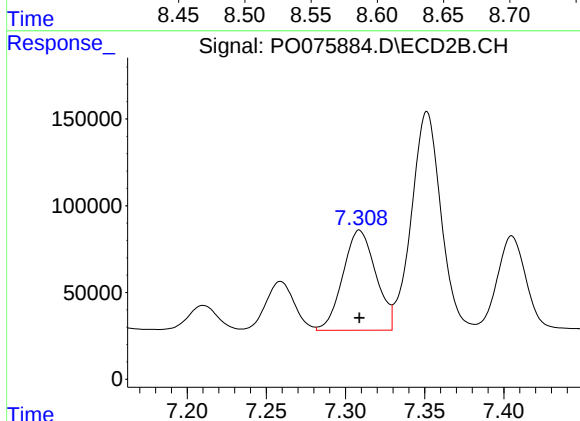


#36 AR-1262-1

R.T.: 7.309 min
Delta R.T.: 0.000 min
Response: 834867
Conc: 485.05 ng/ml

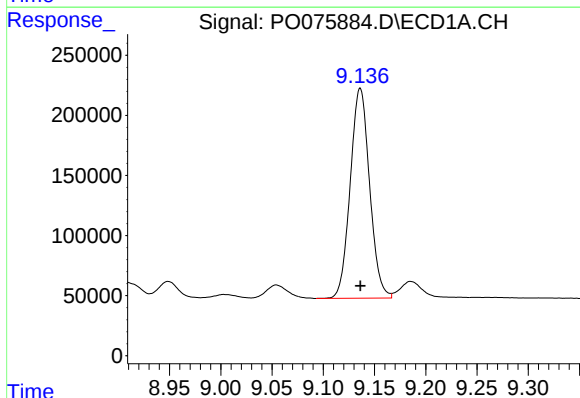


#37 AR-1262-2

R.T.: 9.136 min
Delta R.T.: 0.000 min
Response: 2296715
Conc: 504.00 ng/ml

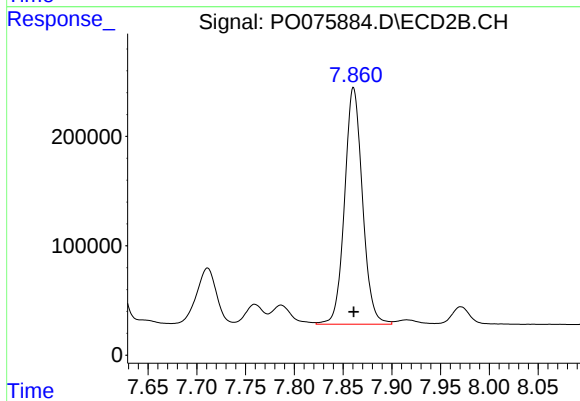

#37 AR-1262-2

R.T.: 7.861 min
Delta R.T.: 0.000 min
Response: 2762173
Conc: 495.59 ng/ml

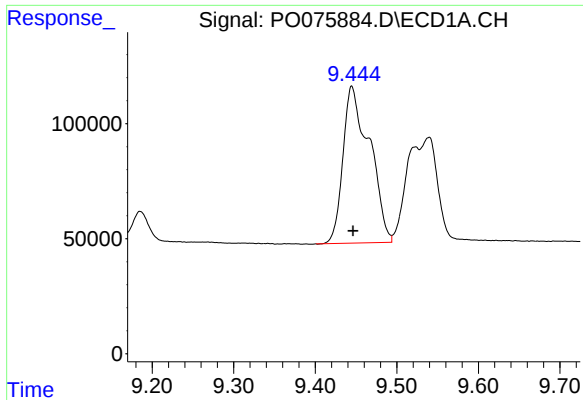


#38 AR-1262-3

R.T.: 9.445 min
Delta R.T.: -0.001 min
Response: 1544357
Conc: 510.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO030421AR1262


Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:31 PM

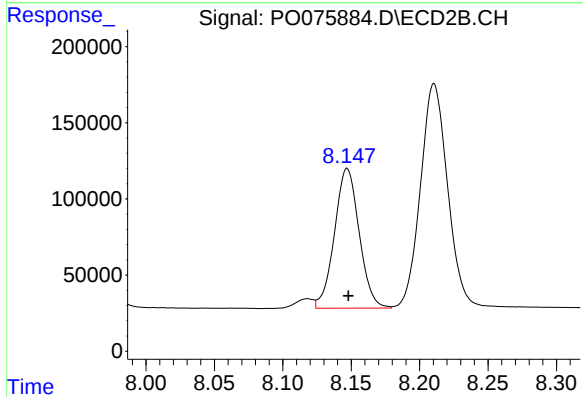


#38 AR-1262-3

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 1152662
Conc: 496.72 ng/ml

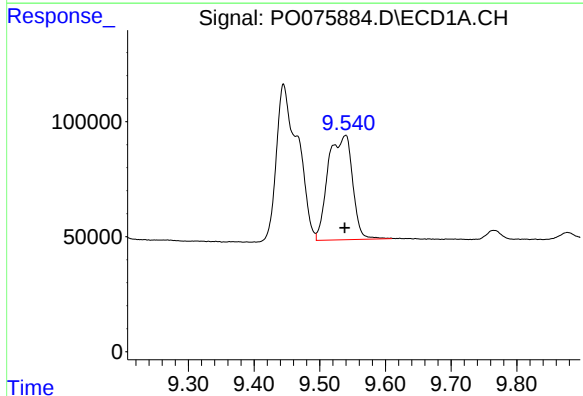


#39 AR-1262-4

R.T.: 9.540 min
Delta R.T.: 0.002 min
Response: 1170673
Conc: 512.42 ng/ml m

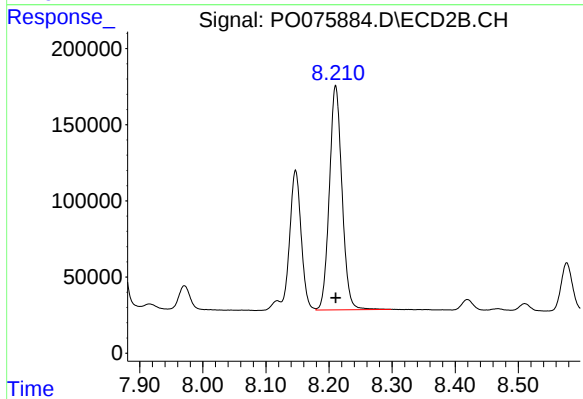

#39 AR-1262-4

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 2045232
Conc: 486.58 ng/ml

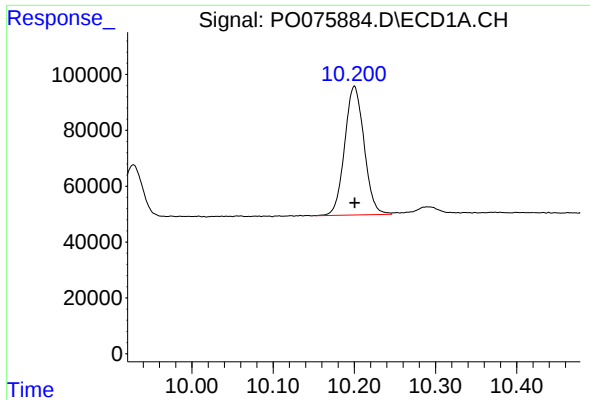


#40 AR-1262-5

R.T.: 10.200 min
Delta R.T.: 0.000 min
Response: 766231
Conc: 505.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO030421AR1262

Manual Integrations
APPROVED

Ankita
3/5/2021 1:35:31 PM

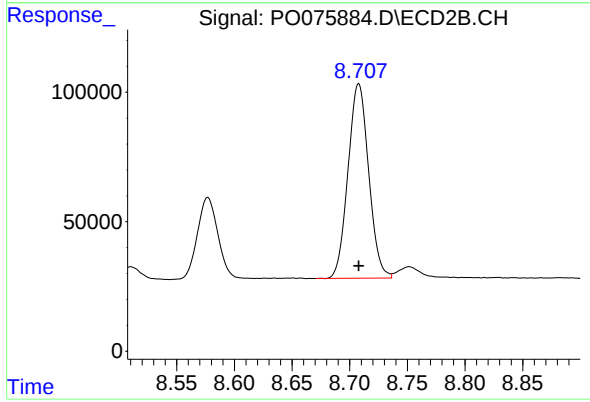

#40 AR-1262-5

R.T.: 8.708 min
Delta R.T.: 0.000 min
Response: 933578
Conc: 516.58 ng/ml