

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030424\
 Data File : P0102302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2024 13:14
 Operator : YP/AJ
 Sample : P1662-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-352

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/05/2024
 Supervised By :Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:23:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.387	65335278	50641056	14.088m	15.585m
2) SA Decachlor...	9.815	8.255	47595981	32157203	18.691m	15.544m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030424\
Data File : PO102302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2024 13:14
Operator : YP/AJ
Sample : P1662-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-352


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/05/2024
Supervised By :Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:23:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

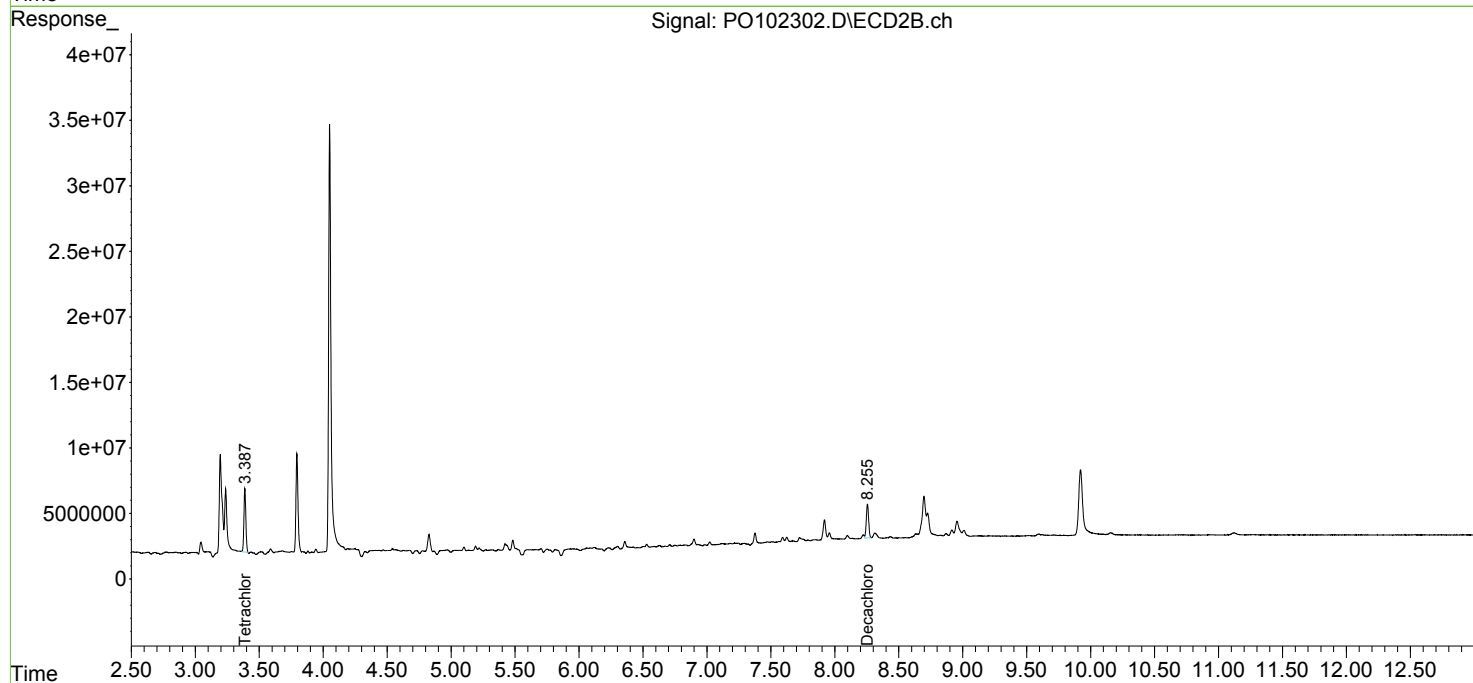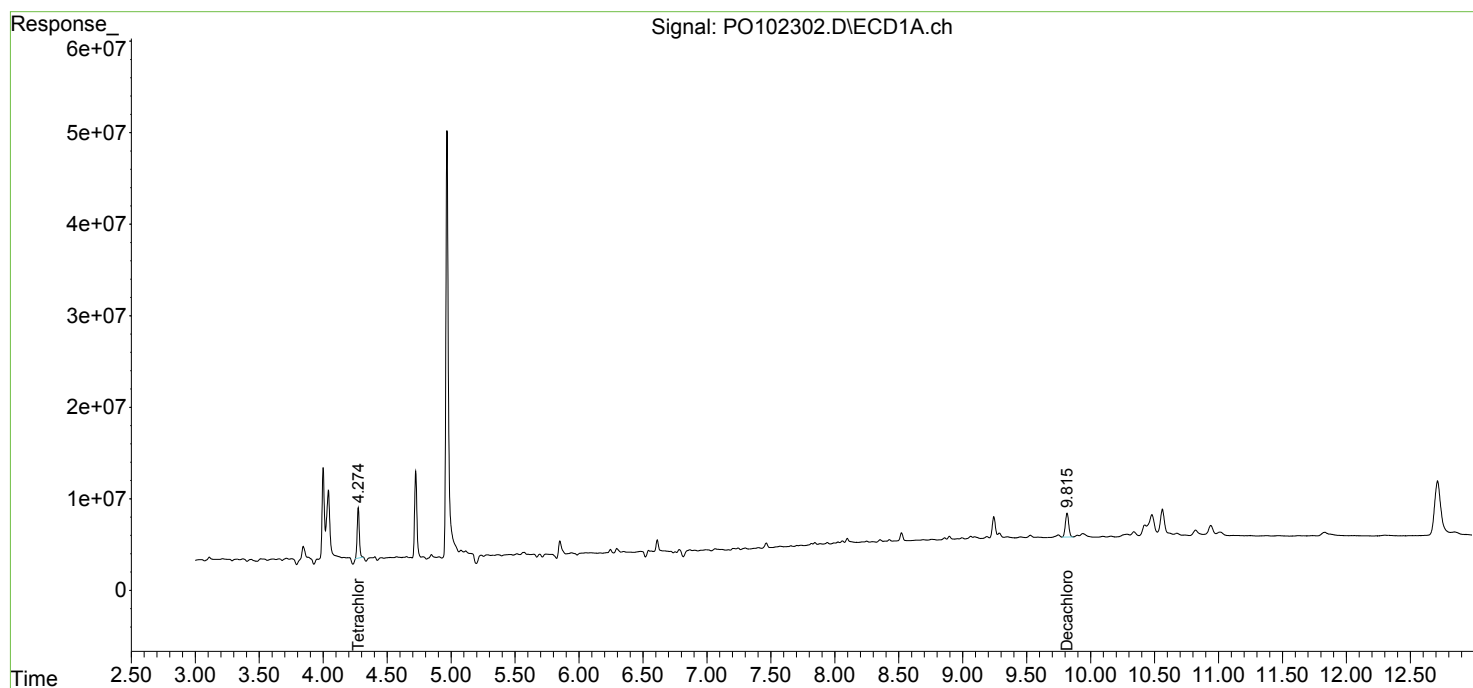

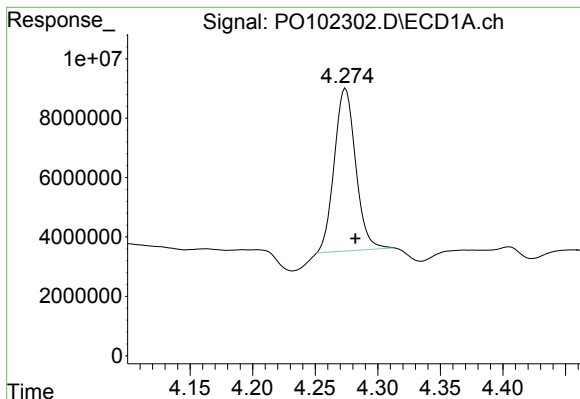


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.008 min
Response: 65335278
Conc: 14.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-352


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/05/2024
Supervised By :Ankita Jodhani 03/05/2024

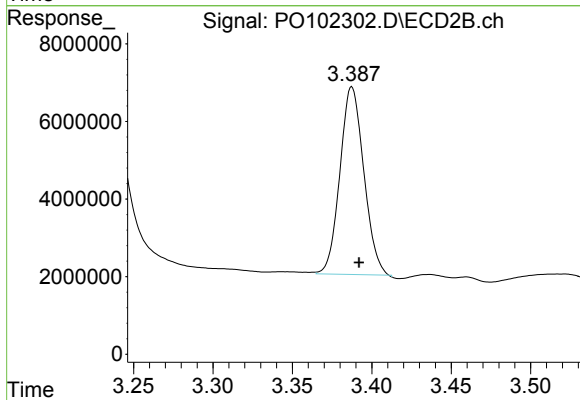


#1 Tetrachloro-m-xylene

R.T.: 3.387 min
Delta R.T.: -0.005 min
Response: 50641056
Conc: 15.58 ng/ml m

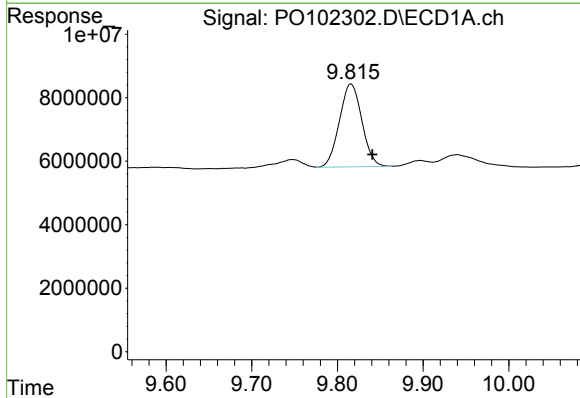

#2 Decachlorobiphenyl

R.T.: 9.815 min
Delta R.T.: -0.026 min
Response: 47595981
Conc: 18.69 ng/ml m

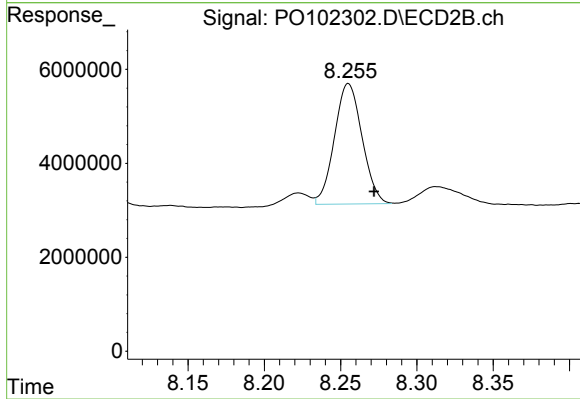

#2 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: -0.017 min
Response: 32157203
Conc: 15.54 ng/ml m