

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030520\
 Data File : P0066953.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2020 13:10
 Operator : DD\AJ
 Sample : PB127281BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB127281BL

Manual Integrations
 APPROVED

Sohil
 3/6/2020 1:22:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 16:19:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.133	3.403	1142702	974717	21.436m	21.024
2) SA Decachlor...	9.606	8.289	1108460	1011481	20.133m	19.564

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030520\
Data File : P0066953.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2020 13:10
Operator : DD\AJ
Sample : PB127281BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PB127281BL


Manual Integrations
APPROVED

Sohil
3/6/2020 1:22:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 16:19:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

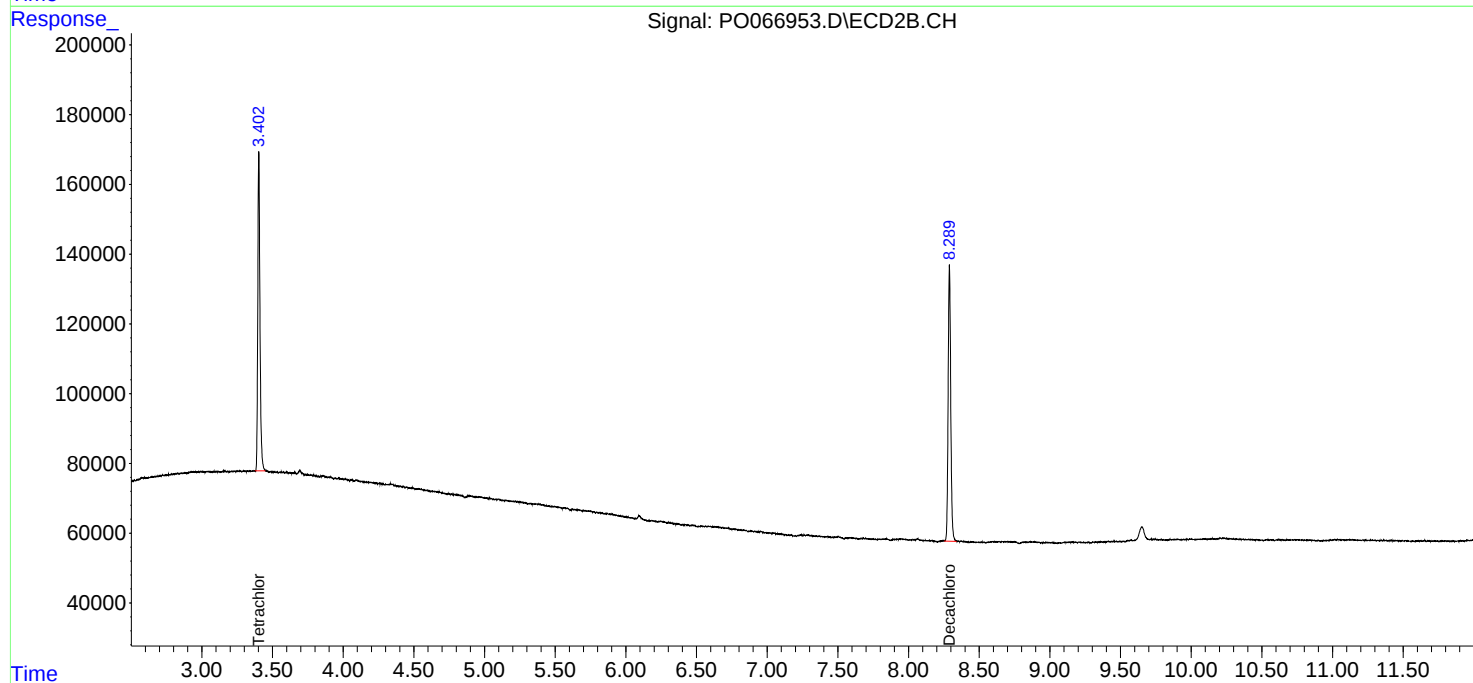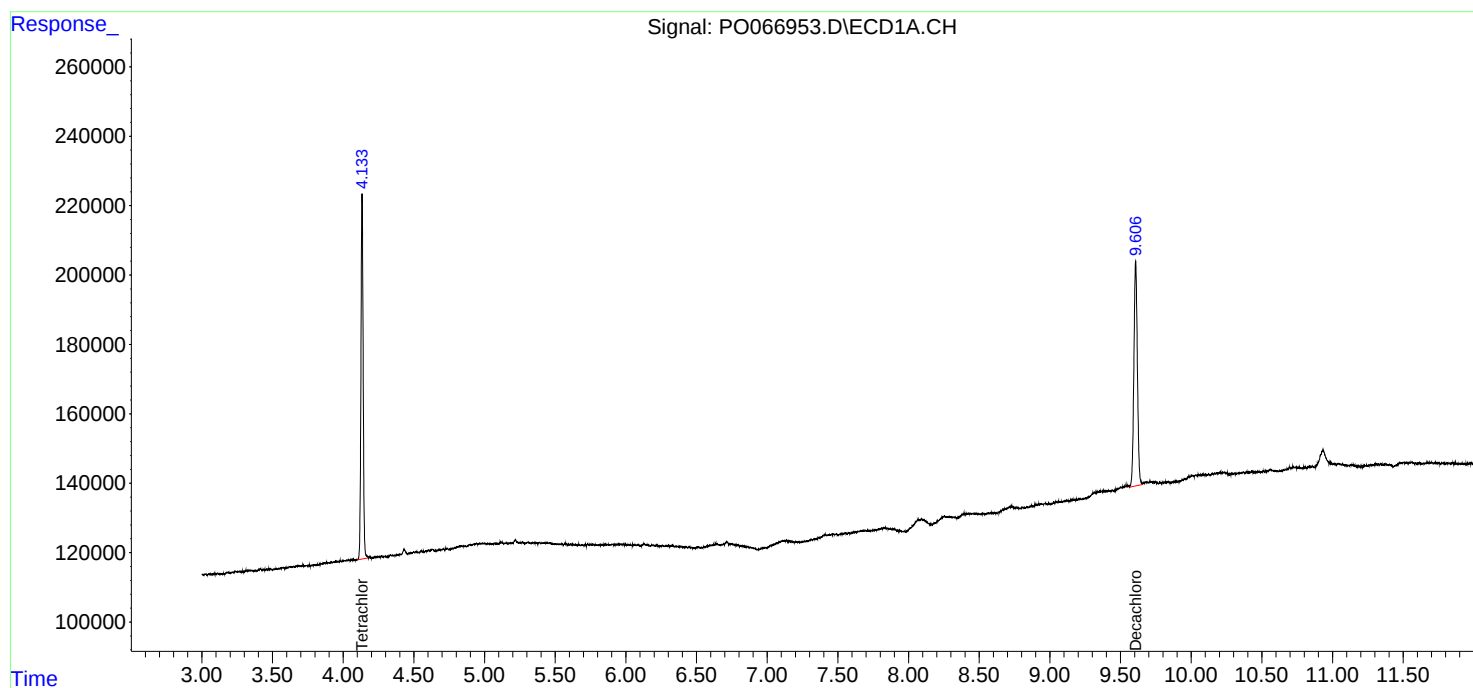

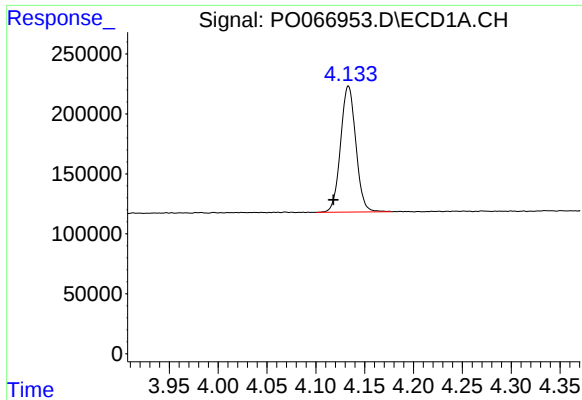


#1 Tetrachloro-m-xylene

R.T.: 4.133 min
Delta R.T.: 0.015 min
Response: 1142702
Conc: 21.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB127281BL


Manual Integrations
APPROVED

Sohil
3/6/2020 1:22:32 PM

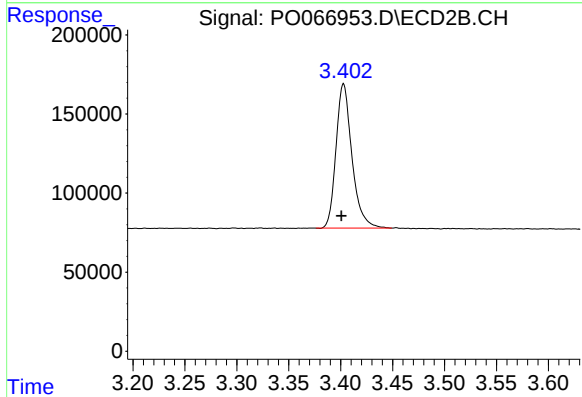


#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.002 min
Response: 974717
Conc: 21.02 ng/ml

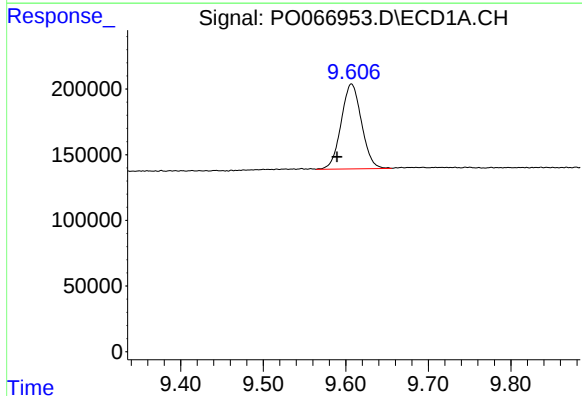

#2 Decachlorobiphenyl

R.T.: 9.606 min
Delta R.T.: 0.017 min
Response: 1108460
Conc: 20.13 ng/ml m

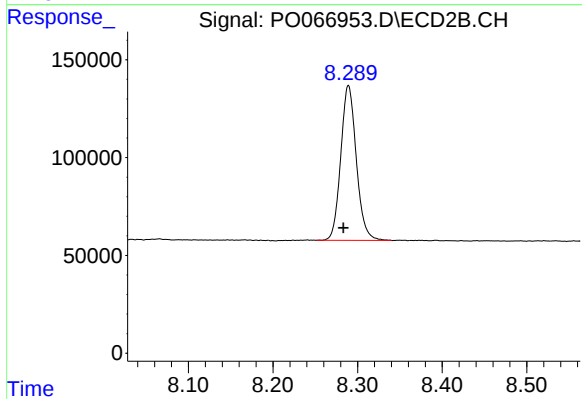

#2 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.006 min
Response: 1011481
Conc: 19.56 ng/ml