

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030520\
Data File : P0066969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2020 17:42
Operator : DD\AJ
Sample : L1791-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
03-04-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 05:34:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.117	3.401	792672	702712	14.870	15.157
2) SA Decachlor...	9.583	8.280	645710	576632	11.728	11.153

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030520\
Data File : P0066969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2020 17:42
Operator : DD\AJ
Sample : L1791-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
03-04-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 05:34:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

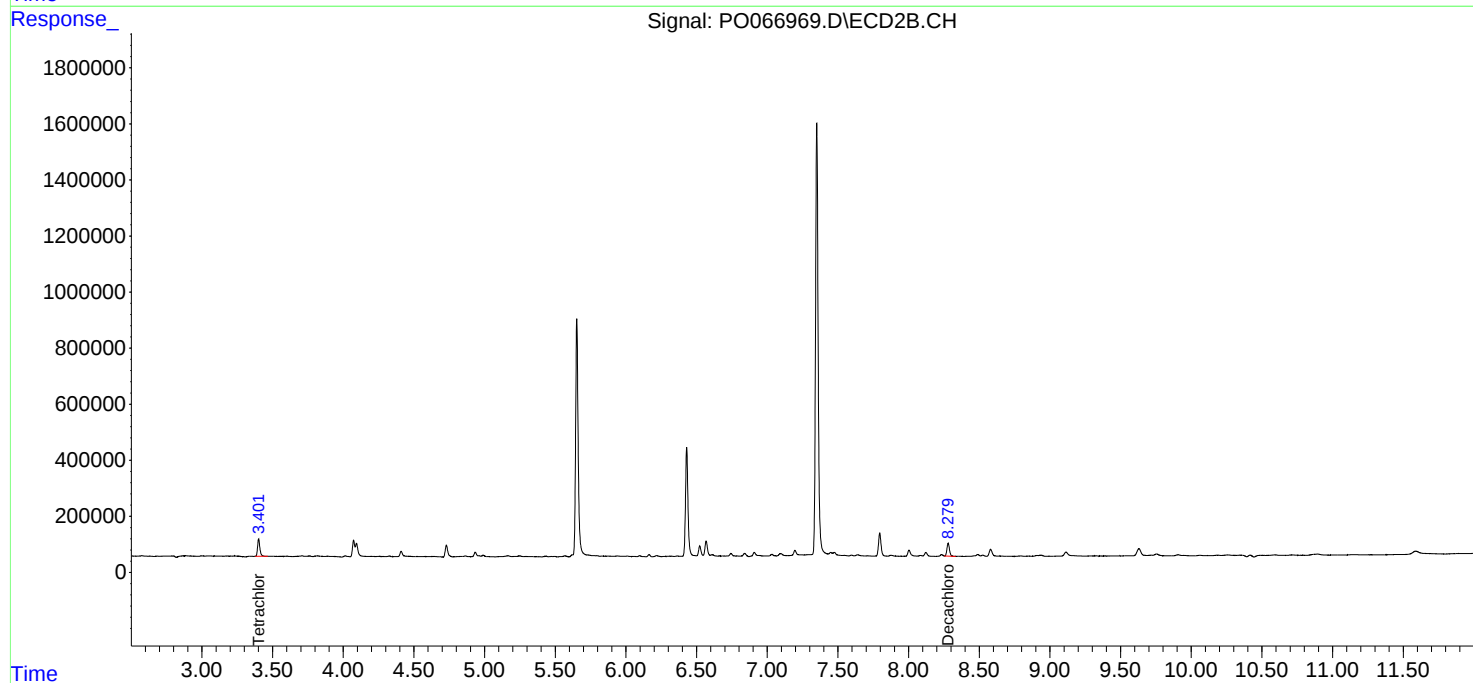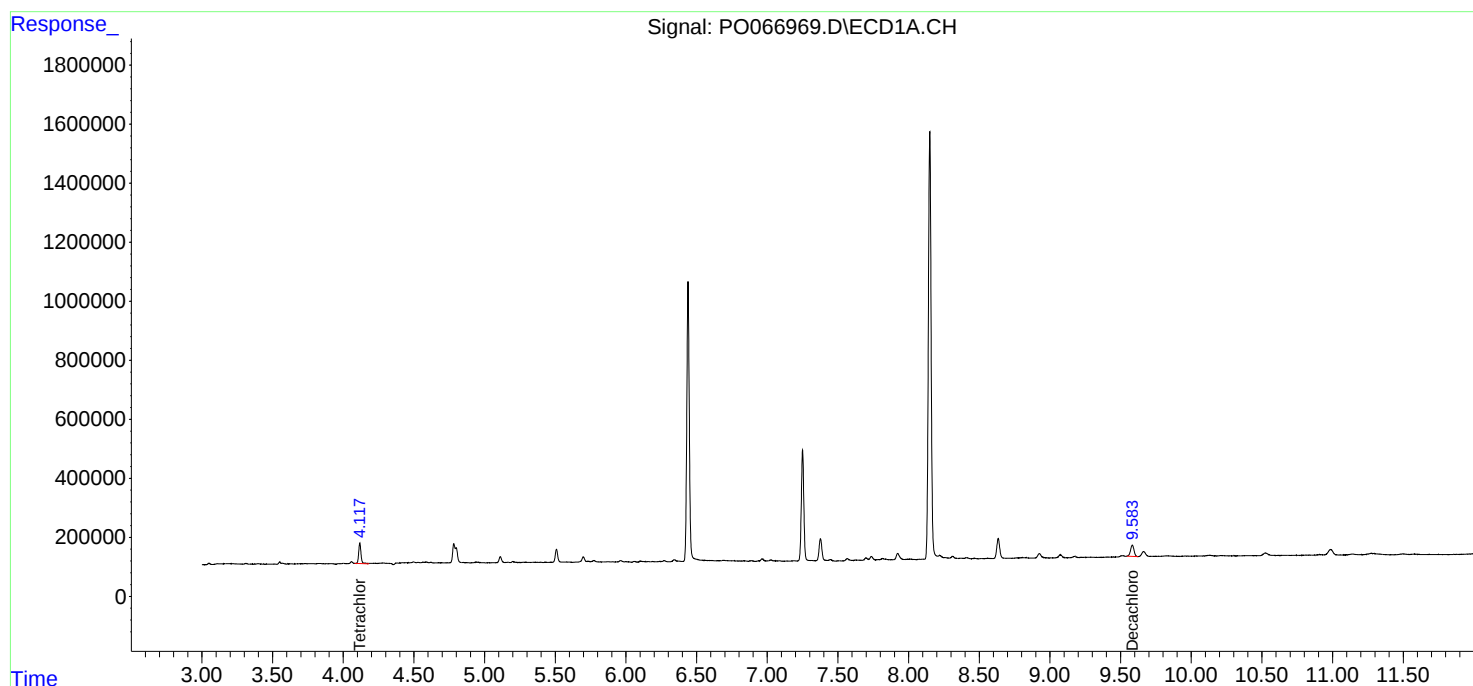


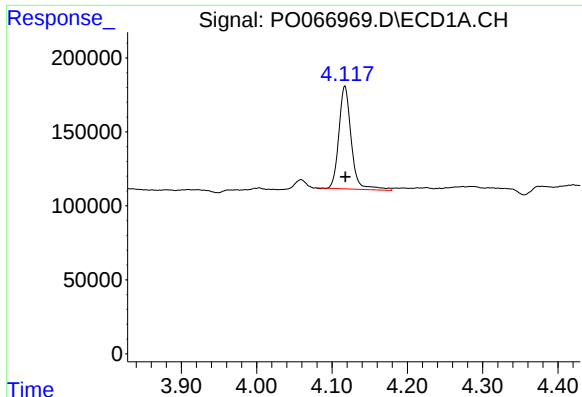

#1 Tetrachloro-m-xylene


R.T.: 4.117 min
Delta R.T.: 0.000 min
Response: 792672
Conc: 14.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-04-B

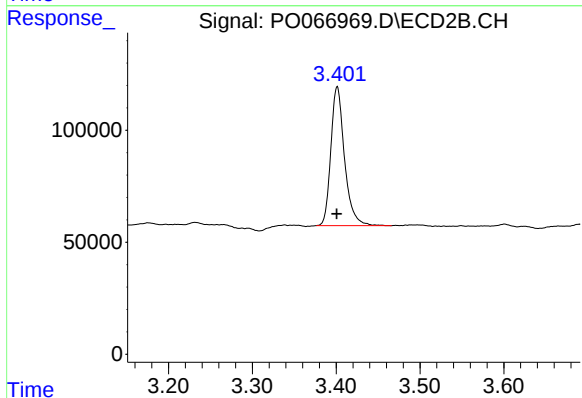


#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 702712
Conc: 15.16 ng/ml

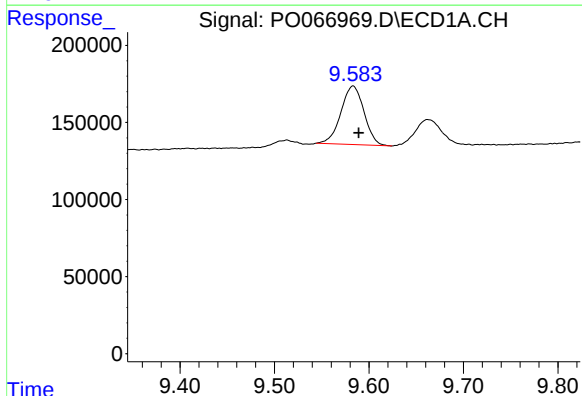

#2 Decachlorobiphenyl

R.T.: 9.583 min
Delta R.T.: -0.006 min
Response: 645710
Conc: 11.73 ng/ml

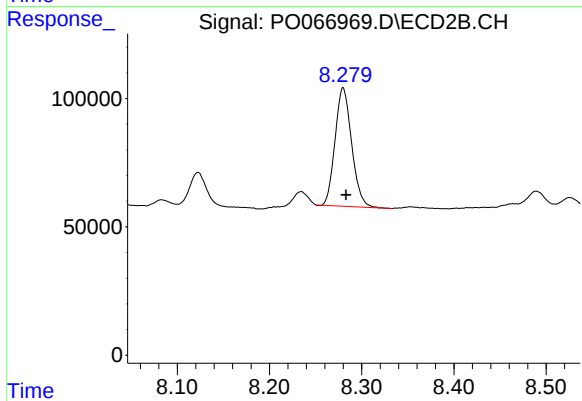

#2 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: -0.003 min
Response: 576632
Conc: 11.15 ng/ml