

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
 Data File : P0075895.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 11:14
 Operator : DD\AJ
 Sample : M1549-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 13:27:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	3.944	1268198	977382	21.276	21.910
2) SA Decachlor...	10.941	9.223	797101	874708	24.264	24.056
Target Compounds						
9) L2 AR-1221-2	5.282	0.000	19978	0	43.560	N.D. #
30) L6 AR-1254-5	8.510	0.000	141643	0	62.228	N.D. #
31) L7 AR-1260-1	0.000	6.796f	0	46565	N.D.	20.518 #
32) L7 AR-1260-2	0.000	7.000f	0	44566	N.D.	16.104 #
33) L7 AR-1260-3	8.588	0.000	234059	0	128.750	N.D. #
36) L8 AR-1262-1	8.588	0.000	234059	0	82.217	N.D. #
38) L8 AR-1262-3	9.459	0.000	117938	0	39.003	N.D. #
41) L9 AR-1268-1	9.459	0.000	117938	0	22.438	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
Data File : P0075895.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 11:14
Operator : DD\AJ
Sample : M1549-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 13:27:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

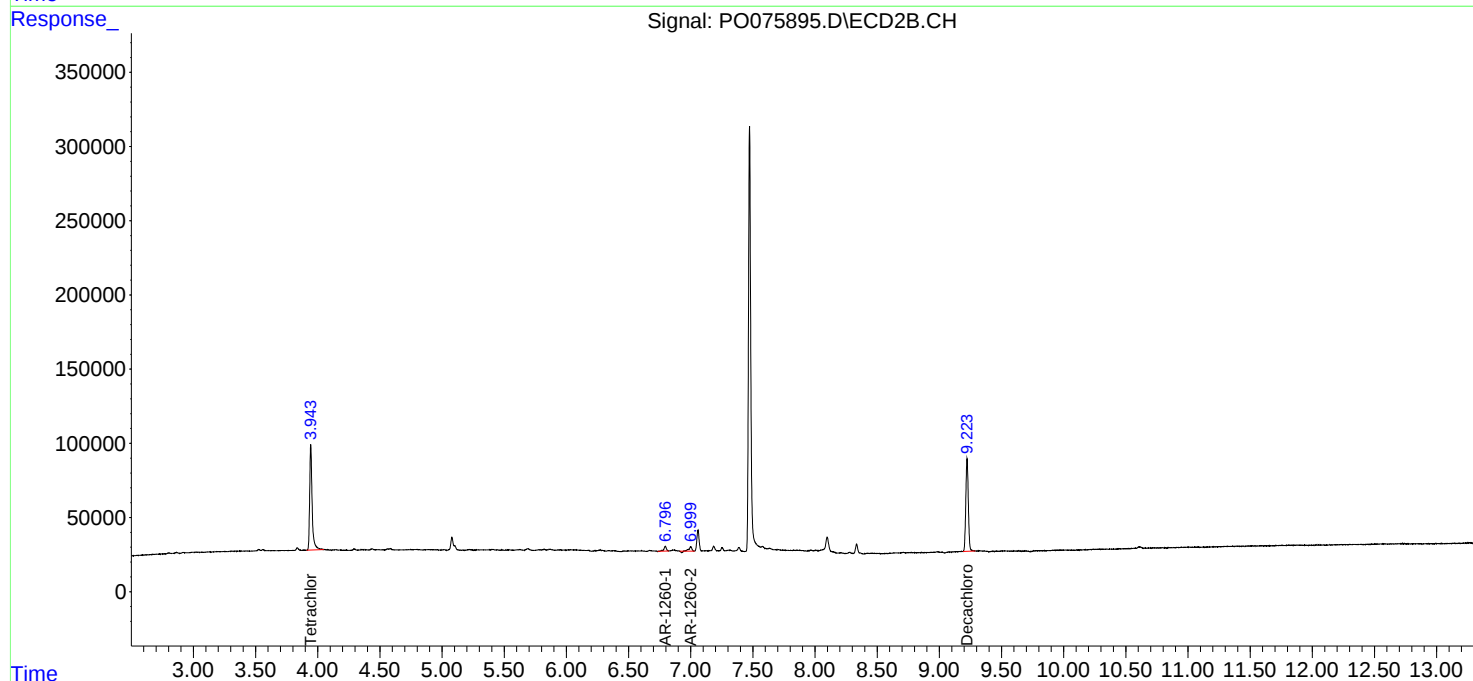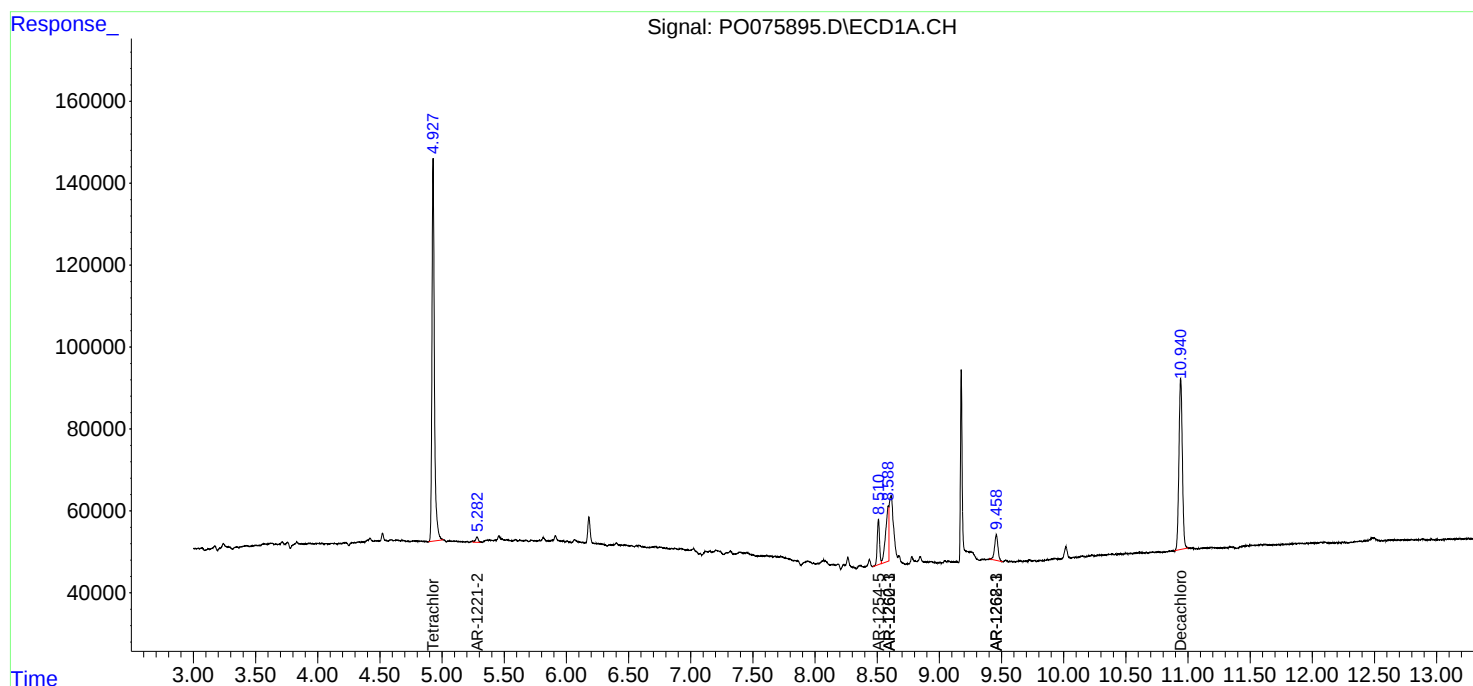


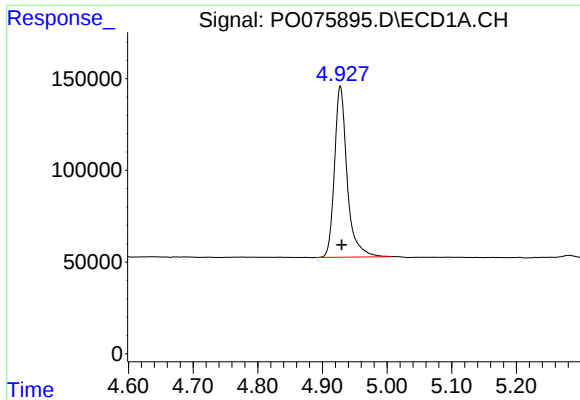

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 1268198
Conc: 21.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

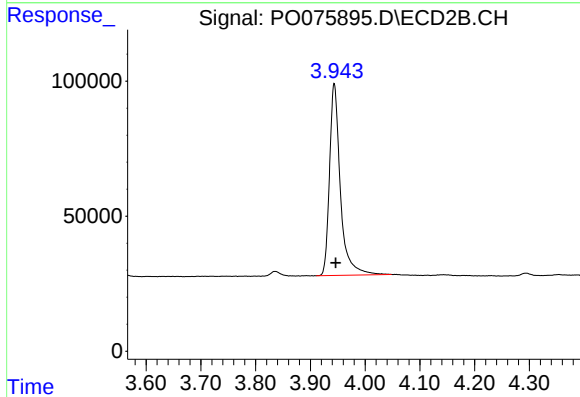


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.003 min
Response: 977382
Conc: 21.91 ng/ml

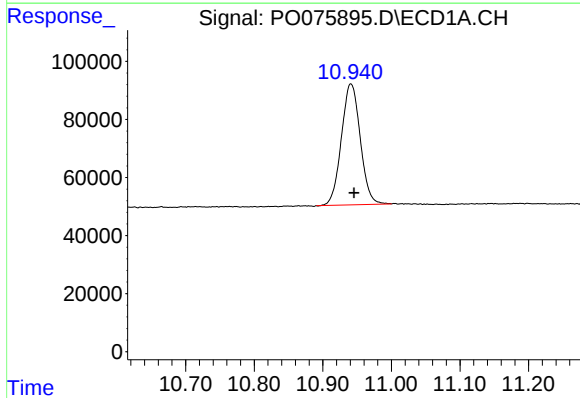


#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: -0.005 min
Response: 797101
Conc: 24.26 ng/ml

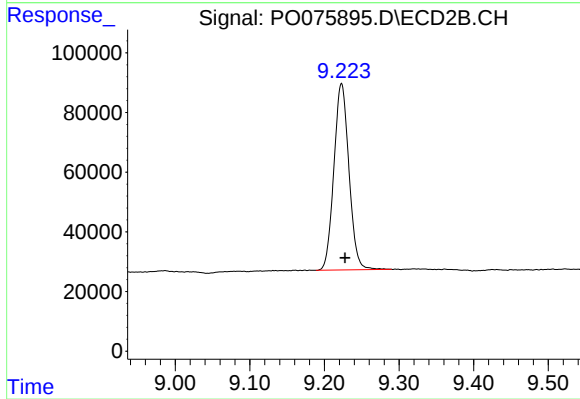

#2 Decachlorobiphenyl


R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 874708
Conc: 24.06 ng/ml

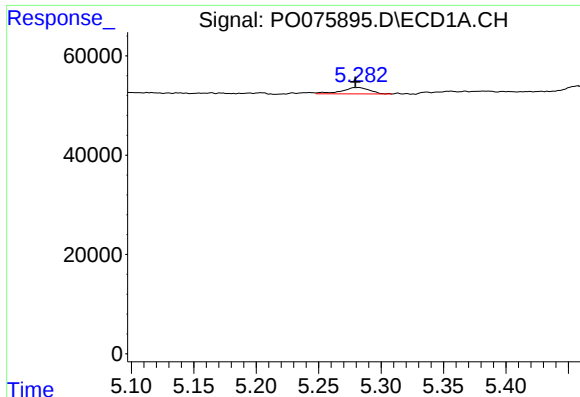

#9 AR-1221-2


R.T.: 5.282 min
Delta R.T.: 0.003 min
Response: 19978
Conc: 43.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

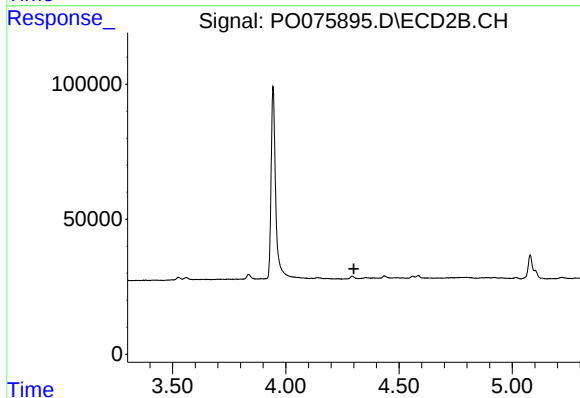


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.

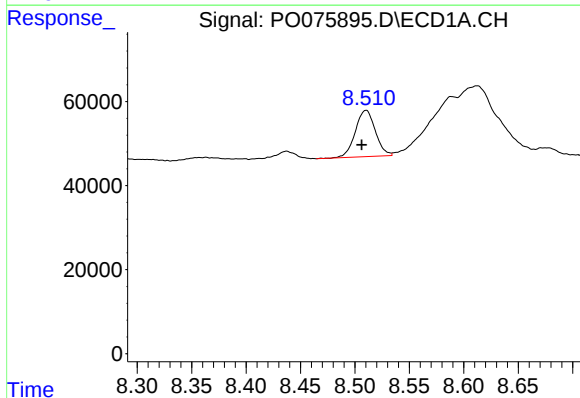


#30 AR-1254-5

R.T.: 8.510 min
Delta R.T.: 0.004 min
Response: 141643
Conc: 62.23 ng/ml

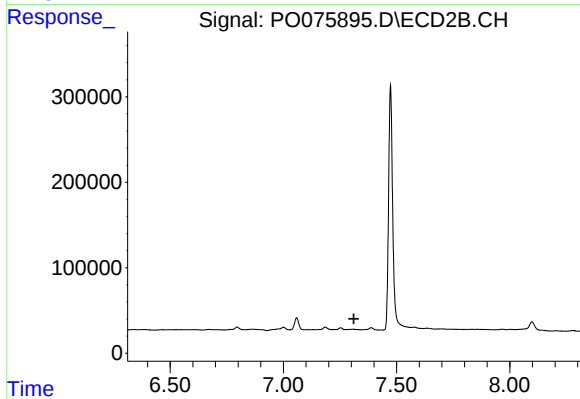

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.311 min
Response: 0
Conc: N.D.

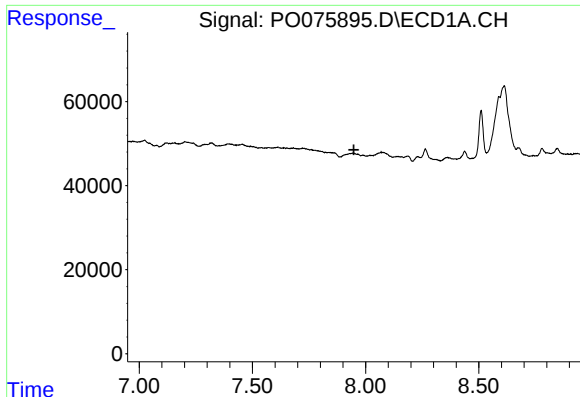

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

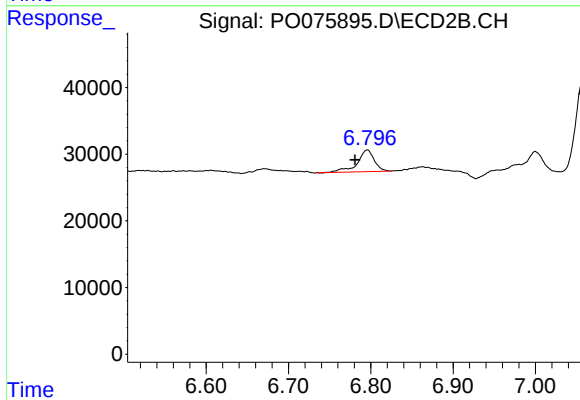


#31 AR-1260-1

R.T.: 6.796 min
Delta R.T.: 0.015 min
Response: 46565
Conc: 20.52 ng/ml

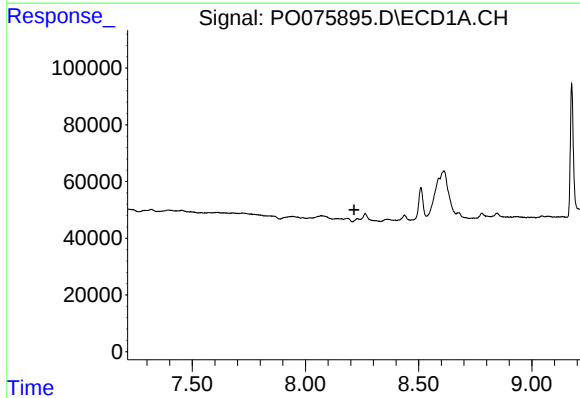


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.214 min
Response: 0
Conc: N.D.

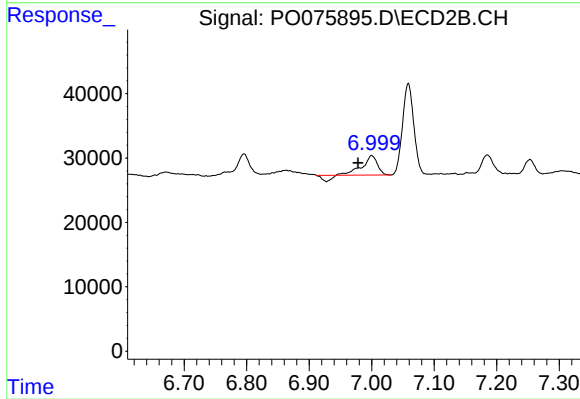

#32 AR-1260-2


R.T.: 7.000 min
Delta R.T.: 0.021 min
Response: 44566
Conc: 16.10 ng/ml

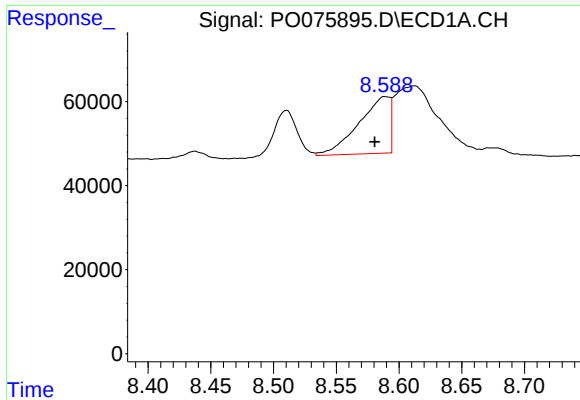

#33 AR-1260-3


R.T.: 8.588 min
Delta R.T.: 0.008 min
Response: 234059
Conc: 128.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

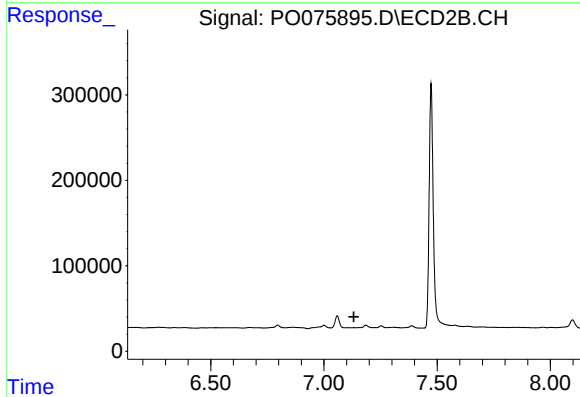


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

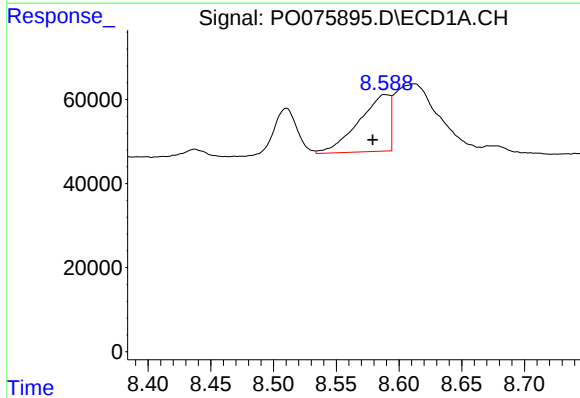


#36 AR-1262-1

R.T.: 8.588 min
Delta R.T.: 0.009 min
Response: 234059
Conc: 82.22 ng/ml

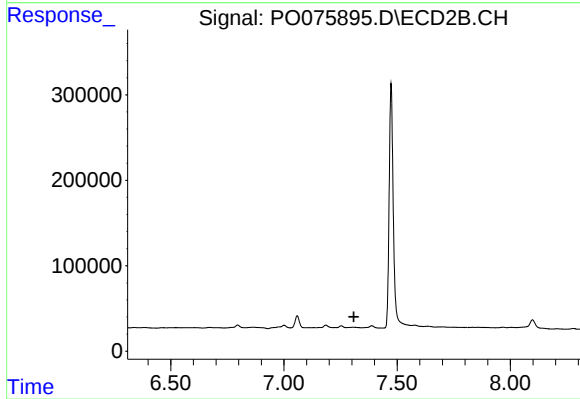

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.309 min
Response: 0
Conc: N.D.

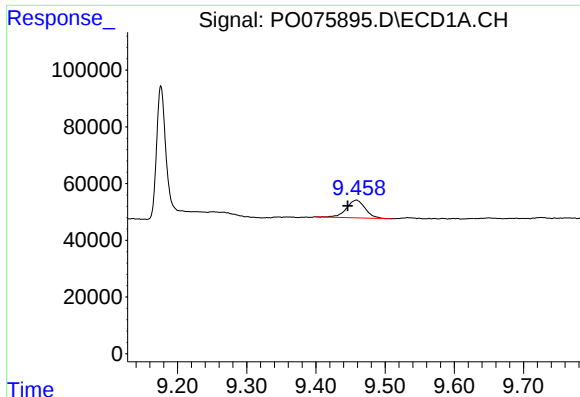

#38 AR-1262-3


R.T.: 9.459 min
Delta R.T.: 0.013 min
Response: 117938
Conc: 39.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

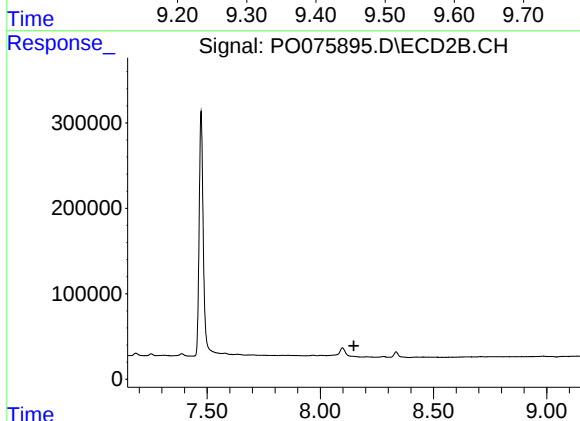


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.148 min
Response: 0
Conc: N.D.

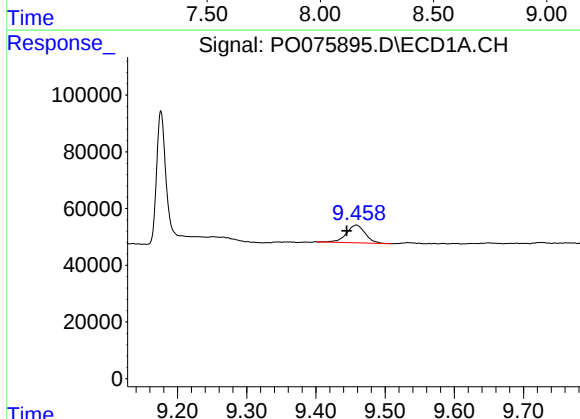

#41 AR-1268-1

R.T.: 9.459 min
Delta R.T.: 0.014 min
Response: 117938
Conc: 22.44 ng/ml

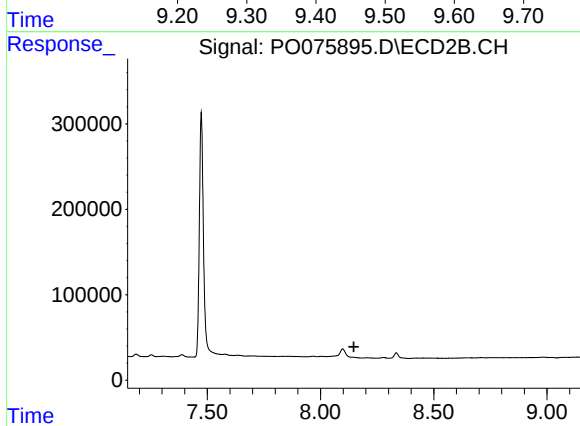

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.147 min
Response: 0
Conc: N.D.