

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
 Data File : P0075900.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 12:40
 Operator : DD\AJ
 Sample : M1556-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-030321

Manual Integrations
 APPROVED

Ankita
 3/8/2021 12:12:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 14:02:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	3.944	1379268	1144087	23.139m	25.648
2) SA Decachlor...	10.942	9.224	927310	891585	28.227	24.520

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
Data File : P0075900.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 12:40
Operator : DD\AJ
Sample : M1556-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-030321


Manual Integrations
APPROVED

Ankita
3/8/2021 12:12:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 14:02:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

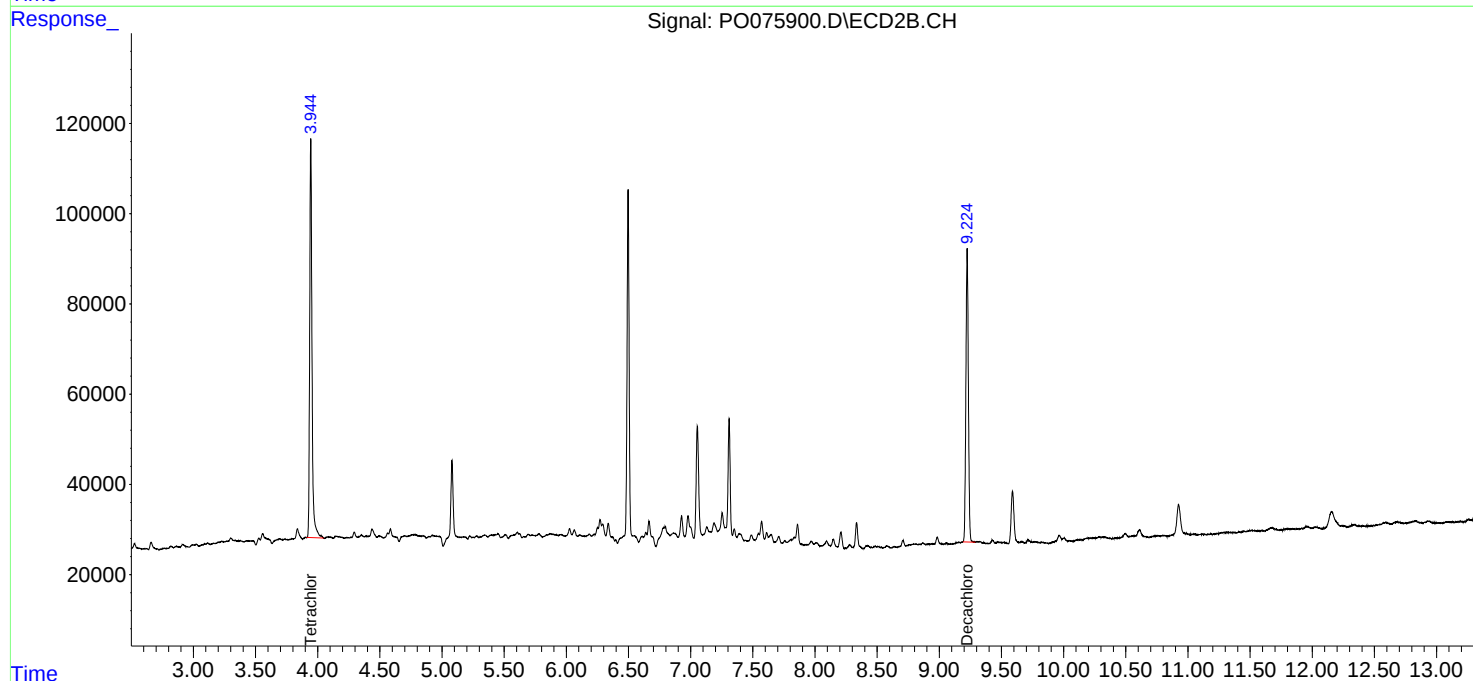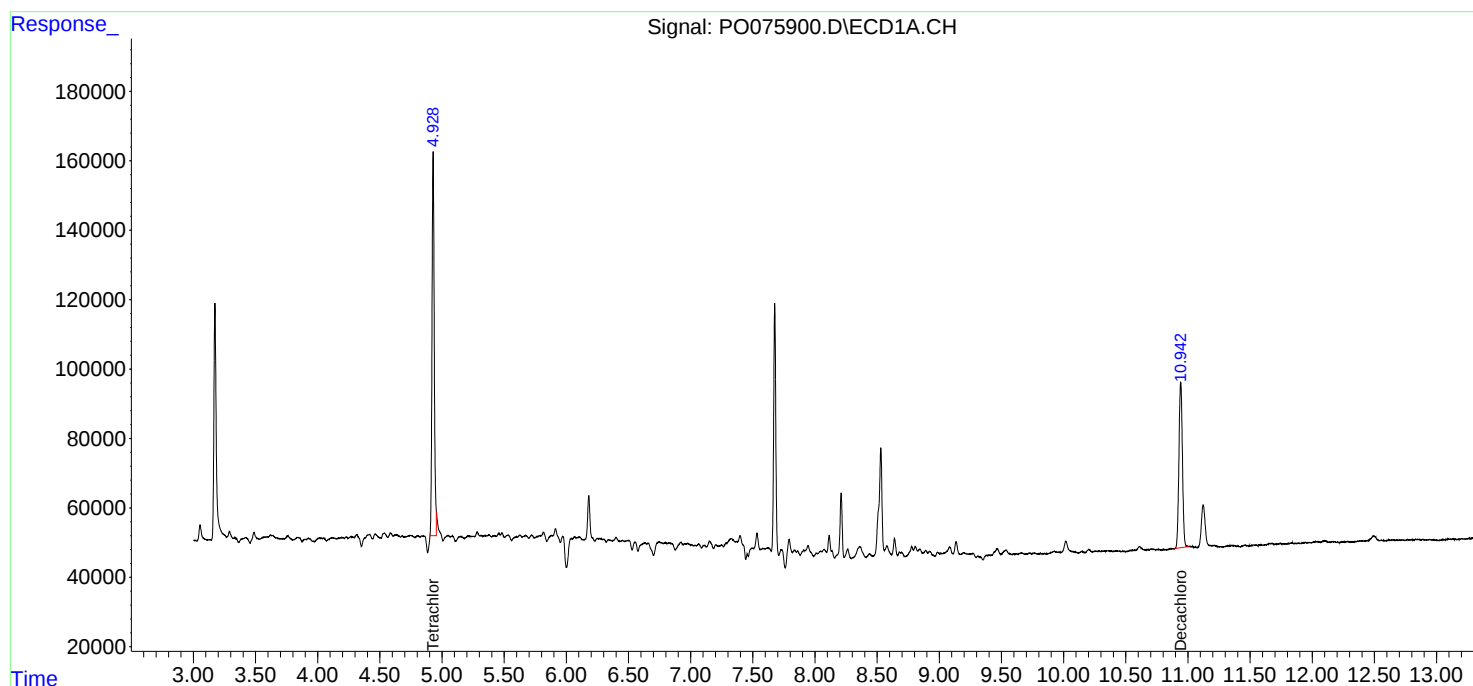

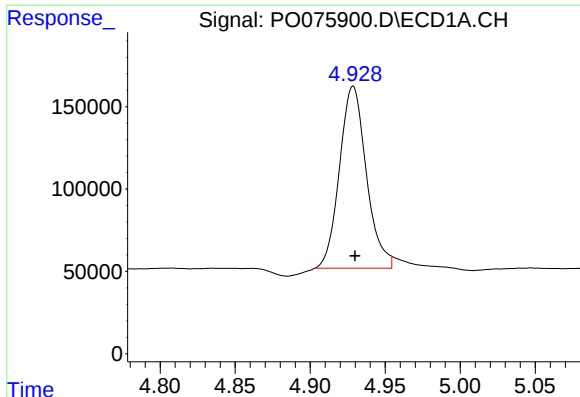


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 1379268
Conc: 23.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TR-04-030321


Manual Integrations
APPROVED

Ankita
3/8/2021 12:12:36 PM

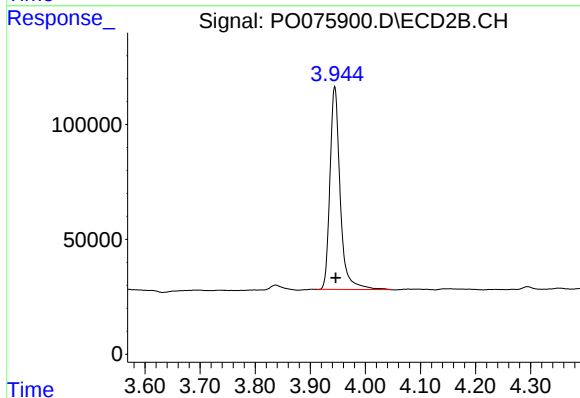


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.002 min
Response: 1144087
Conc: 25.65 ng/ml

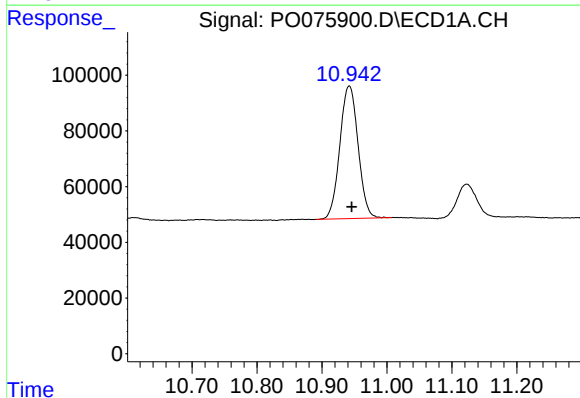

#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 927310
Conc: 28.23 ng/ml

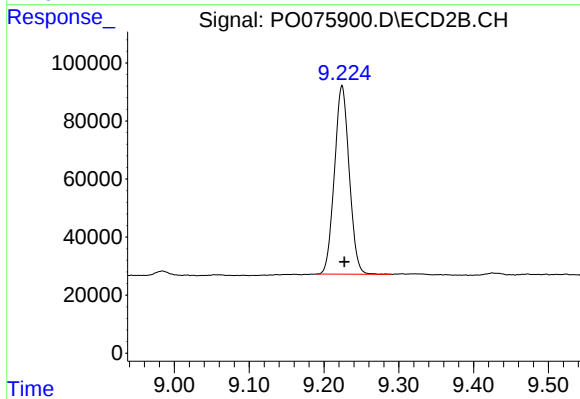

#2 Decachlorobiphenyl

R.T.: 9.224 min
Delta R.T.: -0.003 min
Response: 891585
Conc: 24.52 ng/ml