

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
 Data File : P0075907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 14:58
 Operator : DD\AJ
 Sample : M1567-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-02-030421

Manual Integrations
 APPROVED

Ankita
 3/8/2021 12:12:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 16:23:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	3.943	1126272	941786	18.895m	21.112
2) SA Decachlor...	10.941	9.223	789138	793830	24.021	21.832

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
Data File : P0075907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 14:58
Operator : DD\AJ
Sample : M1567-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-02-030421


Manual Integrations
APPROVED

Ankita
3/8/2021 12:12:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 16:23:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

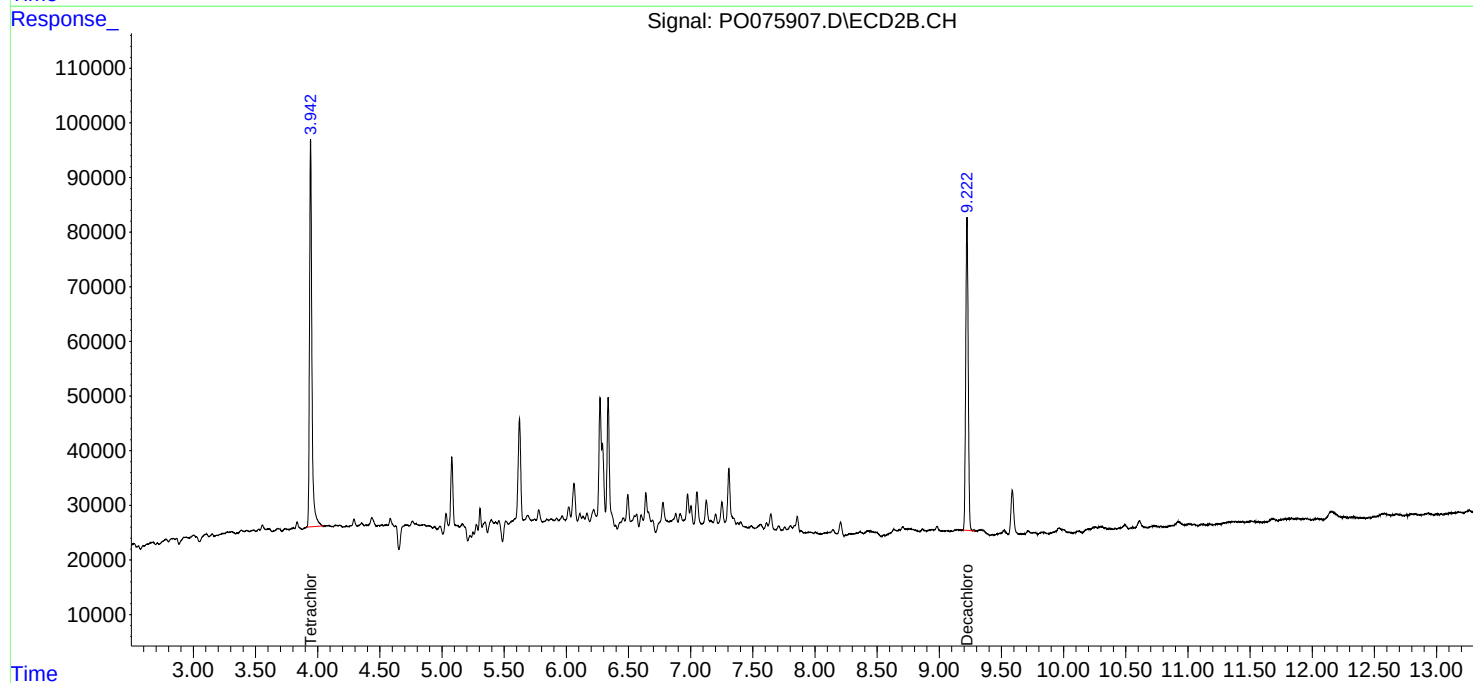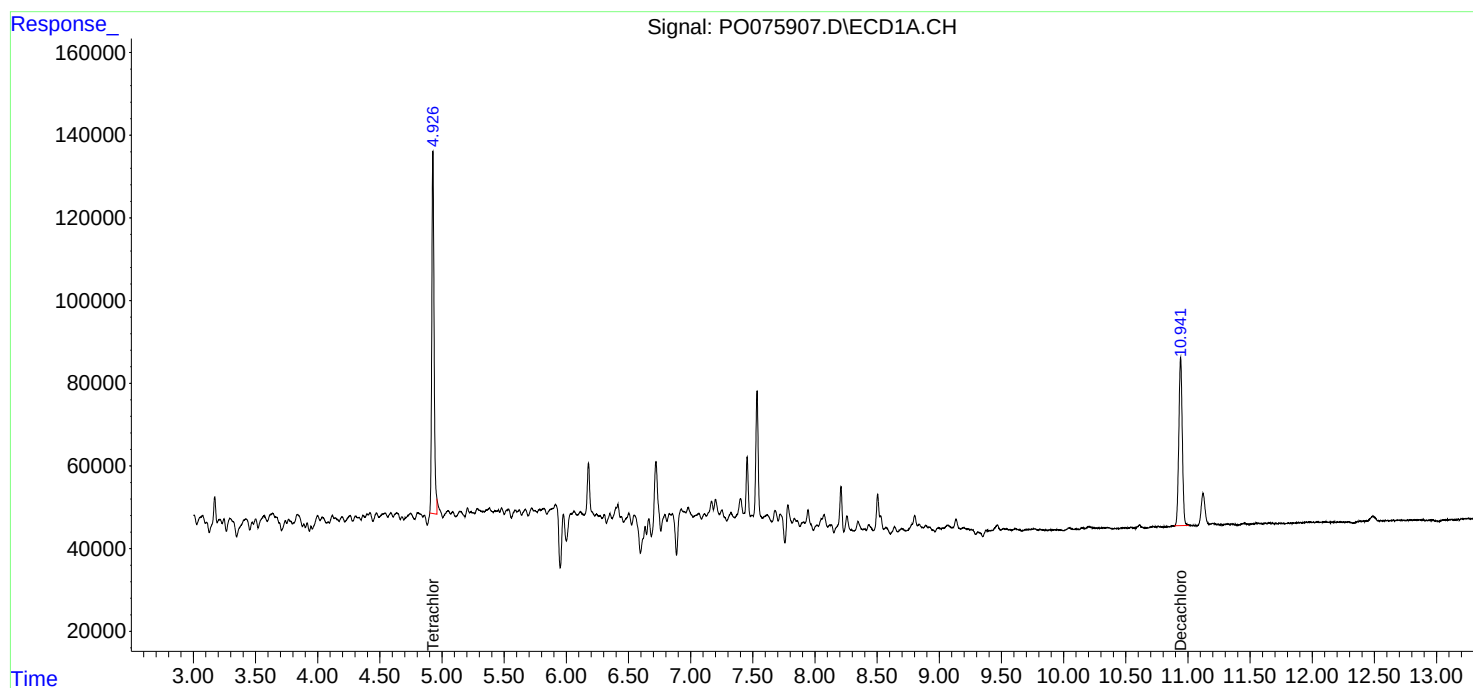

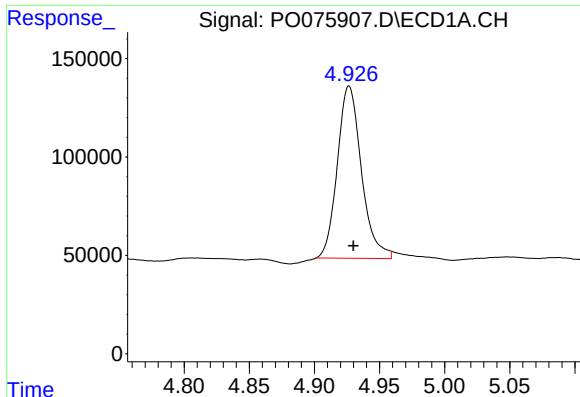


#1 Tetrachloro-m-xylene

R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 1126272
Conc: 18.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PL-02-030421


Manual Integrations
APPROVED

Ankita
3/8/2021 12:12:40 PM

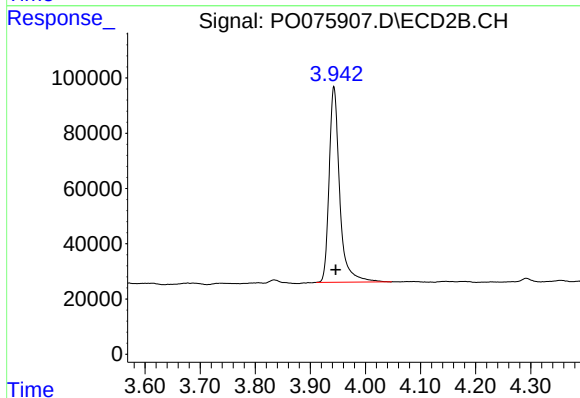


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: -0.003 min
Response: 941786
Conc: 21.11 ng/ml

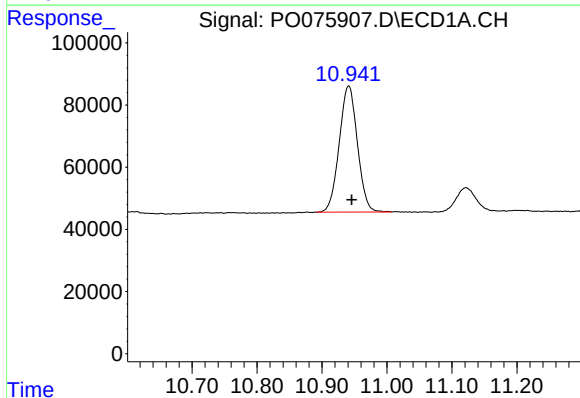

#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: -0.005 min
Response: 789138
Conc: 24.02 ng/ml

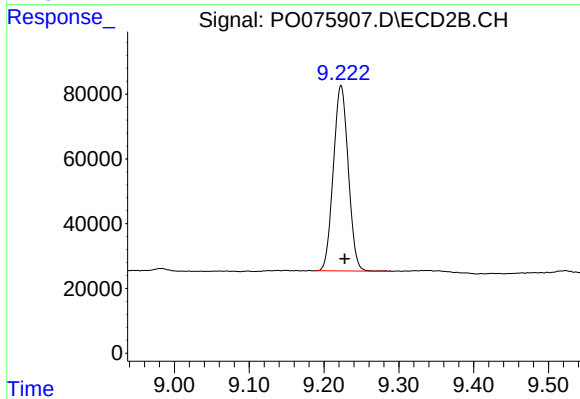

#2 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.005 min
Response: 793830
Conc: 21.83 ng/ml