

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
 Data File : P0075927.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 20:58
 Operator : DD\AJ
 Sample : M1575-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-GW807B-AQ-030421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:54:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	3.944	1248752	974806	20.950	21.853
2) SA Decachlor...	10.940	9.221	678283	758838	20.647	20.870

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
Data File : P0075927.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 20:58
Operator : DD\AJ
Sample : M1575-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-GW807B-AQ-030421

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:54:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

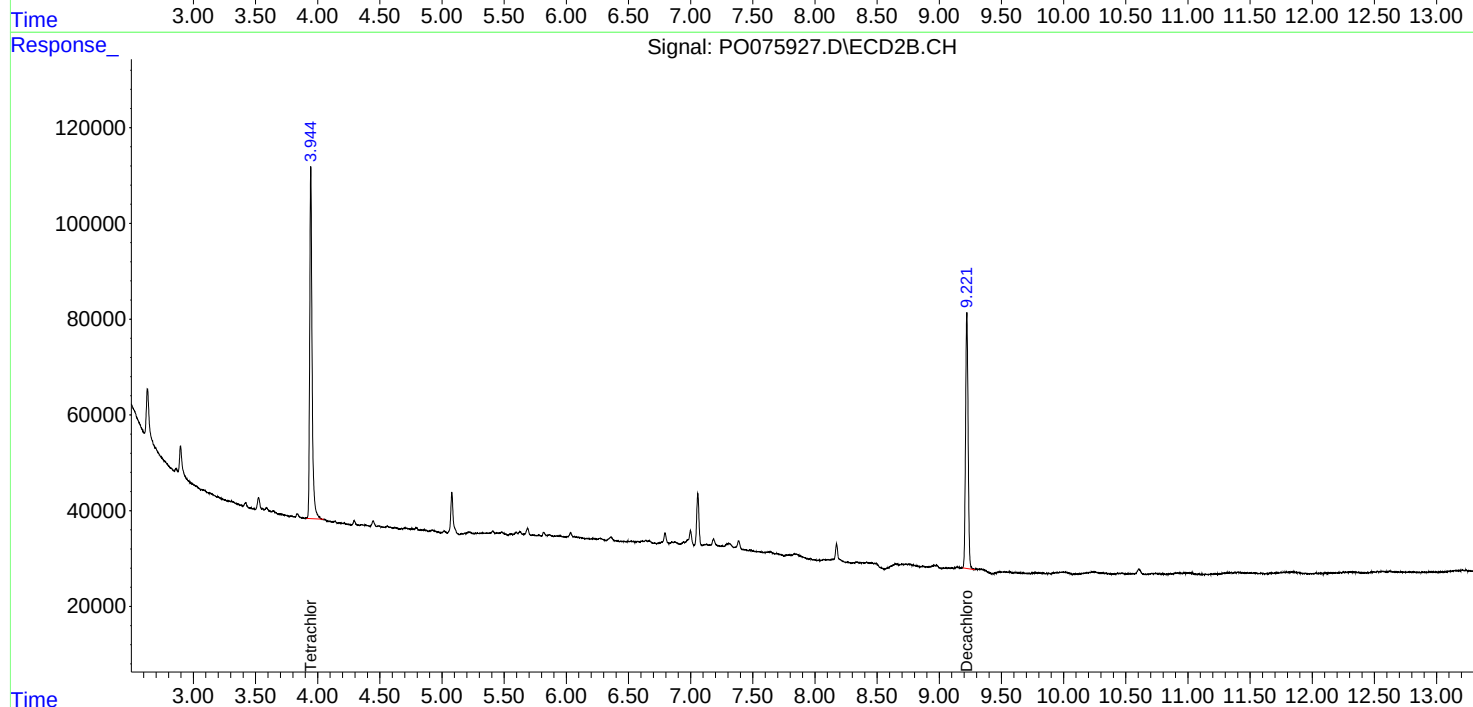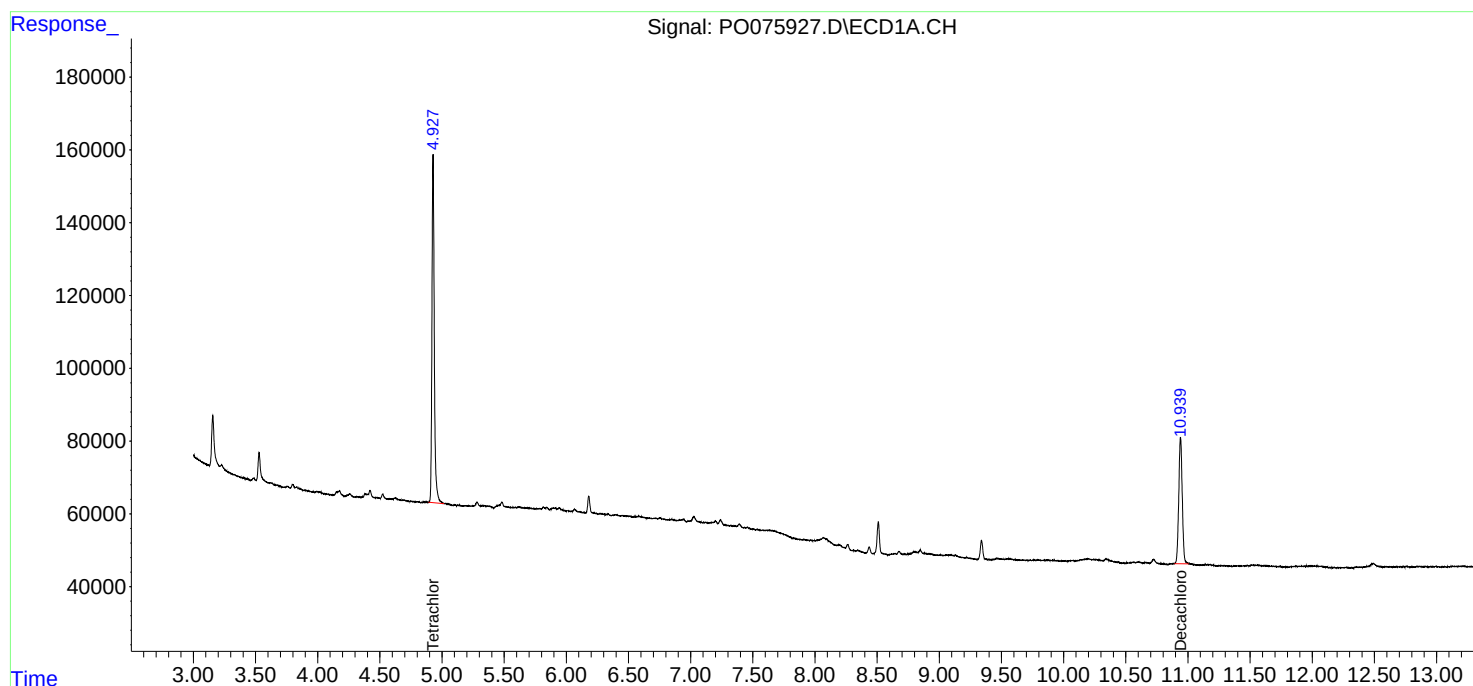


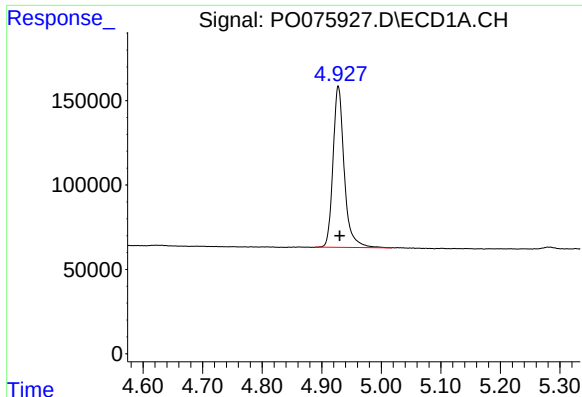

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 1248752
Conc: 20.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-GW807B-AQ-030421

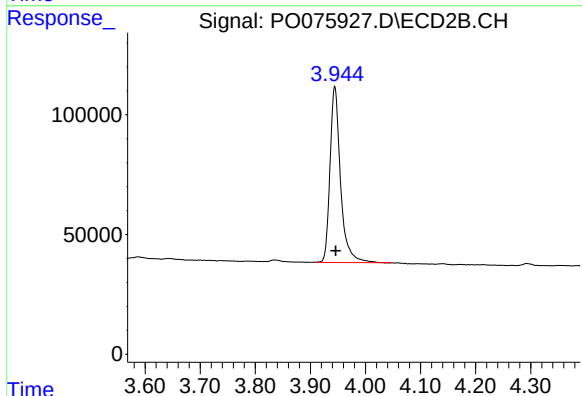


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.002 min
Response: 974806
Conc: 21.85 ng/ml

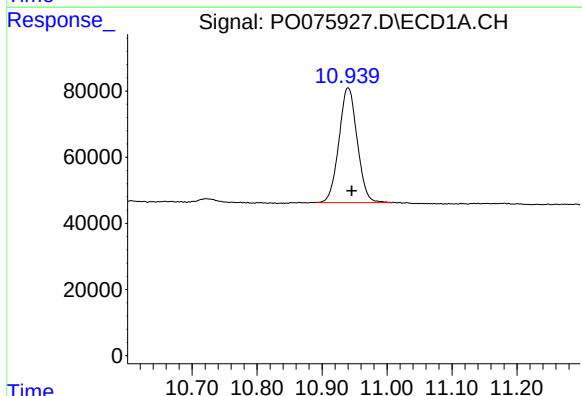

#2 Decachlorobiphenyl

R.T.: 10.940 min
Delta R.T.: -0.006 min
Response: 678283
Conc: 20.65 ng/ml

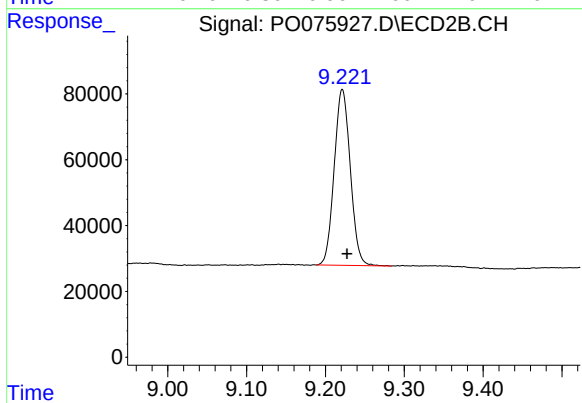

#2 Decachlorobiphenyl

R.T.: 9.221 min
Delta R.T.: -0.006 min
Response: 758838
Conc: 20.87 ng/ml