

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
 Data File : P0075928.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 21:15
 Operator : DD\AJ
 Sample : M1585-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-028-IDWGW-20210304

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:54:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.930	3.945	1233730	970266	20.698	21.751
2)	SA Decachlor...	10.940	9.222	503694	577806	15.333	15.891

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030521\
Data File : P0075928.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 21:15
Operator : DD\AJ
Sample : M1585-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-028-IDWGW-20210304

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:54:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

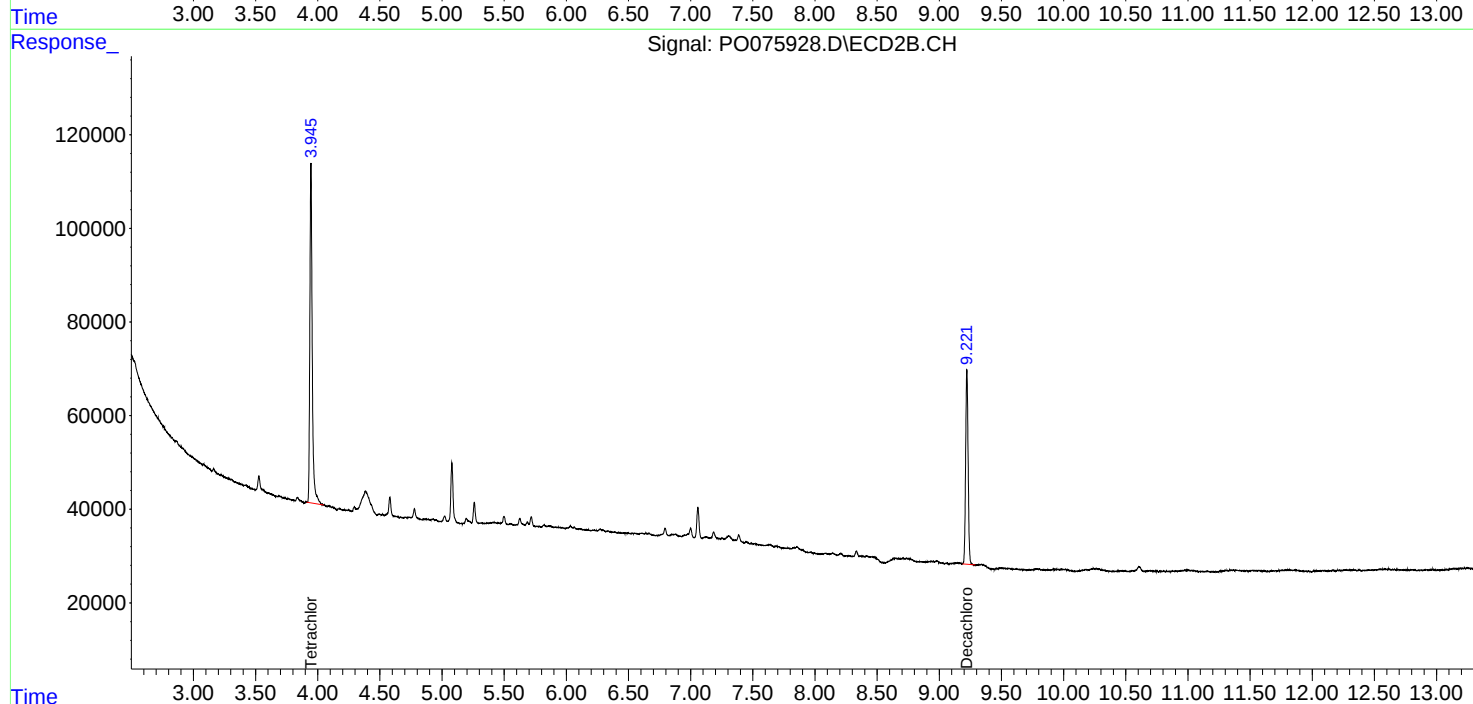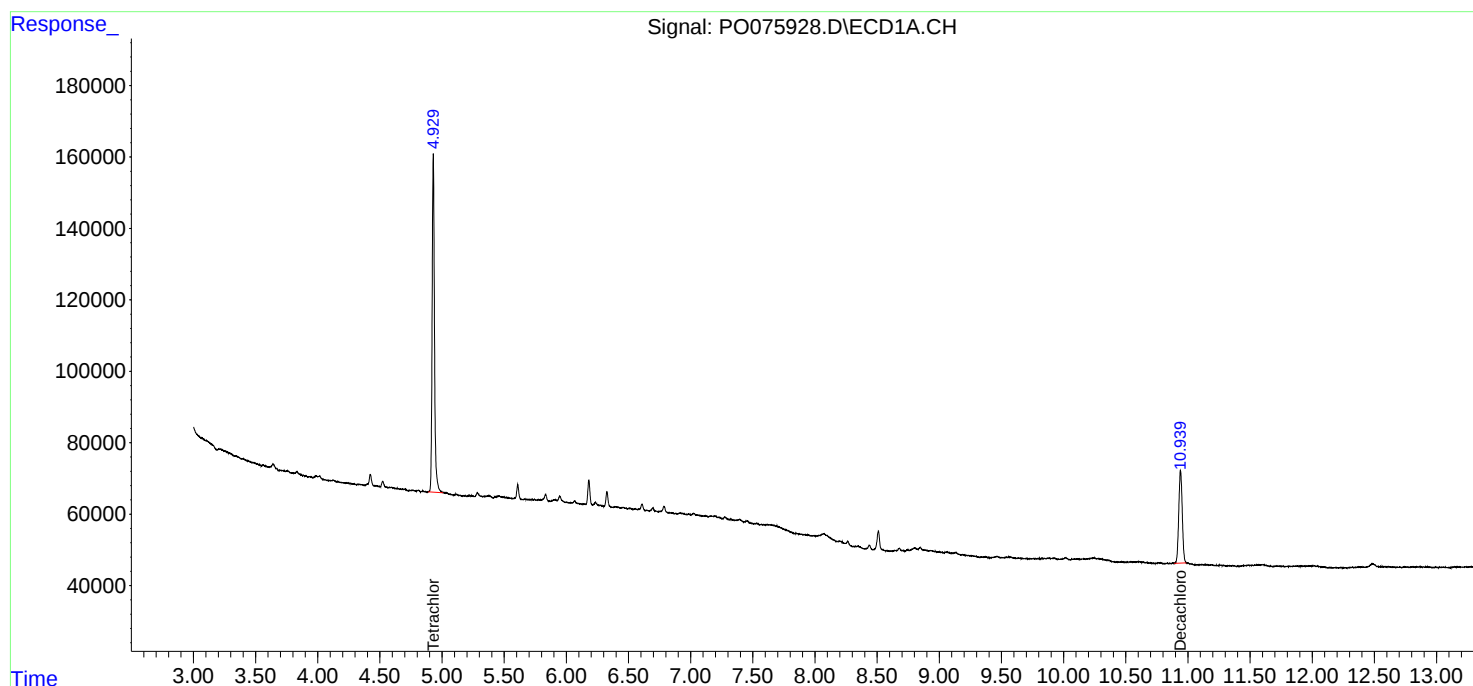


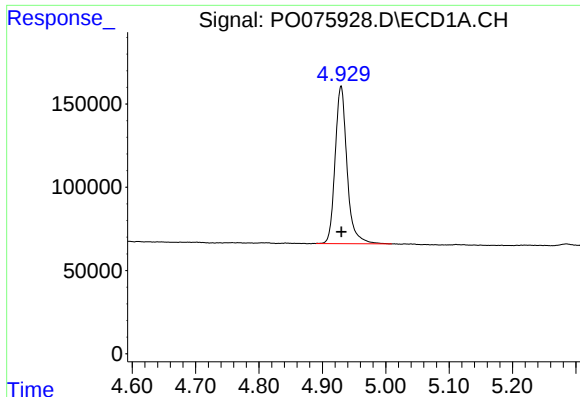

#1 Tetrachloro-m-xylene


R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 1233730
Conc: 20.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-028-IDWGW-20210304

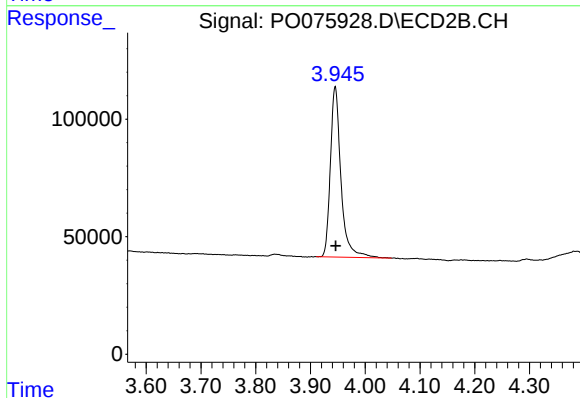


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 970266
Conc: 21.75 ng/ml

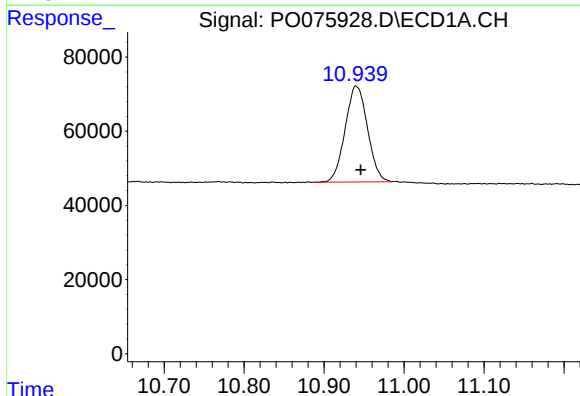

#2 Decachlorobiphenyl

R.T.: 10.940 min
Delta R.T.: -0.006 min
Response: 503694
Conc: 15.33 ng/ml

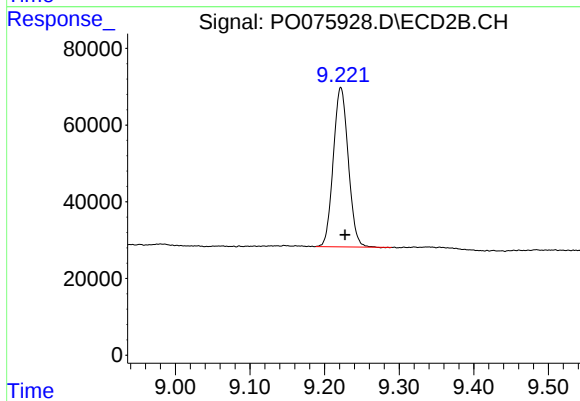

#2 Decachlorobiphenyl

R.T.: 9.222 min
Delta R.T.: -0.006 min
Response: 577806
Conc: 15.89 ng/ml