

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030619\
 Data File : P0054263.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2019 15:16
 Operator : SM/SJ
 Sample : K1732-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-07(22-23)-20190301

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 04:10:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 05 06:51:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.029	3.116	96984285	6510783	17.442	20.723
2) SA Decachlor...	9.346	7.684	25453341	5940598	17.143	18.573

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030619\
Data File : P0054263.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2019 15:16
Operator : SM/SJ
Sample : K1732-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-07(22-23)-20190301

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 04:10:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030419.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 05 06:51:55 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

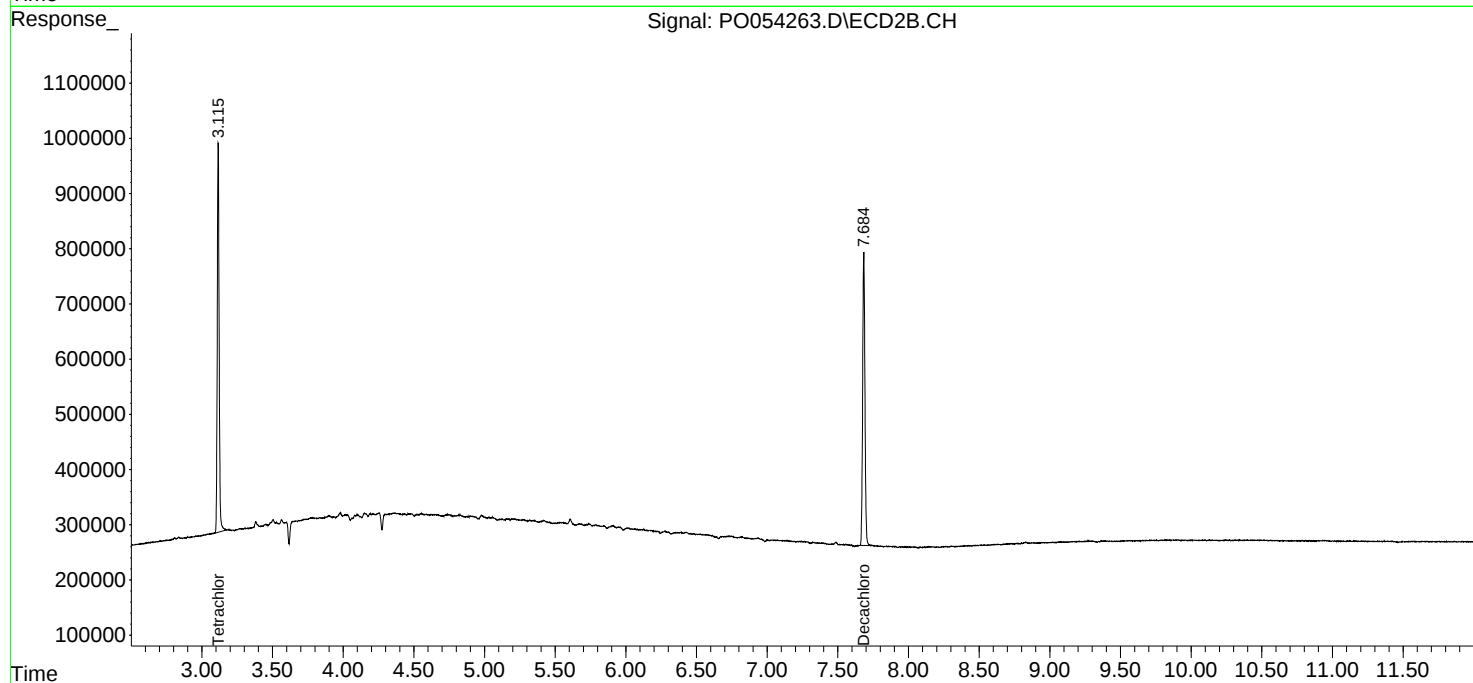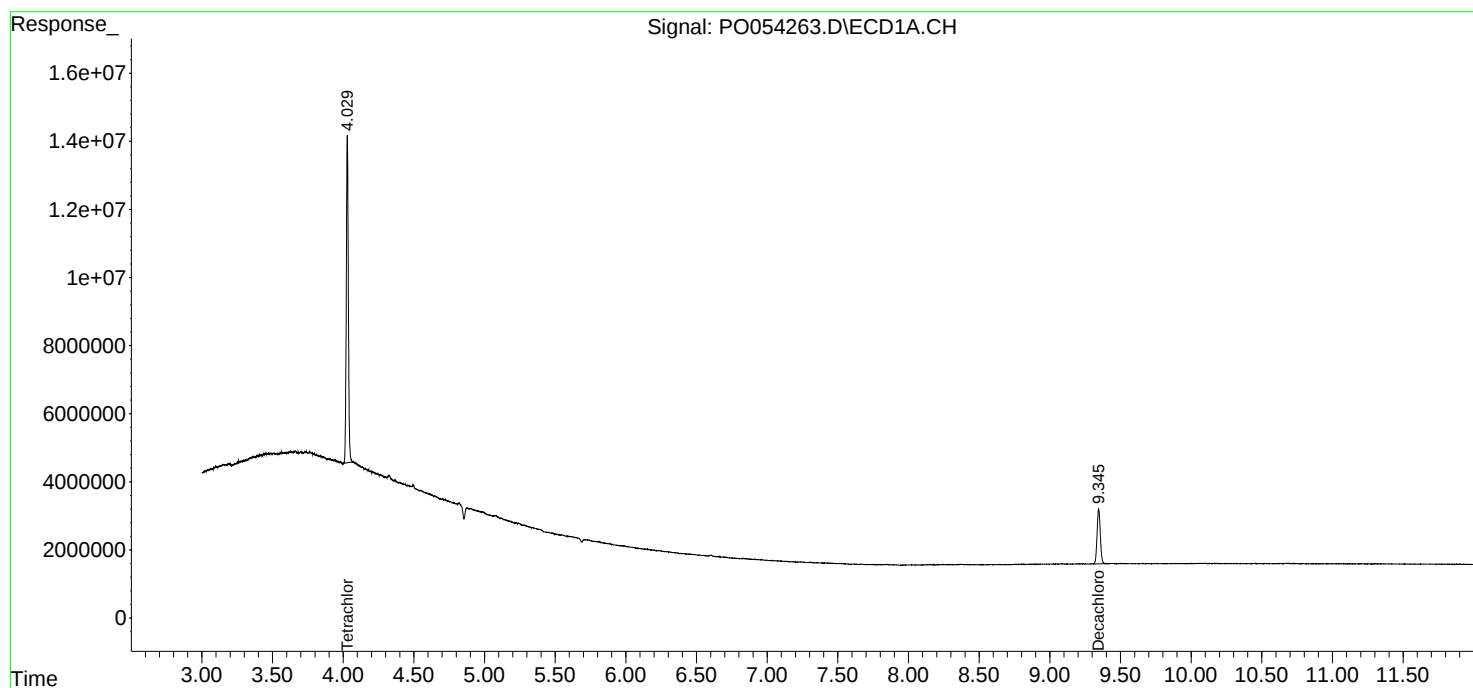


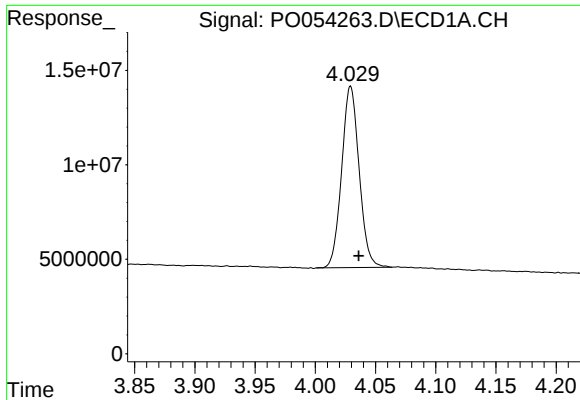

#1 Tetrachloro-m-xylene


R.T.: 4.029 min
Delta R.T.: -0.007 min
Response: 96984285
Conc: 17.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-07(22-23)-20190301

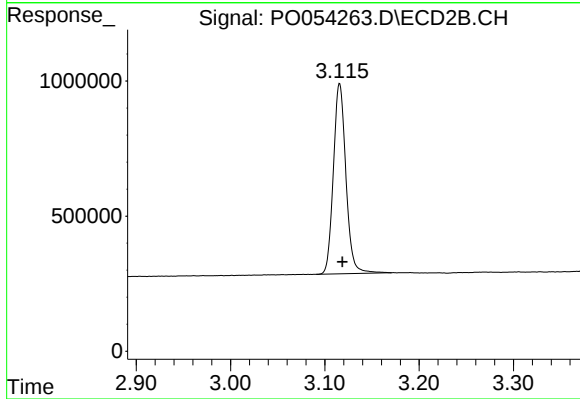


#1 Tetrachloro-m-xylene

R.T.: 3.116 min
Delta R.T.: -0.003 min
Response: 6510783
Conc: 20.72 ng/ml

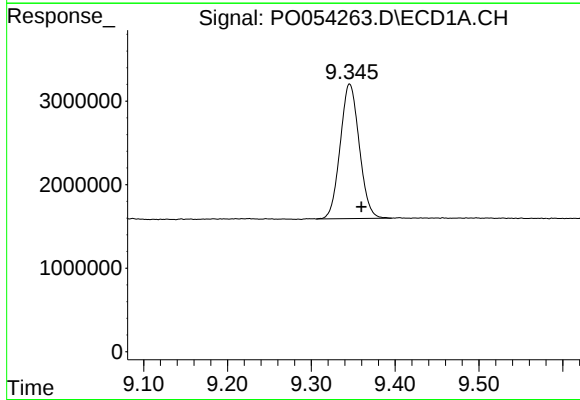

#2 Decachlorobiphenyl

R.T.: 9.346 min
Delta R.T.: -0.014 min
Response: 25453341
Conc: 17.14 ng/ml

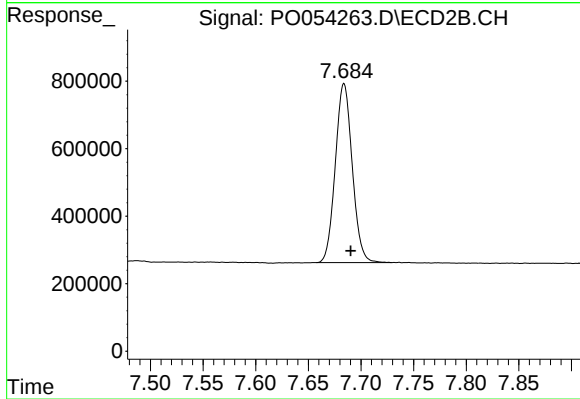

#2 Decachlorobiphenyl

R.T.: 7.684 min
Delta R.T.: -0.007 min
Response: 5940598
Conc: 18.57 ng/ml