

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030623\
 Data File : P0092999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 01:36
 Operator : YP/AJ
 Sample : 01803-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31906

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2023
 Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 03:31:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.637	32270391	18143171	10.747m	14.234m#
2) SA Decachlor...	10.265	8.669	20434684	7986194	10.624m	6.853m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030623\
Data File : PO092999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 01:36
Operator : YP/AJ
Sample : 01803-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31906


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 03:31:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

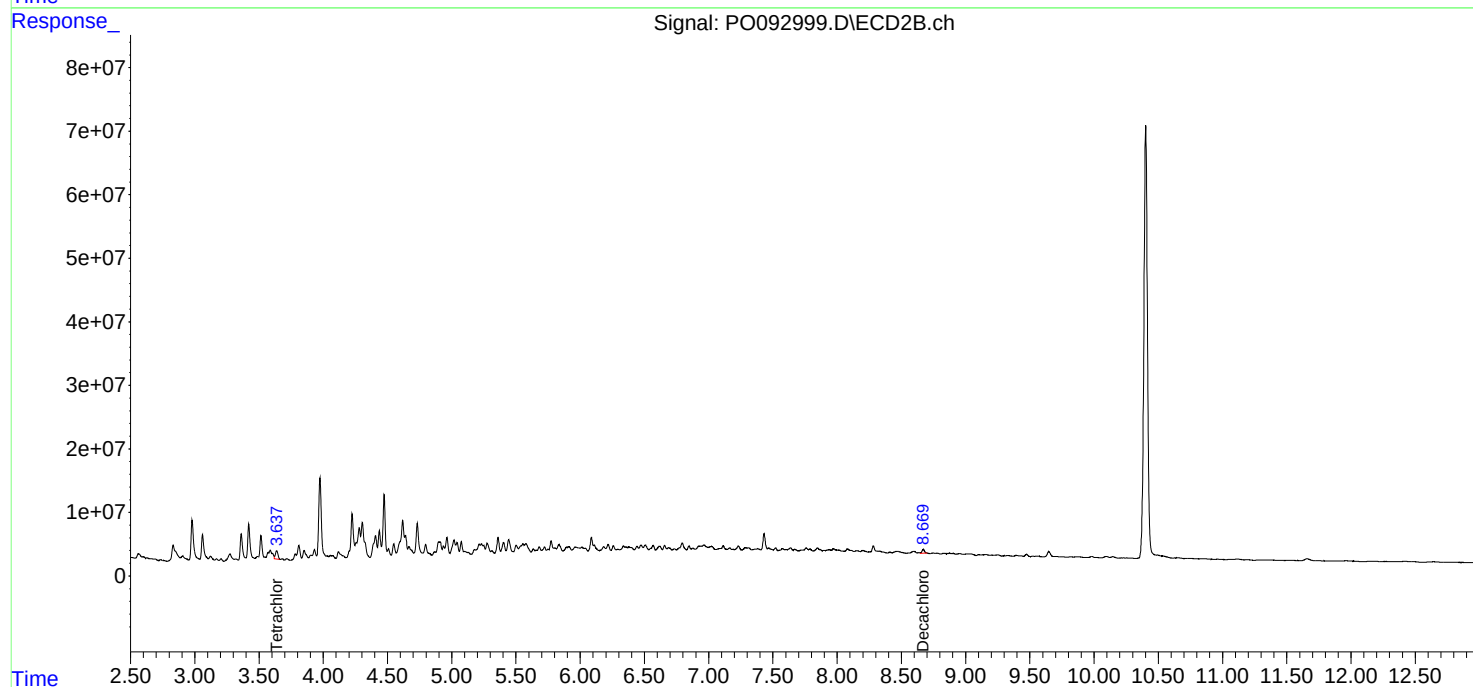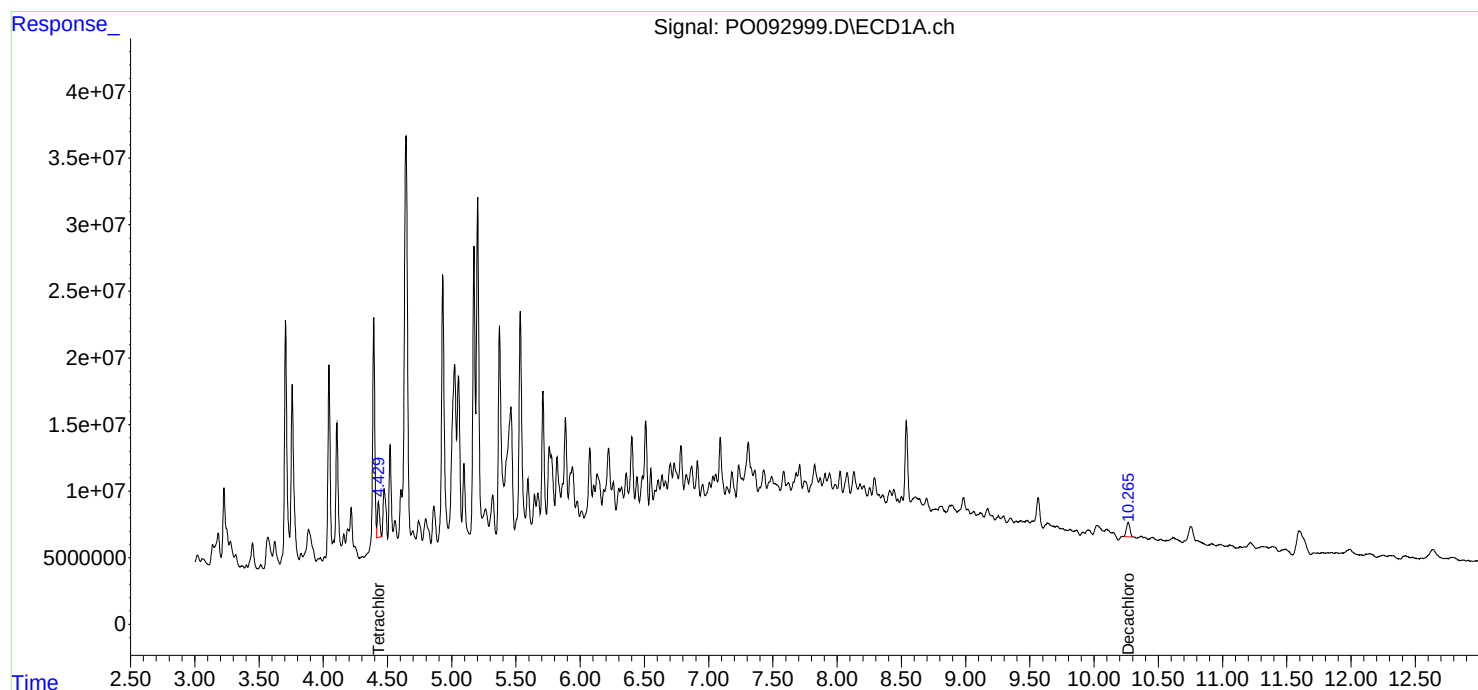

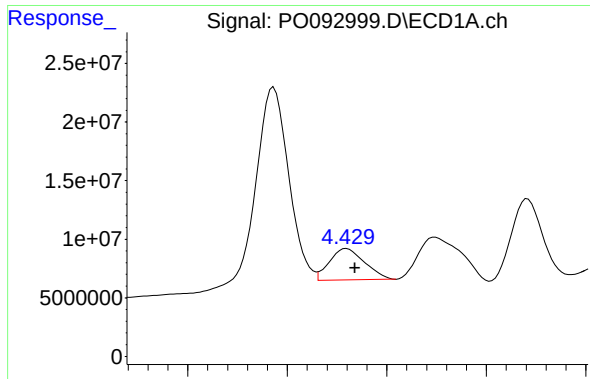


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: -0.005 min
Response: 32270391
Conc: 10.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
31906


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

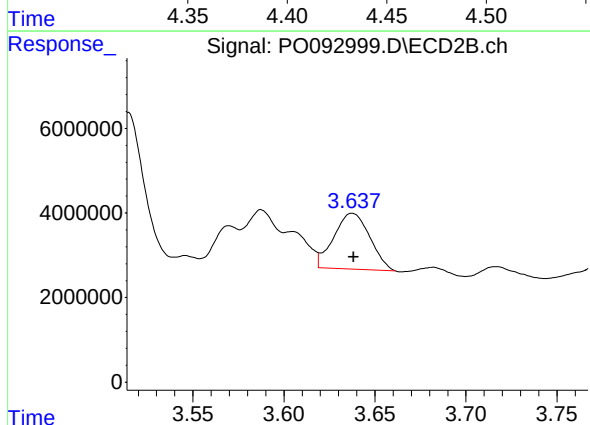


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.001 min
Response: 18143171
Conc: 14.23 ng/ml

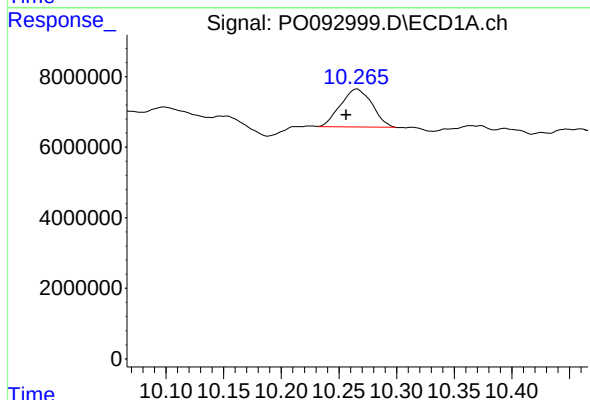

#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: 0.009 min
Response: 20434684
Conc: 10.62 ng/ml

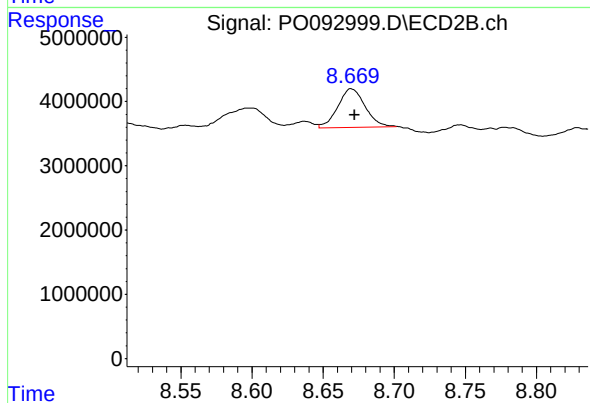

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 7986194
Conc: 6.85 ng/ml