

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030623\
 Data File : P0093001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 04:27
 Operator : YP/AJ
 Sample : 01816-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 91

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2023
 Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 05:02:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.437	3.634	42596082	19588323	14.186m	15.367
2) SA Decachlor...	10.282	8.670	27732220	13040473	14.418m	11.190m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030623\
Data File : PO093001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 04:27
Operator : YP/AJ
Sample : 01816-02
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
91


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 05:02:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

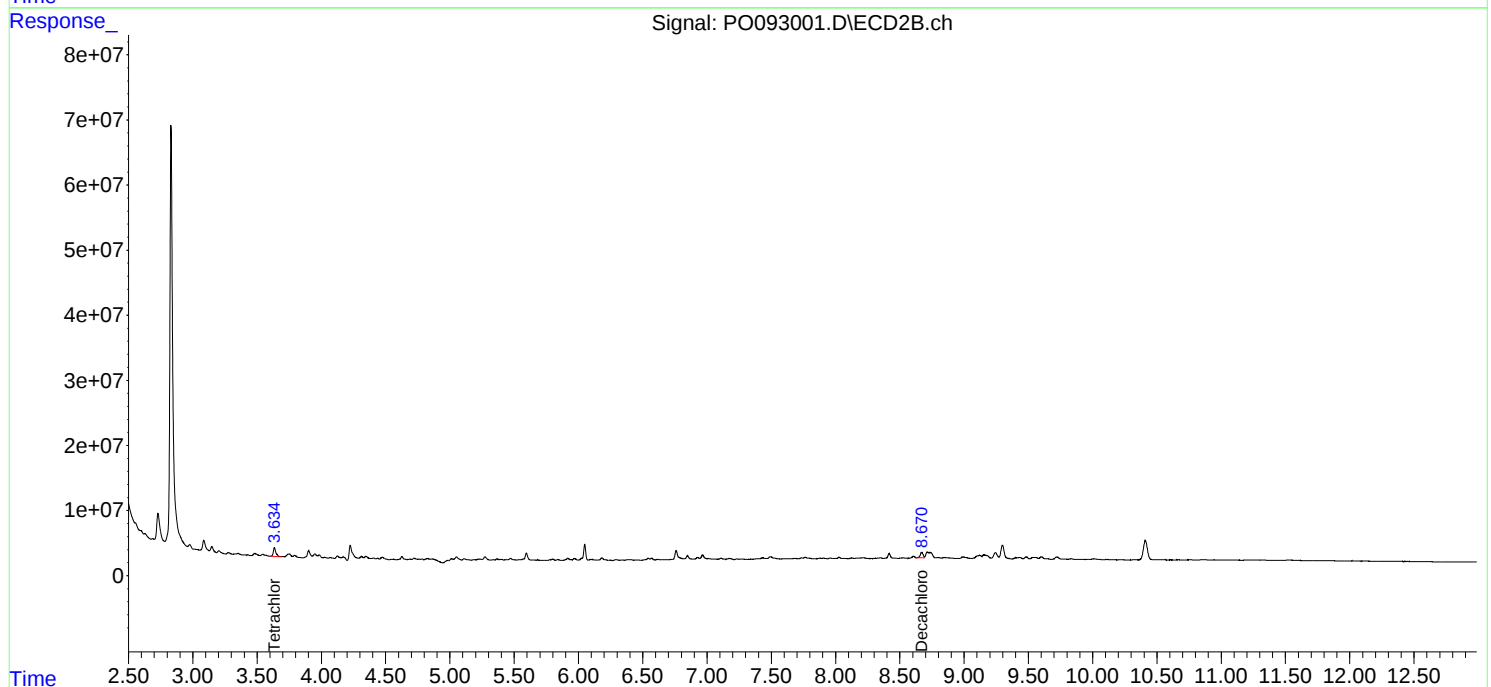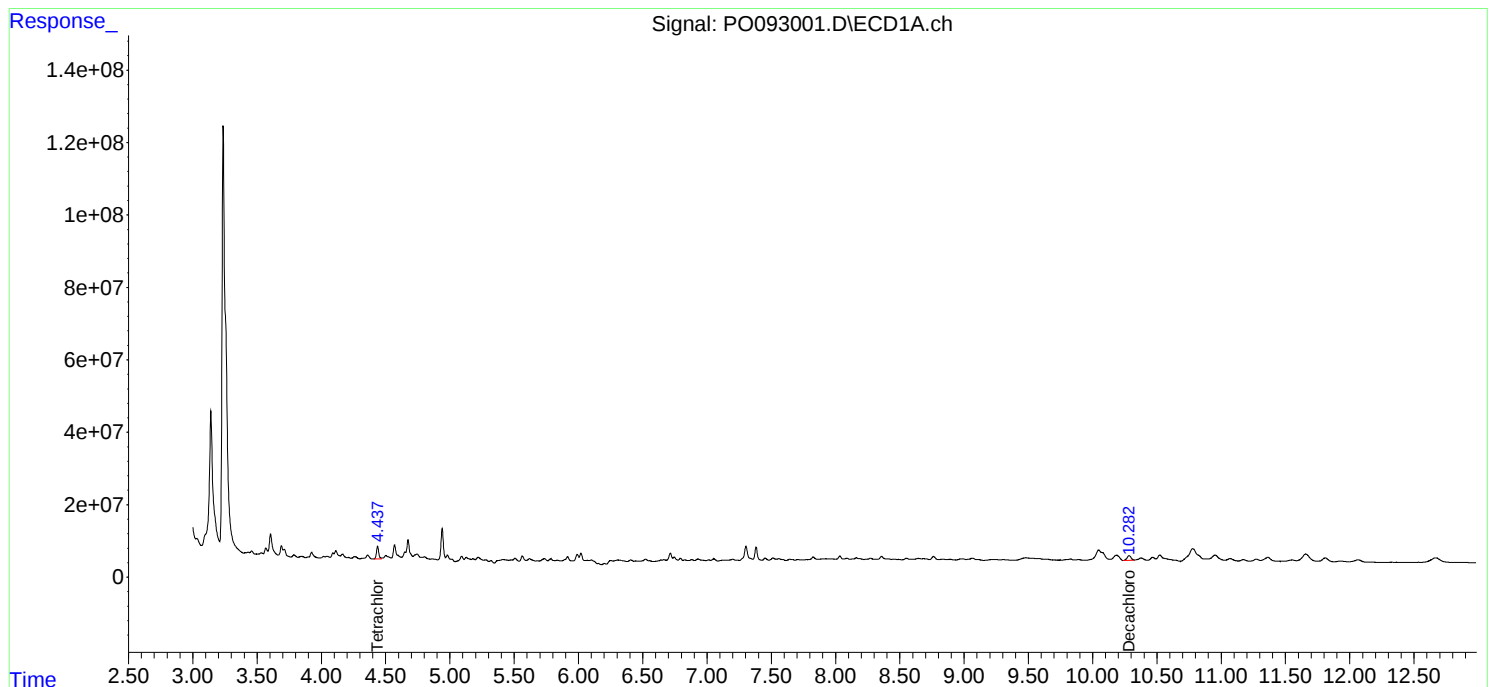

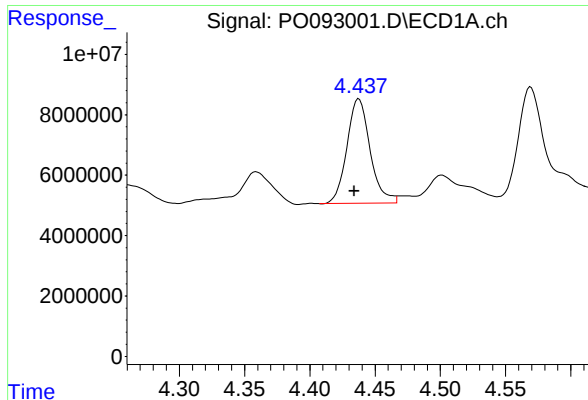


#1 Tetrachloro-m-xylene

R.T.: 4.437 min
Delta R.T.: 0.003 min
Response: 42596082
Conc: 14.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
91


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

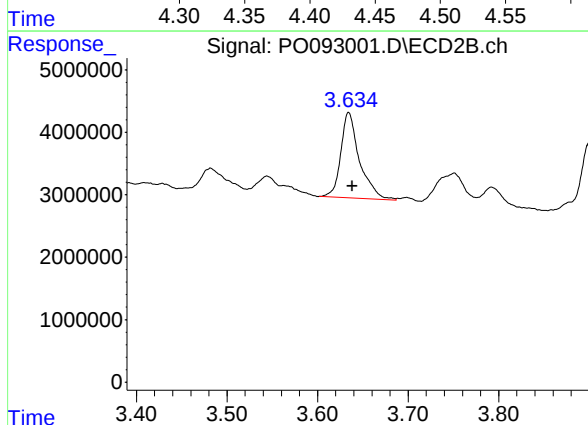


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 19588323
Conc: 15.37 ng/ml

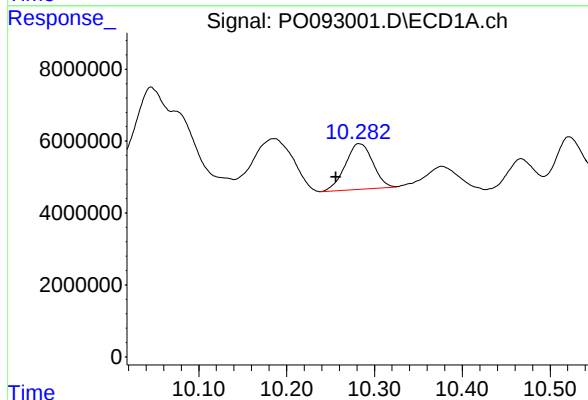

#2 Decachlorobiphenyl

R.T.: 10.282 min
Delta R.T.: 0.025 min
Response: 27732220
Conc: 14.42 ng/ml m

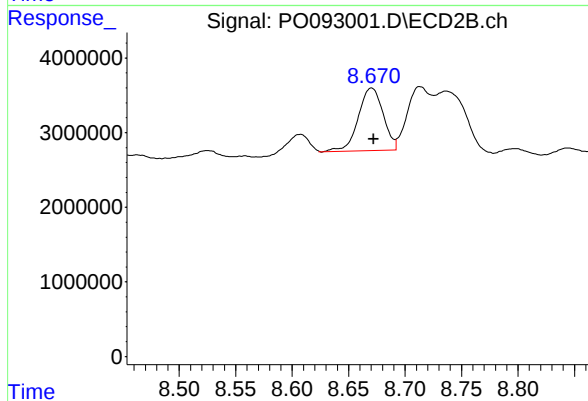

#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 13040473
Conc: 11.19 ng/ml m