

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030624\
 Data File : P0102368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2024 20:47
 Operator : YP/AJ
 Sample : P1682-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-04-03052024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2024
 Supervised By :Ankita Jodhani 03/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:53:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.387	75412237	51008294	16.261m	15.698m
2) SA Decachlor...	9.822	8.258	50118864	29228342	19.682m	14.128m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030624\
Data File : PO102368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 20:47
Operator : YP/AJ
Sample : P1682-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-04-03052024


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 03/07/2024
Supervised By : Ankita Jodhani 03/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:53:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

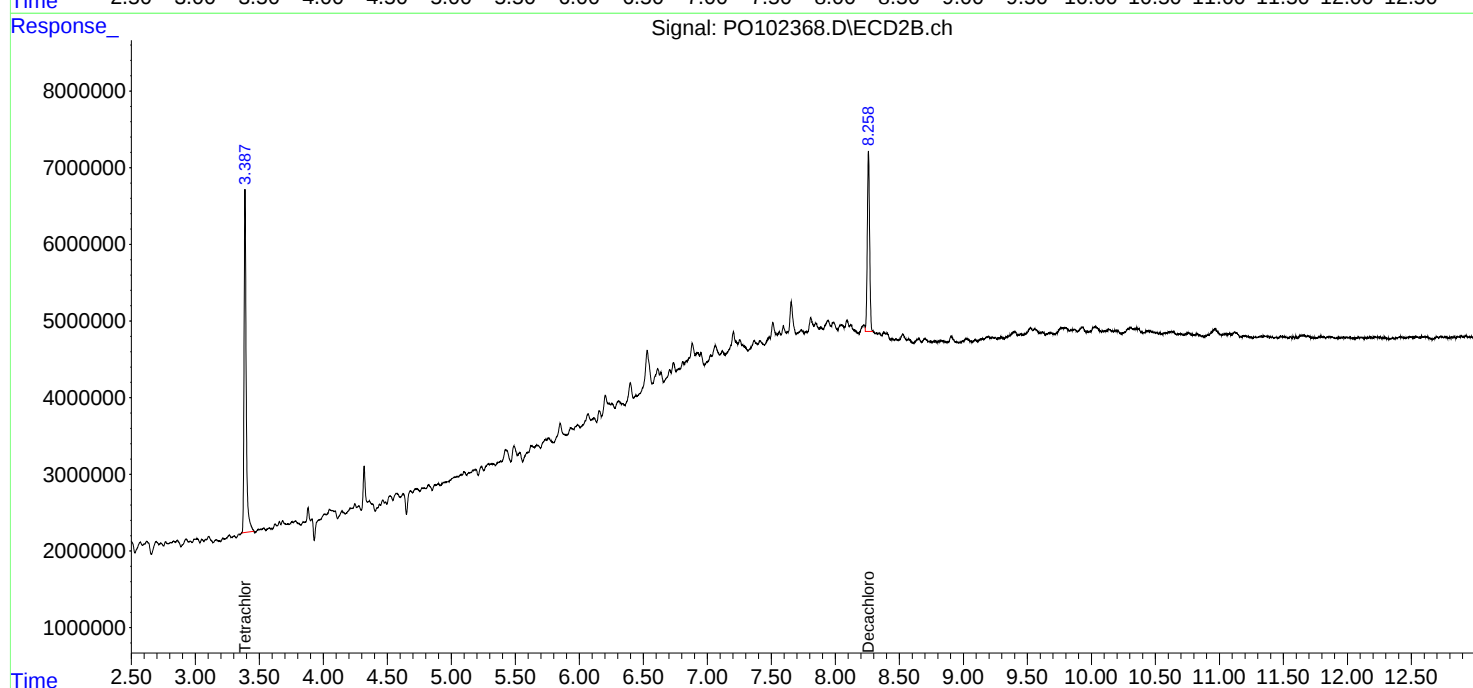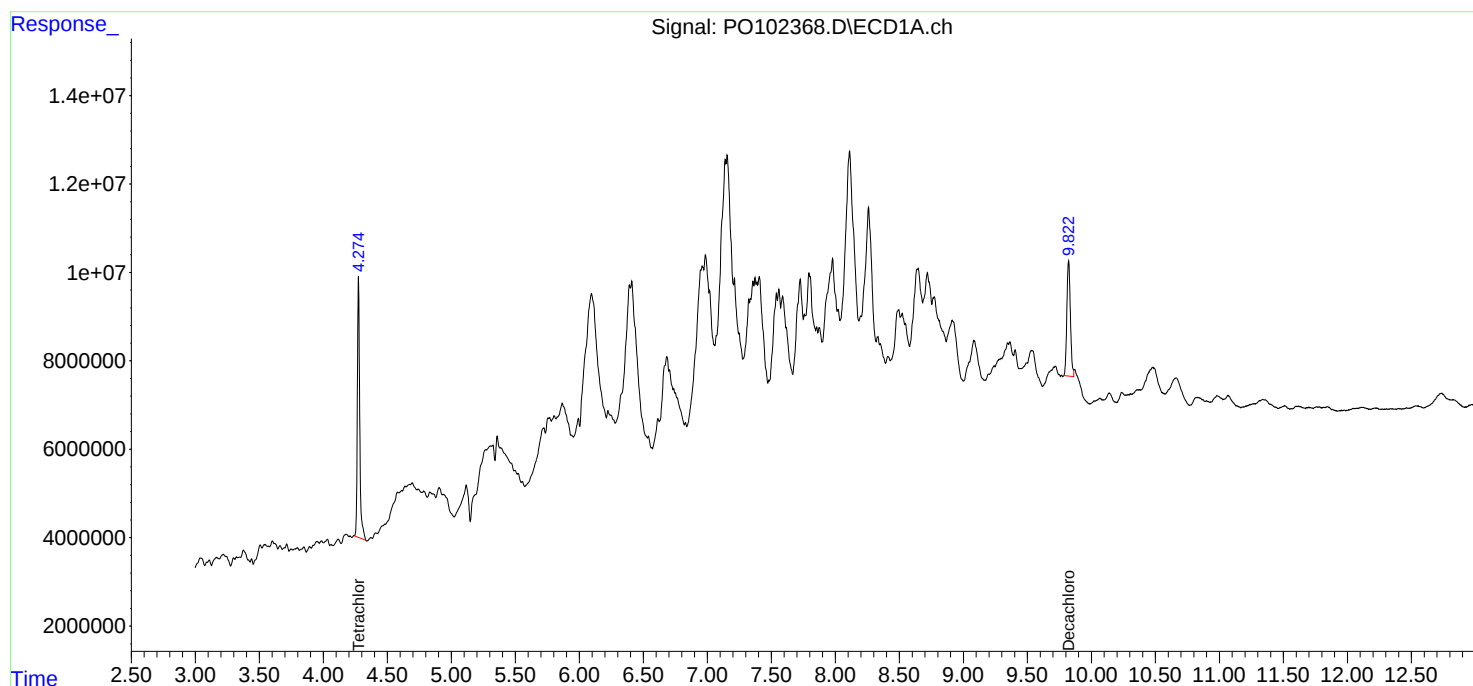

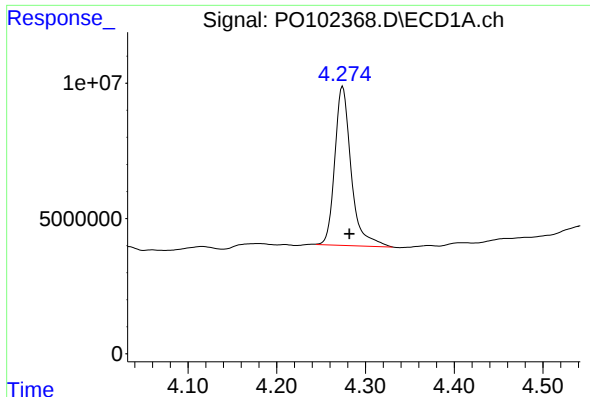


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.008 min
Response: 75412237
Conc: 16.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-04-03052024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2024
Supervised By :Ankita Jodhani 03/07/2024

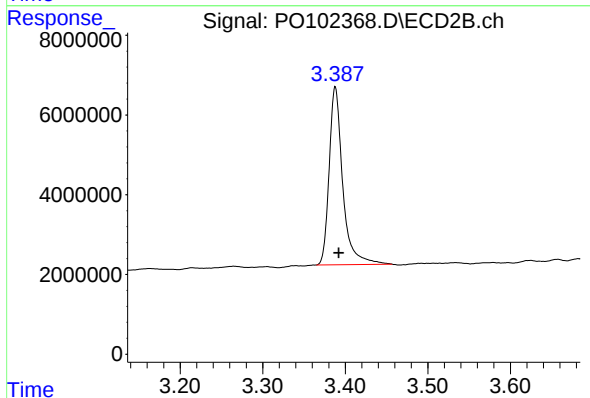


#1 Tetrachloro-m-xylene

R.T.: 3.387 min
Delta R.T.: -0.005 min
Response: 51008294
Conc: 15.70 ng/ml m

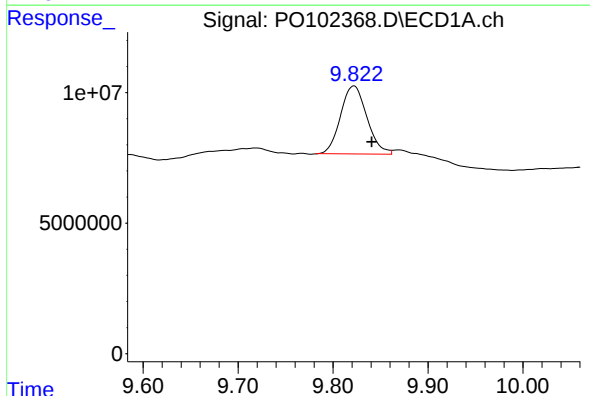

#2 Decachlorobiphenyl

R.T.: 9.822 min
Delta R.T.: -0.019 min
Response: 50118864
Conc: 19.68 ng/ml m

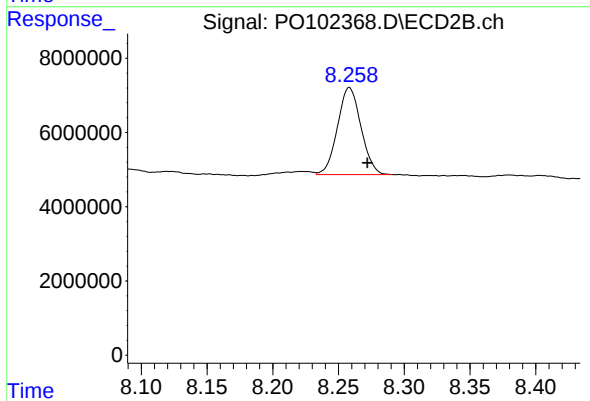

#2 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: -0.014 min
Response: 29228342
Conc: 14.13 ng/ml m