

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030723\
 Data File : P0093011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 10:08
 Operator : YP/AJ
 Sample : 01803-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1711

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/08/2023
 Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 14:46:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.634	40977057	18101480	13.646m	14.201m
2) SA Decachlor...	10.271	8.676	14603104	5268511	7.592	4.521m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030723\
Data File : PO093011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 10:08
Operator : YP/AJ
Sample : 01803-08
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1711


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 14:46:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

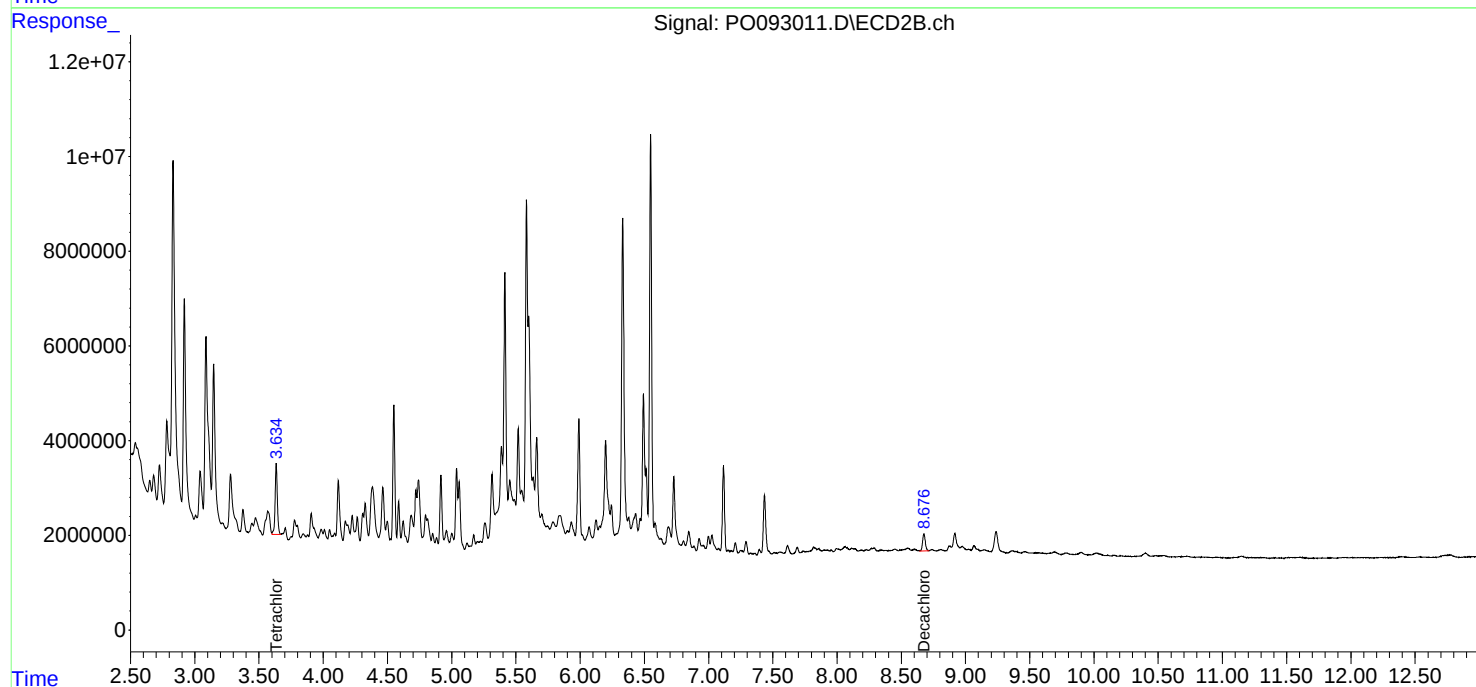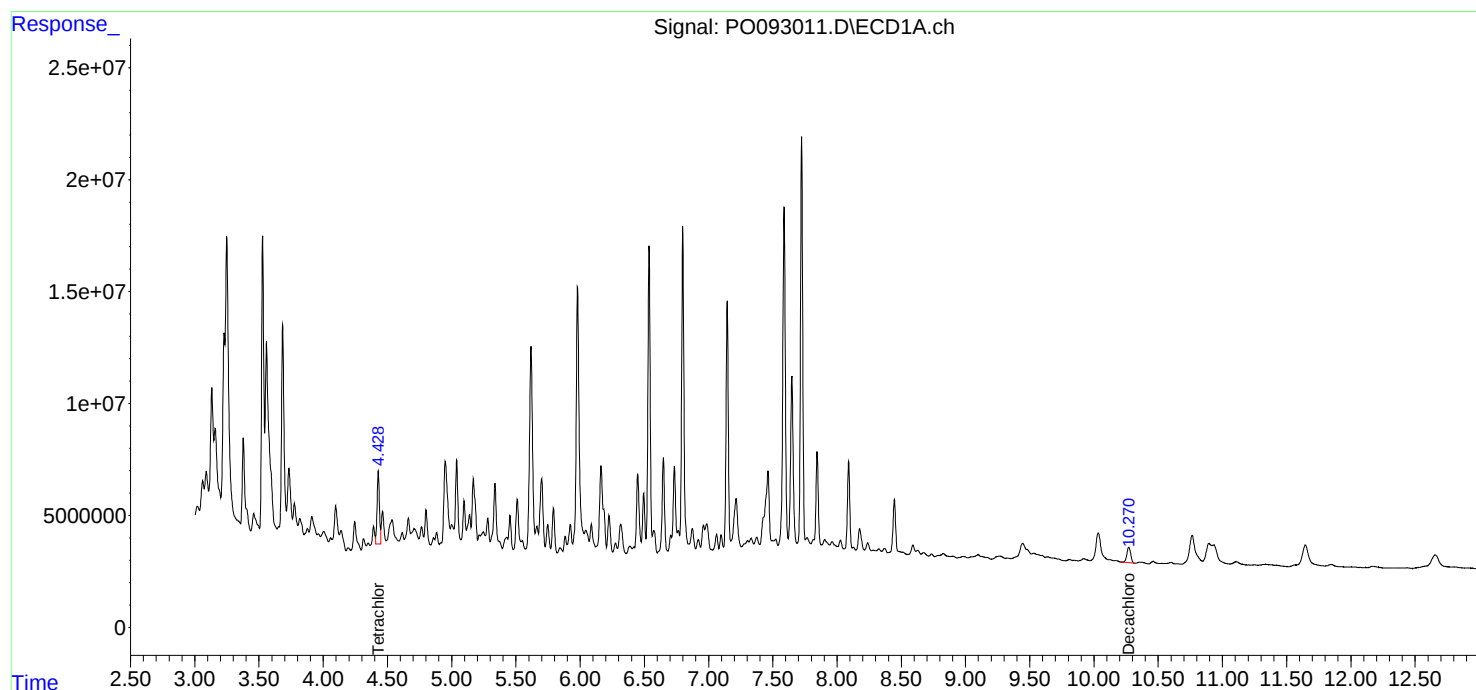

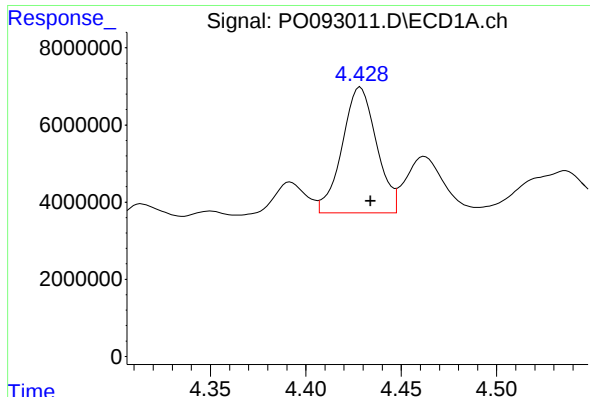


#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: -0.006 min
Response: 40977057
Conc: 13.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
1711


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

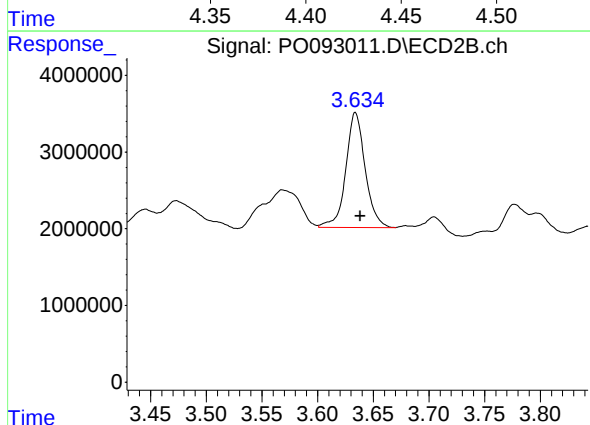


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.005 min
Response: 18101480
Conc: 14.20 ng/ml m

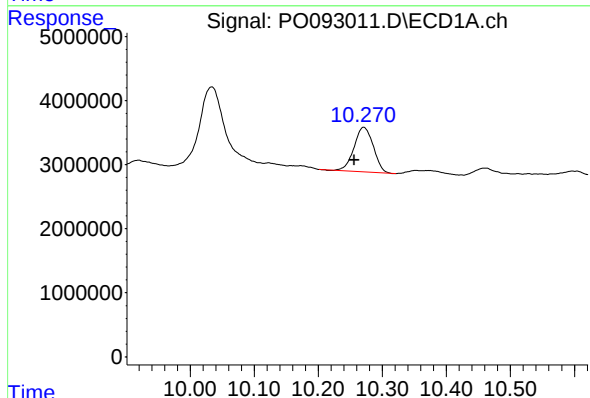

#2 Decachlorobiphenyl

R.T.: 10.271 min
Delta R.T.: 0.015 min
Response: 14603104
Conc: 7.59 ng/ml

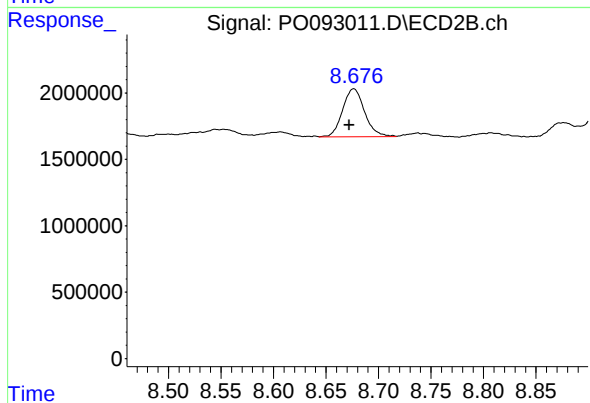

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: 0.004 min
Response: 5268511
Conc: 4.52 ng/ml m