

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030723\
 Data File : P0093021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 14:04
 Operator : YP/AJ
 Sample : 01821-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-IDW-S-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/08/2023
 Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 16:55:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.635	56227358	22040200	18.725m	17.291
2) SA Decachlor...	10.266	8.669	37071165	18453946	19.273	15.835

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030723\
Data File : PO093021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 14:04
Operator : YP/AJ
Sample : 01821-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-IDW-S-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 16:55:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

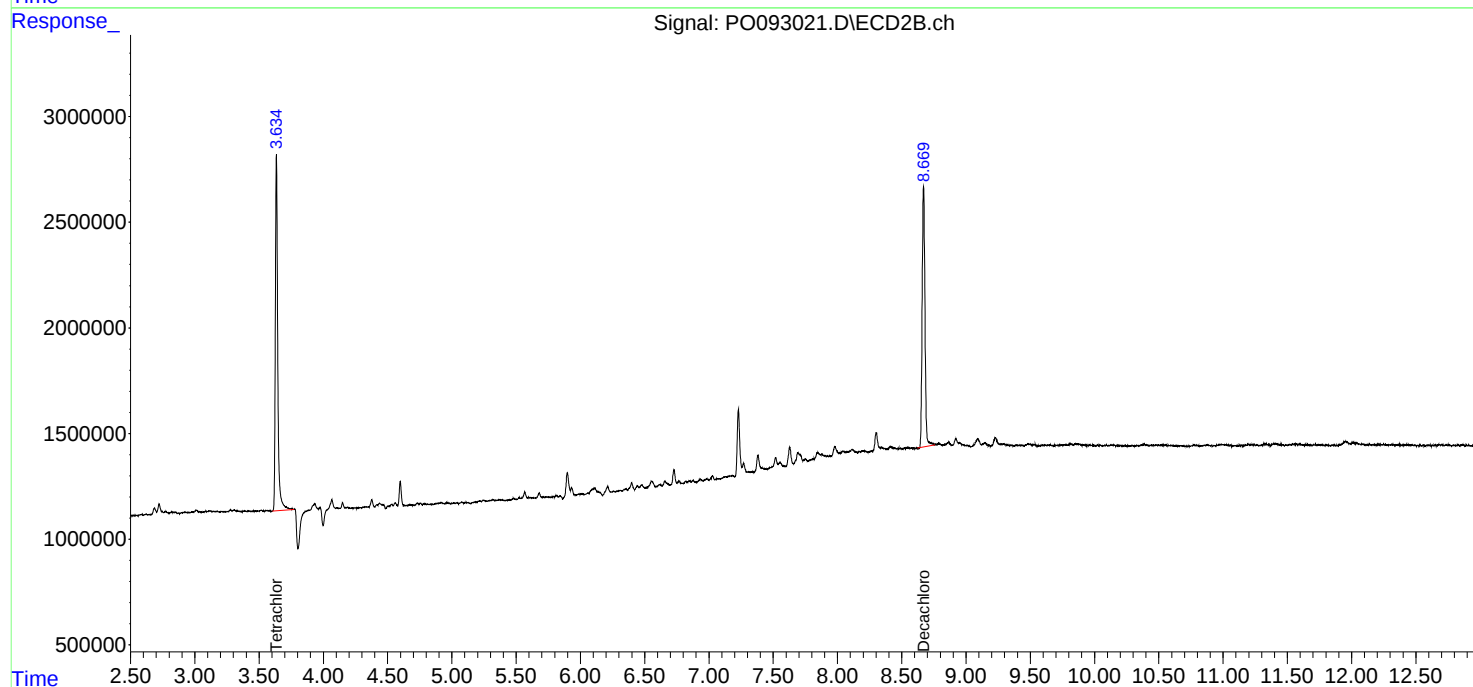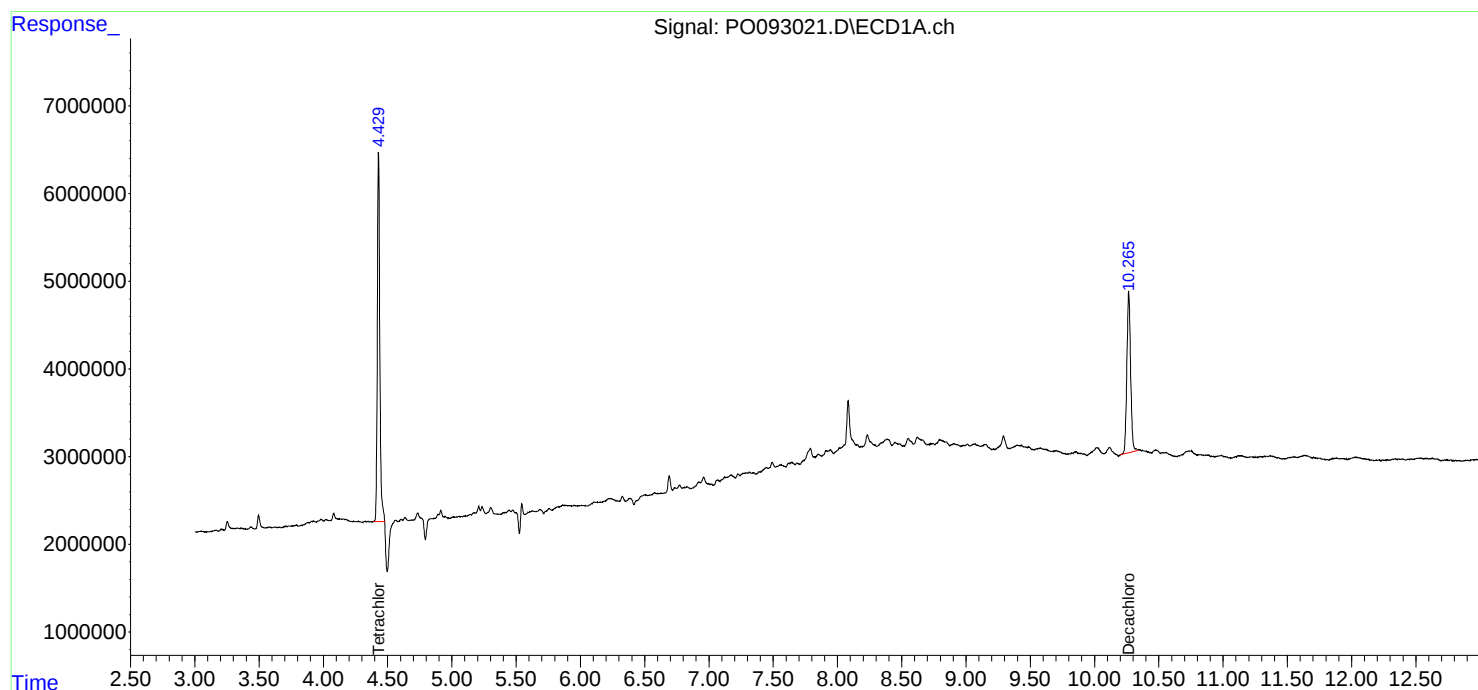

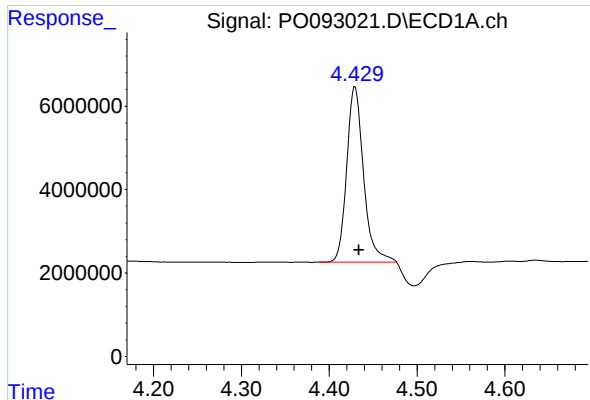


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: -0.005 min
Response: 56227358
Conc: 18.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-IDW-S-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

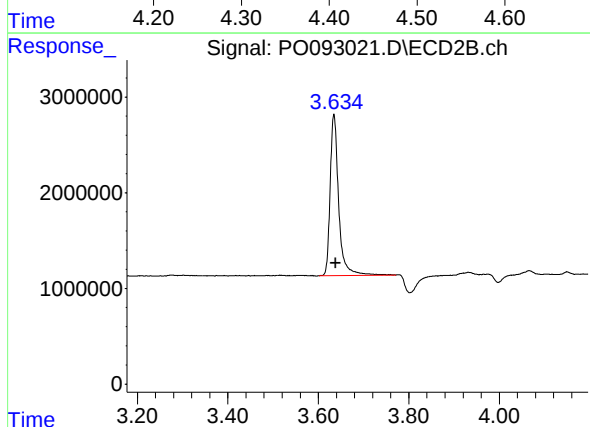


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.004 min
Response: 22040200
Conc: 17.29 ng/ml

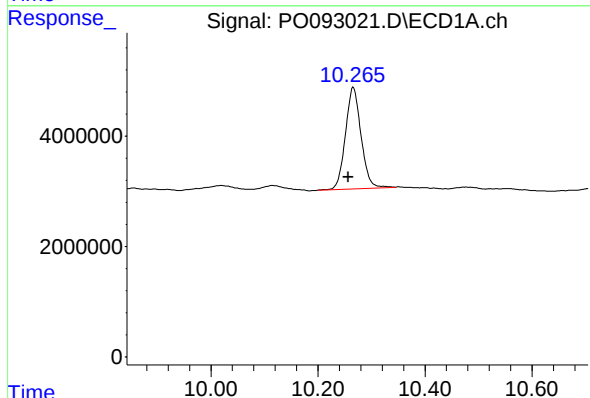

#2 Decachlorobiphenyl

R.T.: 10.266 min
Delta R.T.: 0.009 min
Response: 37071165
Conc: 19.27 ng/ml

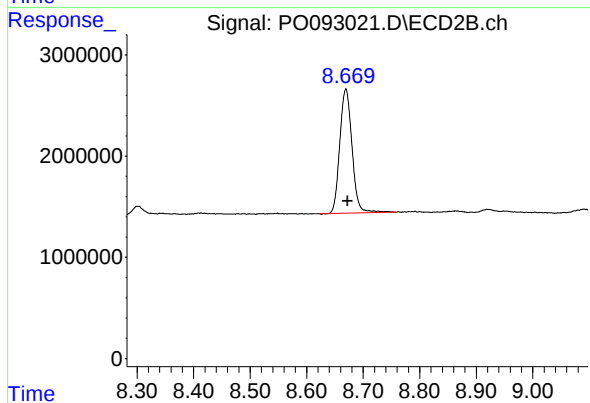

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 18453946
Conc: 15.83 ng/ml