

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030723\
 Data File : P0093024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 14:56
 Operator : YP/AJ
 Sample : 01825-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HH-TP3-0306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/08/2023
 Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 16:55:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.634	63536042	24242250	21.159	19.018
2) SA Decachlor...	10.267	8.669	38422329	18782163	19.975	16.116
Target Compounds						
21) L5 AR-1248-1	5.610	4.725	1713548	586190	27.953m	22.387m
22) L5 AR-1248-2	5.883	4.958	4728700	2189647	49.135	54.121
23) L5 AR-1248-3	6.089	4.999	8979651	2865863	87.506	67.999
24) L5 AR-1248-4	6.496	5.171	8772913	4417396	87.660	91.452
25) L5 AR-1248-5	6.534	5.565	20199686	8251734	199.545	197.709

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030723\
Data File : PO093024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 14:56
Operator : YP/AJ
Sample : 01825-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HH-TP3-0306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 16:55:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

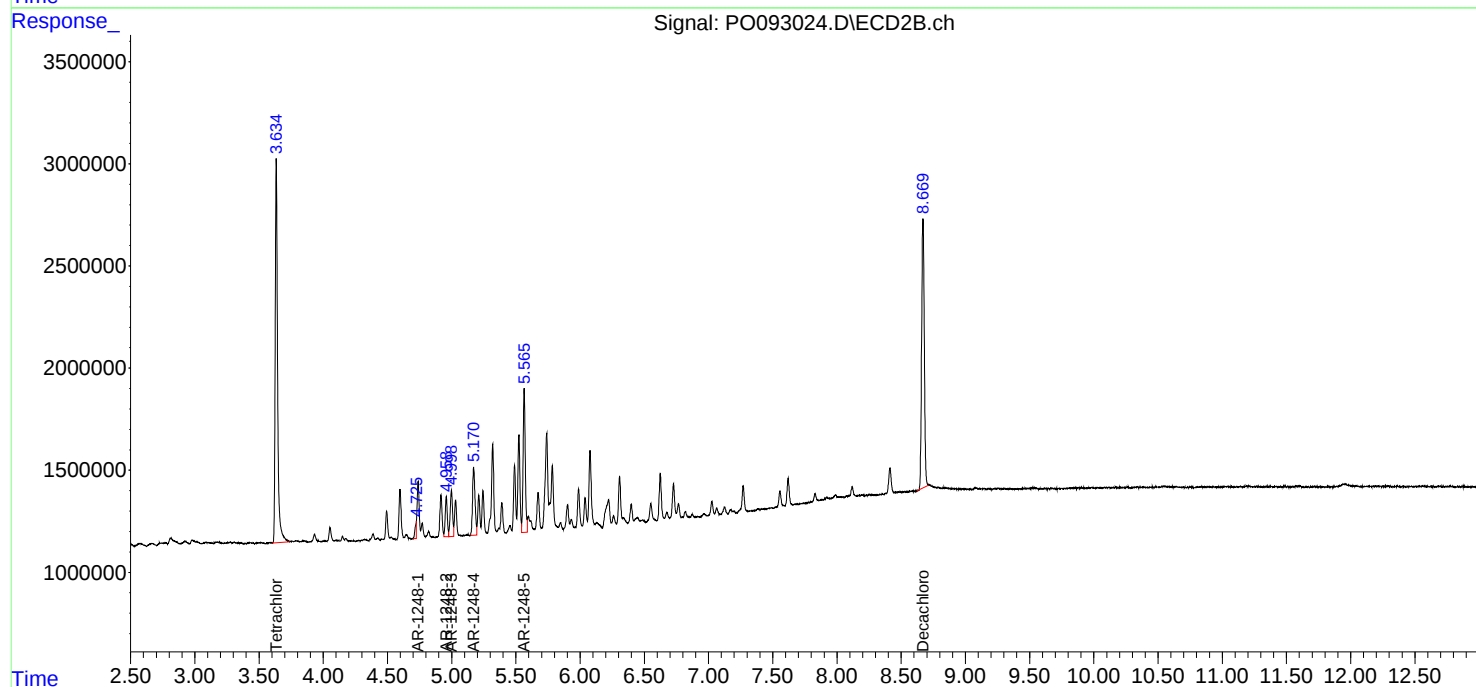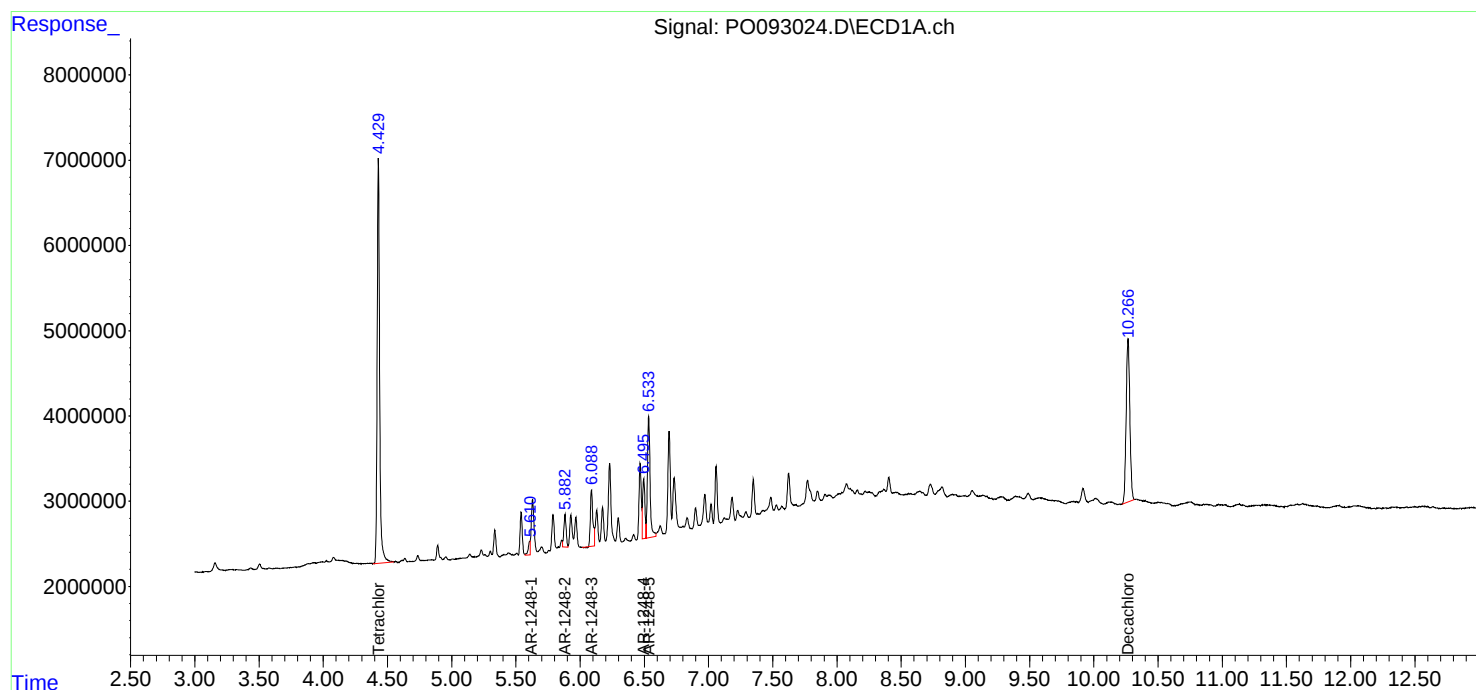

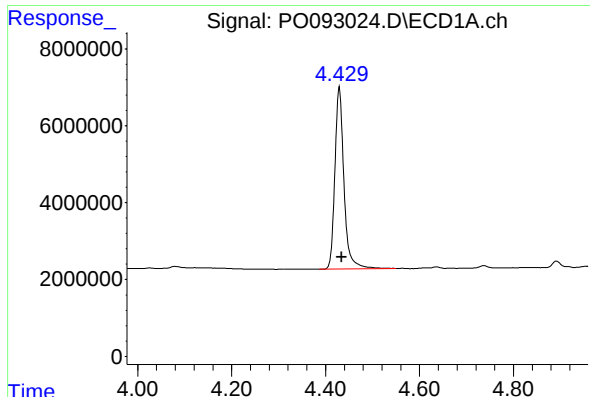


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: -0.005 min
Response: 63536042
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
HH-TP3-0306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

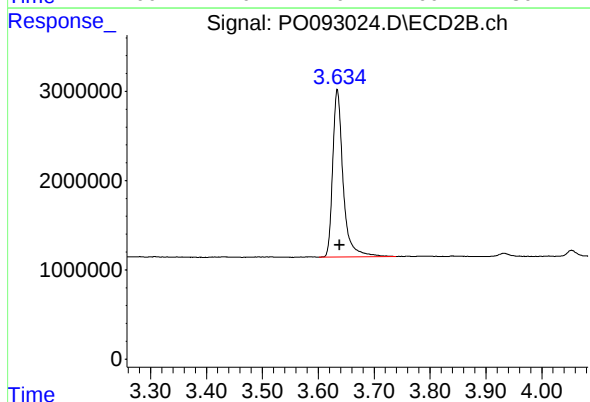


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 24242250
Conc: 19.02 ng/ml

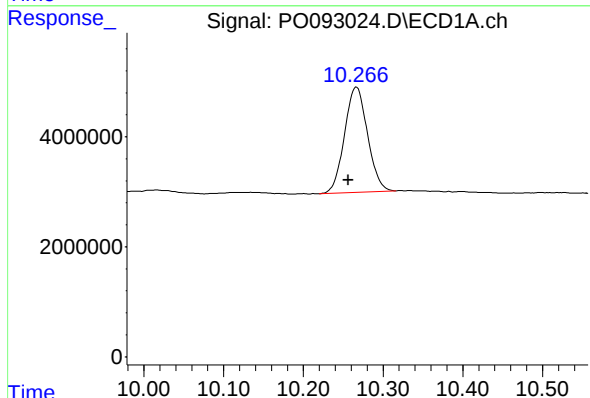


#2 Decachlorobiphenyl

R.T.: 10.267 min
Delta R.T.: 0.010 min
Response: 38422329
Conc: 19.98 ng/ml

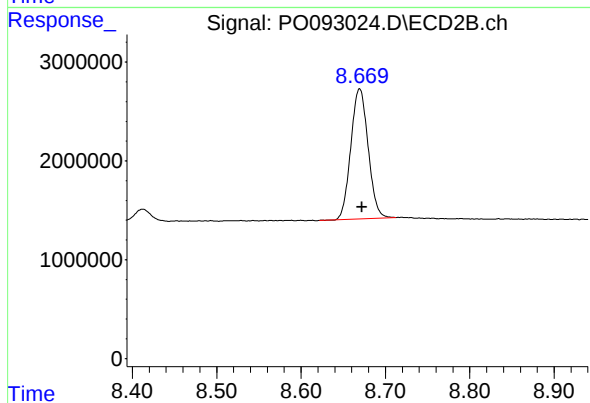

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 18782163
Conc: 16.12 ng/ml

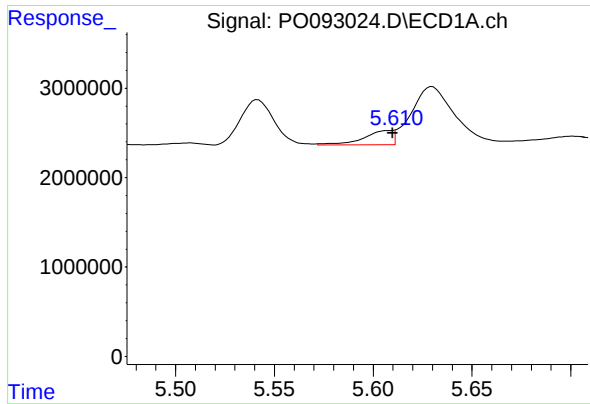


#21 AR-1248-1

R.T.: 5.610 min
Delta R.T.: 0.000 min
Response: 1713548
Conc: 27.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
HH-TP3-0306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

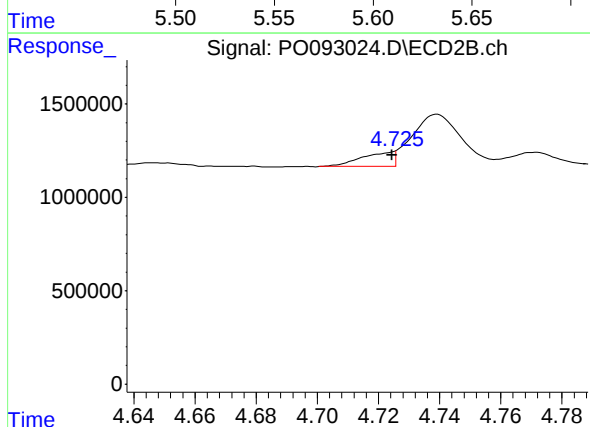


#21 AR-1248-1

R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 586190
Conc: 22.39 ng/ml

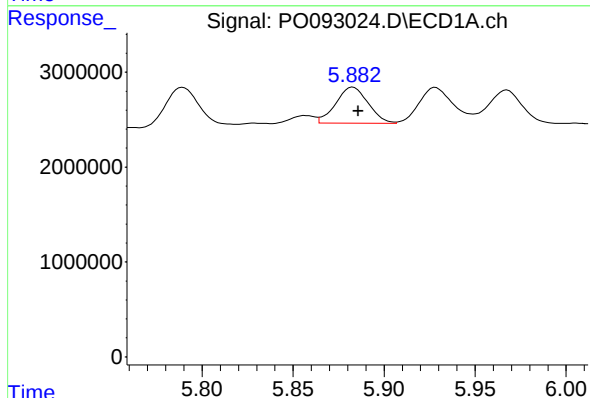


#22 AR-1248-2

R.T.: 5.883 min
Delta R.T.: -0.003 min
Response: 4728700
Conc: 49.14 ng/ml

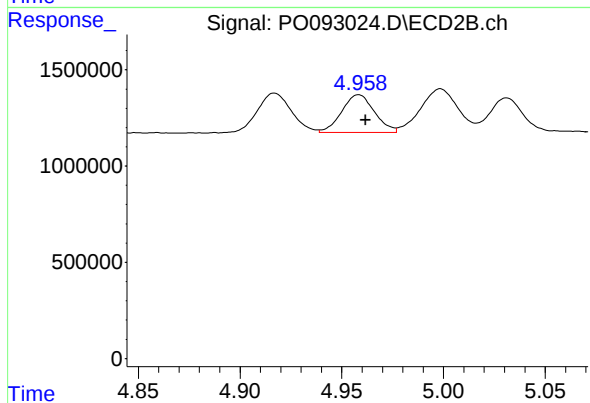

#22 AR-1248-2

R.T.: 4.958 min
Delta R.T.: -0.003 min
Response: 2189647
Conc: 54.12 ng/ml

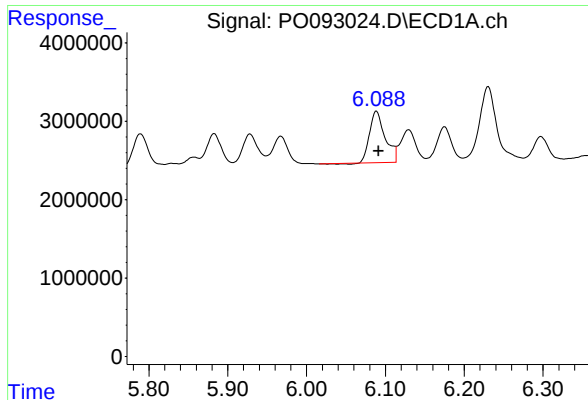


#23 AR-1248-3

R.T.: 6.089 min
Delta R.T.: -0.003 min
Response: 8979651
Conc: 87.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
HH-TP3-0306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

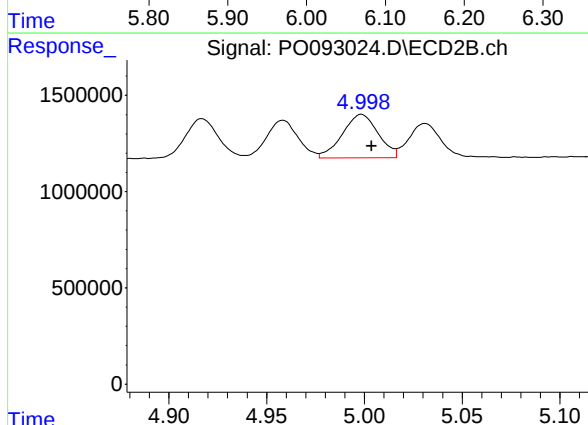


#23 AR-1248-3

R.T.: 4.999 min
Delta R.T.: -0.005 min
Response: 2865863
Conc: 68.00 ng/ml

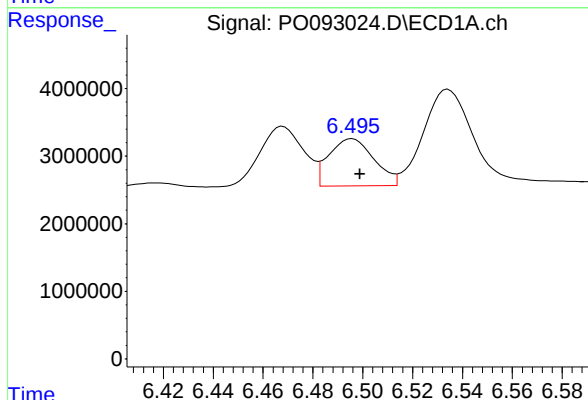


#24 AR-1248-4

R.T.: 6.496 min
Delta R.T.: -0.003 min
Response: 8772913
Conc: 87.66 ng/ml

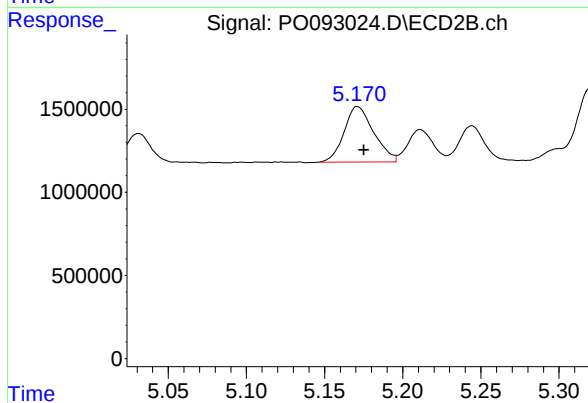

#24 AR-1248-4

R.T.: 5.171 min
Delta R.T.: -0.004 min
Response: 4417396
Conc: 91.45 ng/ml

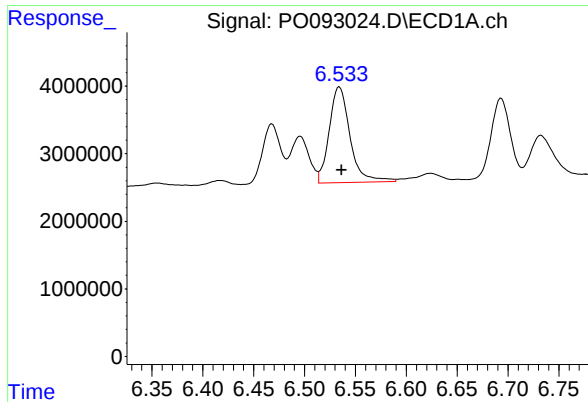


#25 AR-1248-5

R.T.: 6.534 min
Delta R.T.: -0.002 min
Response: 20199686
Conc: 199.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
HH-TP3-0306

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

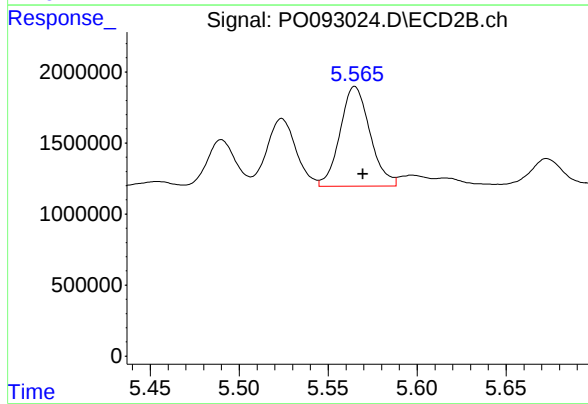

#25 AR-1248-5

R.T.: 5.565 min
Delta R.T.: -0.004 min
Response: 8251734
Conc: 197.71 ng/ml