

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030723\
 Data File : P0093026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 15:30
 Operator : YP/AJ
 Sample : 01826-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MMC-CON-0306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/08/2023
 Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 16:56:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.633	60325803	23264100	20.090	18.251m
2) SA Decachlor...	10.266	8.669	42103870	20799963	21.889	17.848

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030723\
Data File : PO093026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 15:30
Operator : YP/AJ
Sample : 01826-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MMC-CON-0306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 16:56:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

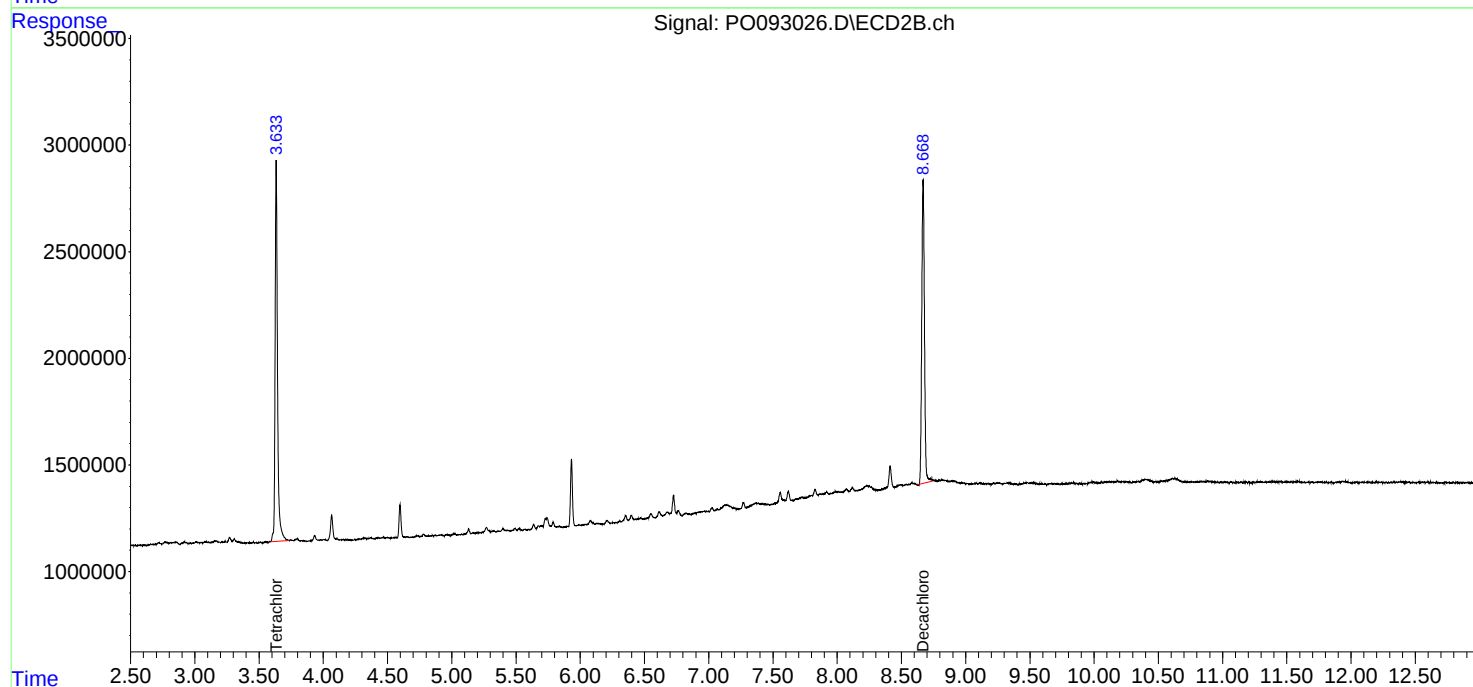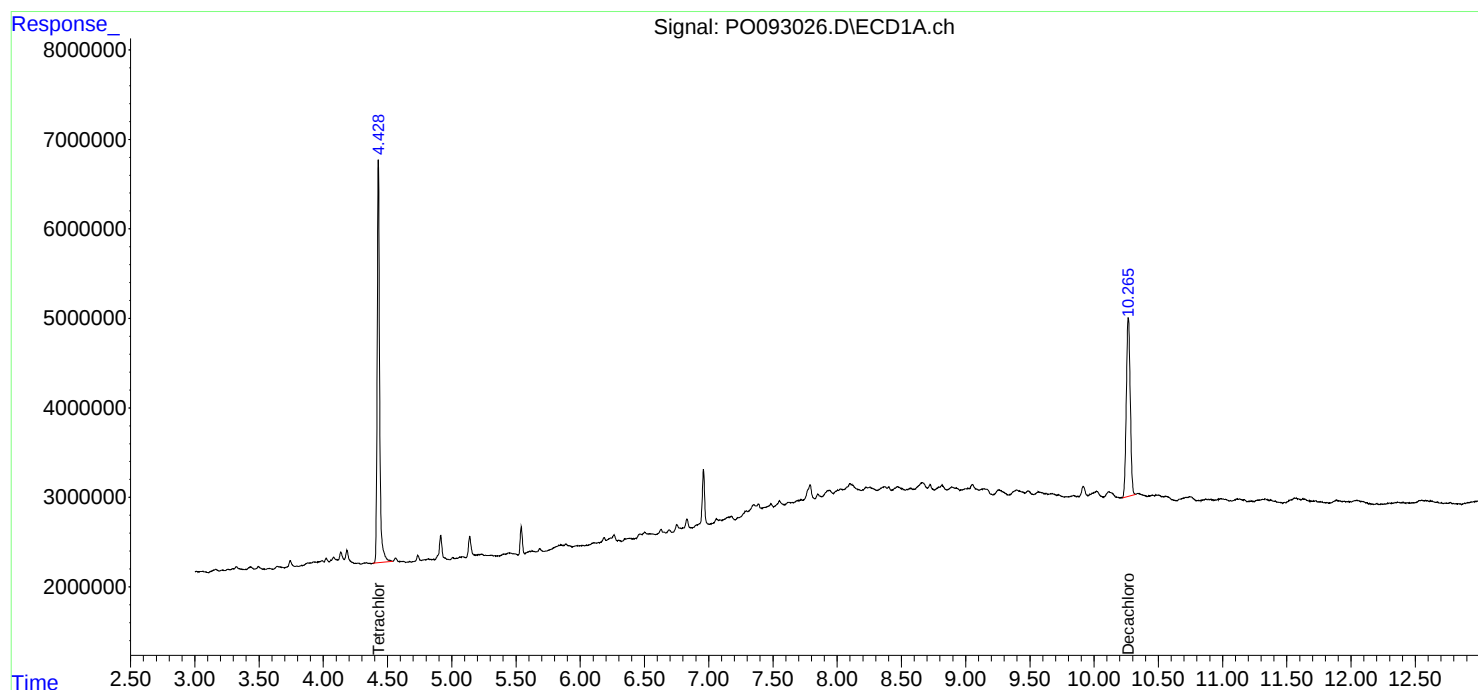

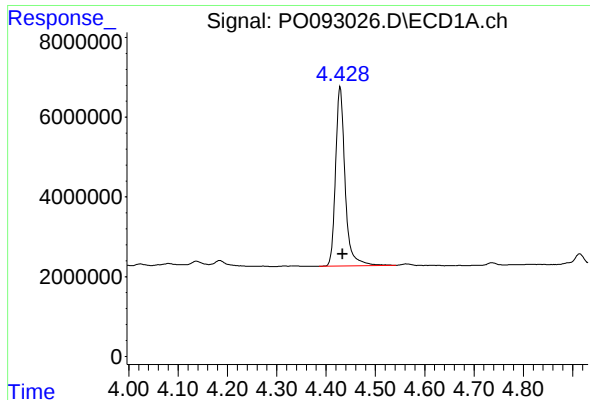


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: -0.005 min
Response: 60325803
Conc: 20.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MMC-CON-0306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

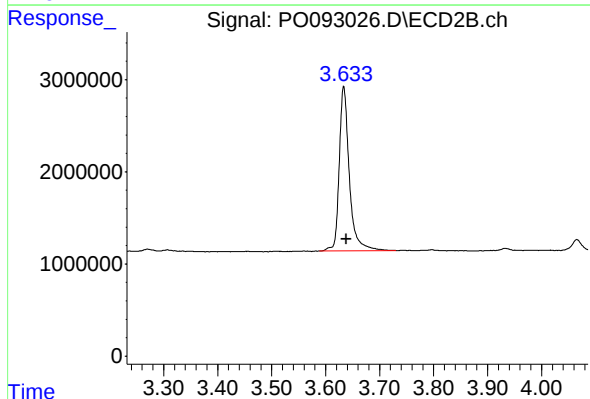


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.005 min
Response: 23264100
Conc: 18.25 ng/ml m

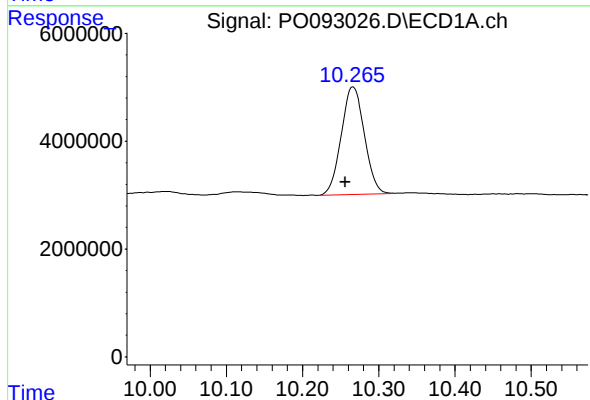

#2 Decachlorobiphenyl

R.T.: 10.266 min
Delta R.T.: 0.010 min
Response: 42103870
Conc: 21.89 ng/ml

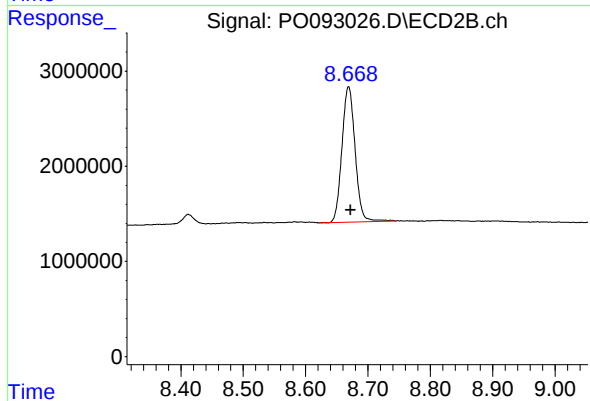

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 20799963
Conc: 17.85 ng/ml