

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030724\
 Data File : P0102395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2024 19:52
 Operator : YP/AJ
 Sample : P1688-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/08/2024
 Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 21:59:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.273	3.386	96355919	60719631	20.777	18.686m
2) SA Decachlor...	9.816	8.254	44801855	29250665	17.594	14.139m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030724\
Data File : PO102395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2024 19:52
Operator : YP/AJ
Sample : P1688-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/08/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 21:59:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

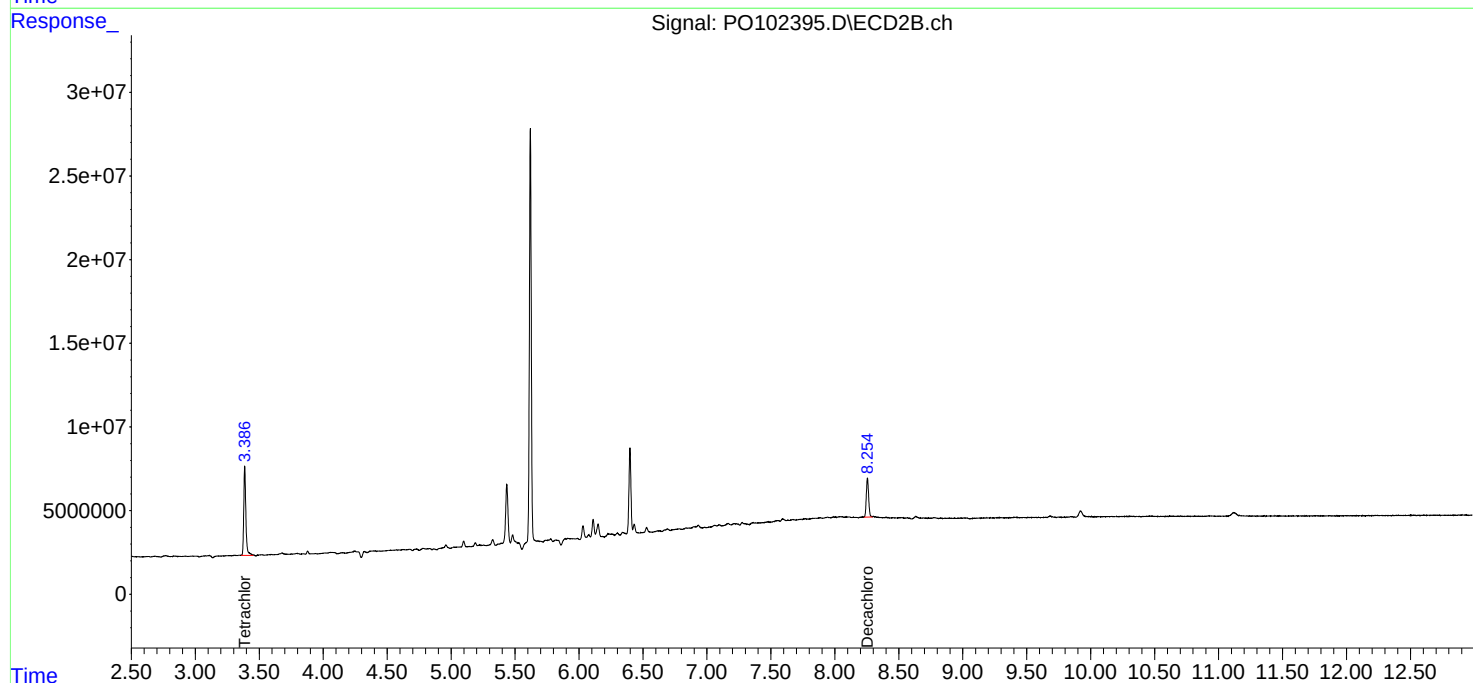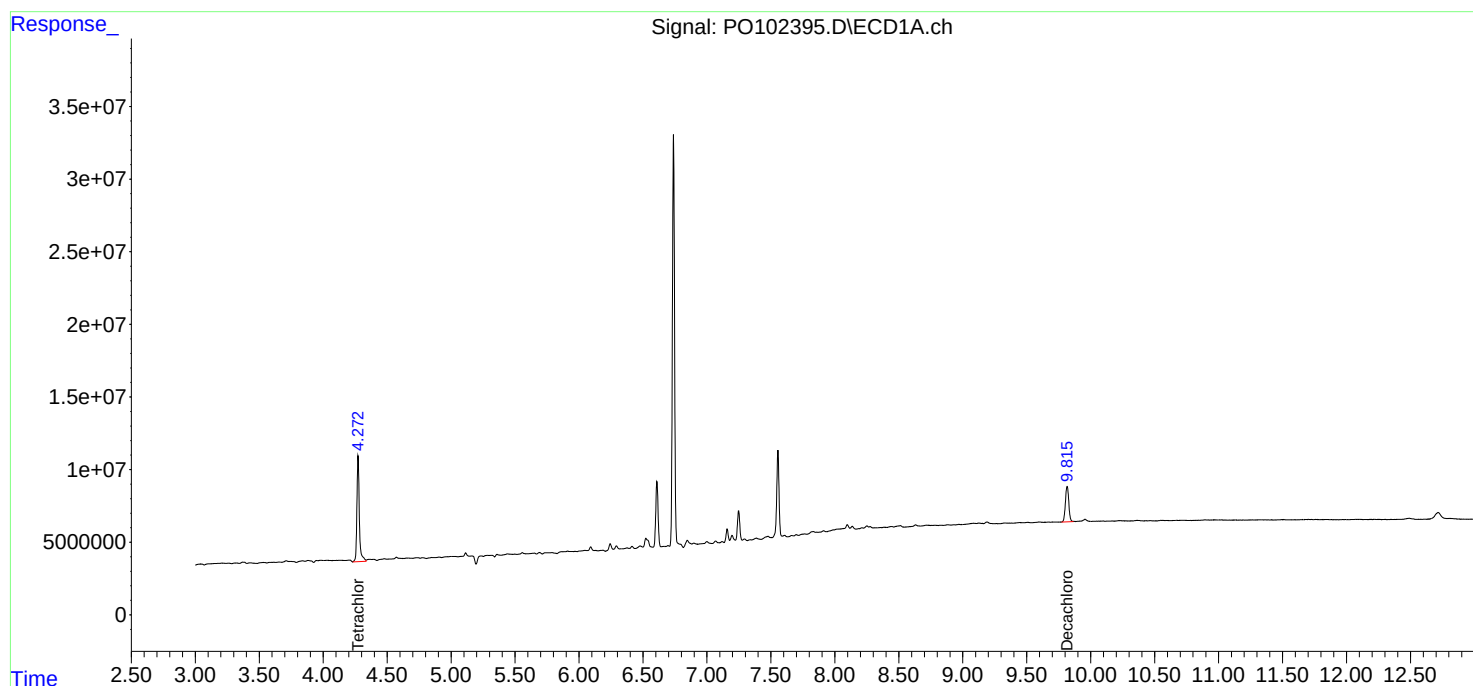

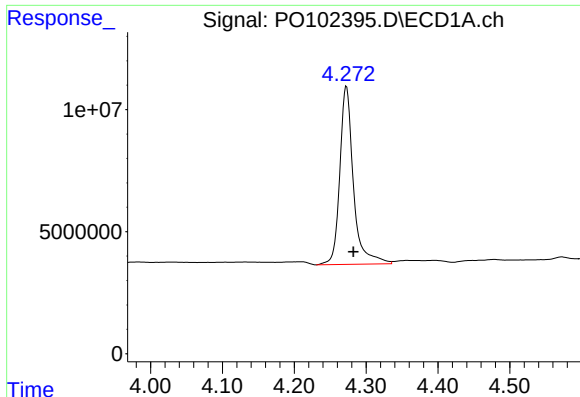

#1 Tetrachloro-m-xylene

R.T.: 4.273 min
Delta R.T.: -0.009 min
Response: 96355919
Conc: 20.78 ng/ml

Instrument :

ECD_O


ClientSampleId :

COMP-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 03/08/2024
Supervised By :Ankita Jodhani 03/08/2024

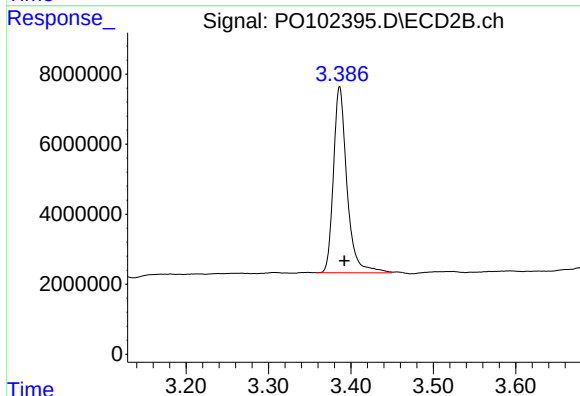


#1 Tetrachloro-m-xylene

R.T.: 3.386 min
Delta R.T.: -0.006 min
Response: 60719631
Conc: 18.69 ng/ml m

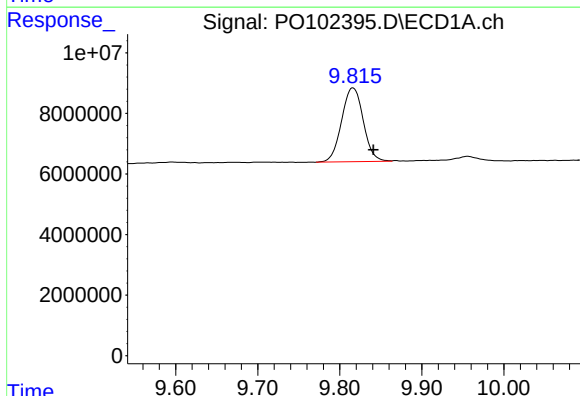

#2 Decachlorobiphenyl

R.T.: 9.816 min
Delta R.T.: -0.025 min
Response: 44801855
Conc: 17.59 ng/ml

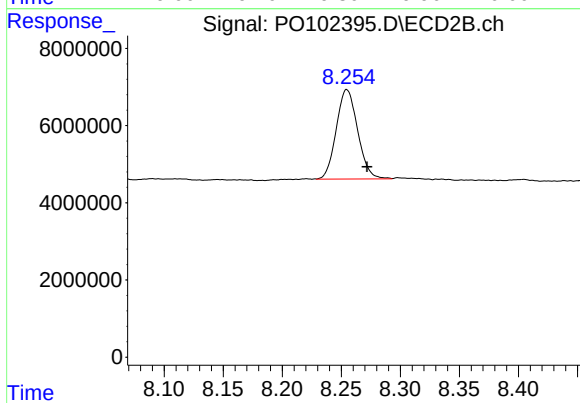

#2 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: -0.018 min
Response: 29250665
Conc: 14.14 ng/ml m