

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030821\
 Data File : P0075941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2021 12:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 01:23:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.941	1349200	1045600	22.635	23.440
2) SA Decachlor...	10.927	9.213	789717	845572	24.039	23.255
Target Compounds						
9) L2 AR-1221-2	5.277	0.000	16661	0	36.327	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030821\
Data File : P0075941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2021 12:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 01:23:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

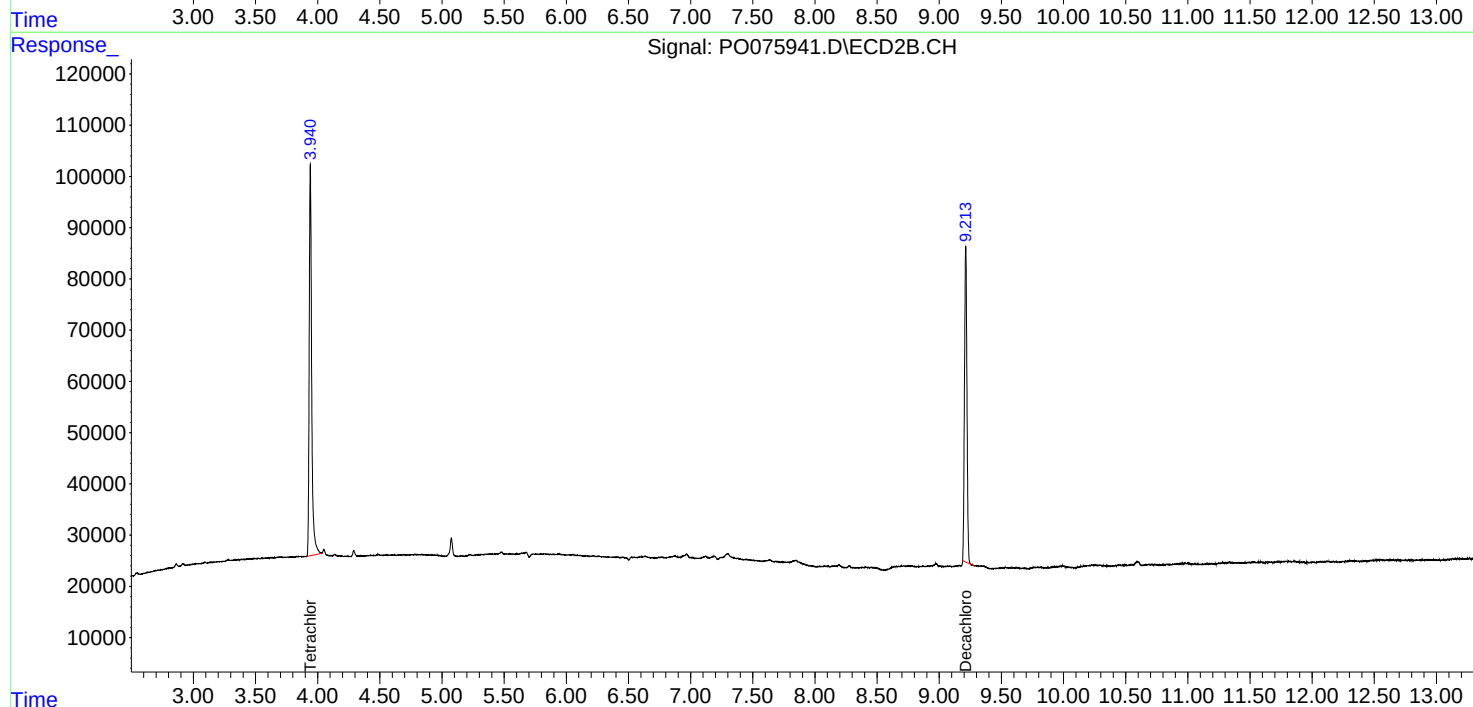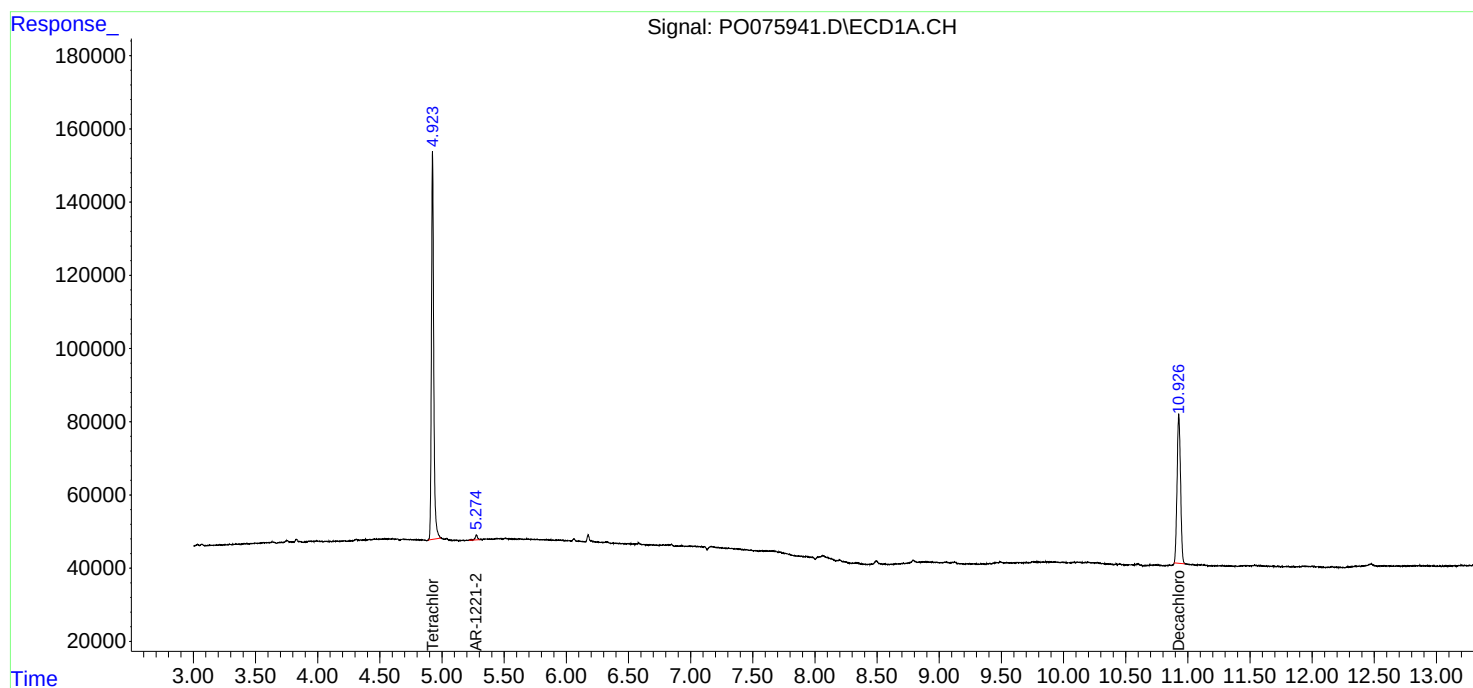


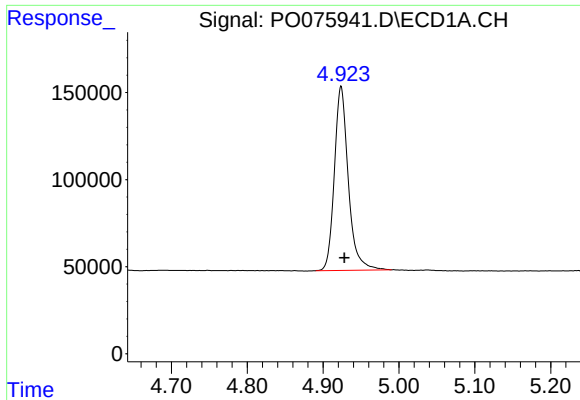

#1 Tetrachloro-m-xylene


R.T.: 4.924 min
Delta R.T.: -0.004 min
Response: 1349200
Conc: 22.63 ng/ml

Instrument :
ECD_O
ClientSampleId :

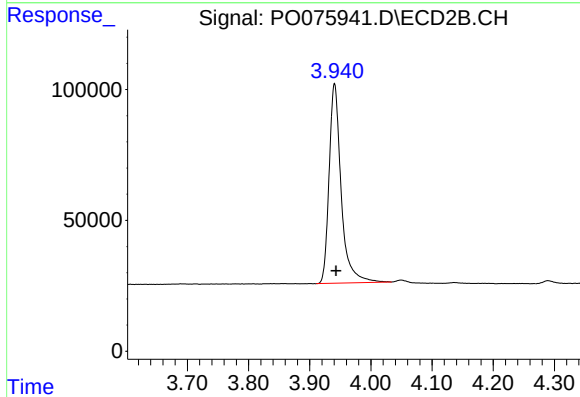


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 1045600
Conc: 23.44 ng/ml

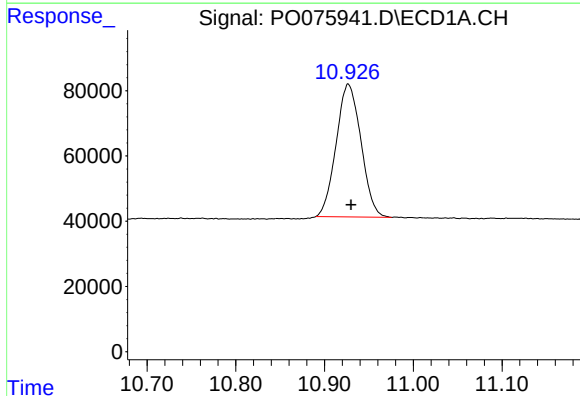


#2 Decachlorobiphenyl

R.T.: 10.927 min
Delta R.T.: -0.003 min
Response: 789717
Conc: 24.04 ng/ml

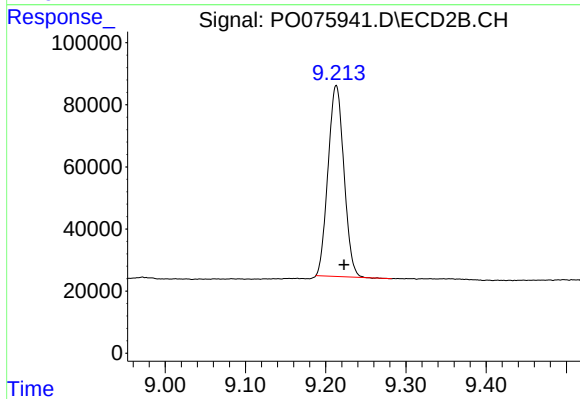

#2 Decachlorobiphenyl


R.T.: 9.213 min
Delta R.T.: -0.010 min
Response: 845572
Conc: 23.25 ng/ml

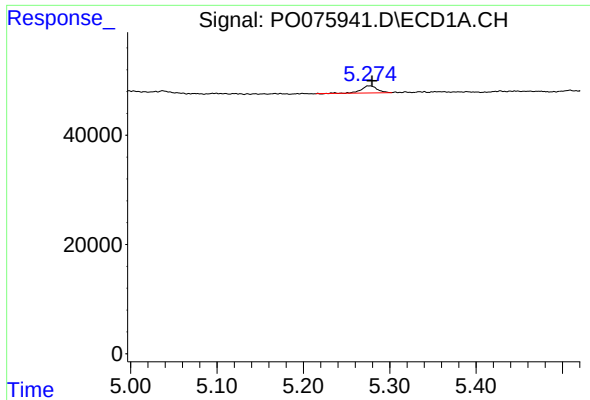

#9 AR-1221-2

R.T.: 5.277 min
Delta R.T.: -0.002 min
Response: 16661
Conc: 36.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

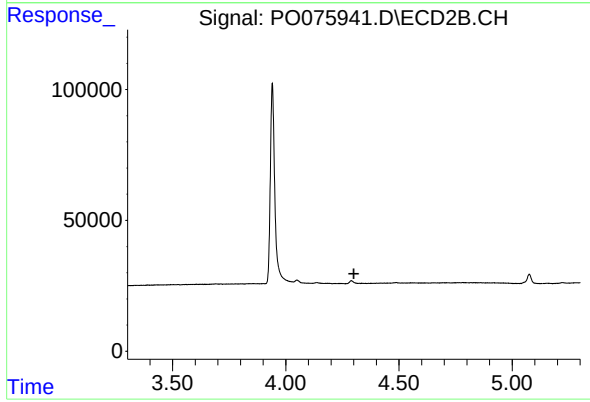

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.