

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030821\
 Data File : P0075944.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2021 13:15
 Operator : DD\AJ
 Sample : M1576-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 01:24:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.925	3.941	1039655	800916	17.442	17.955
2)	SA Decachlor...	10.929	9.213	540274	578265	16.446	15.903
Target Compounds							
5)	L1 AR-1016-3	0.000	5.399	0	72525	N.D.	60.061 #
7)	L1 AR-1016-5	6.790f	0.000	58618	0	44.518	N.D. #
12)	L3 AR-1232-2	5.980f	0.000	167634	0	268.278	N.D. #
13)	L3 AR-1232-3	0.000	5.399	0	72525	N.D.	142.560 #
18)	L4 AR-1242-3	0.000	5.399	0	72525	N.D.	74.091 #
23)	L5 AR-1248-3	6.790f	0.000	58618	0	32.634	N.D. #
30)	L6 AR-1254-5	8.503	0.000	51236	0	22.510	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030821\
Data File : PO075944.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2021 13:15
Operator : DD\AJ
Sample : M1576-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 01:24:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

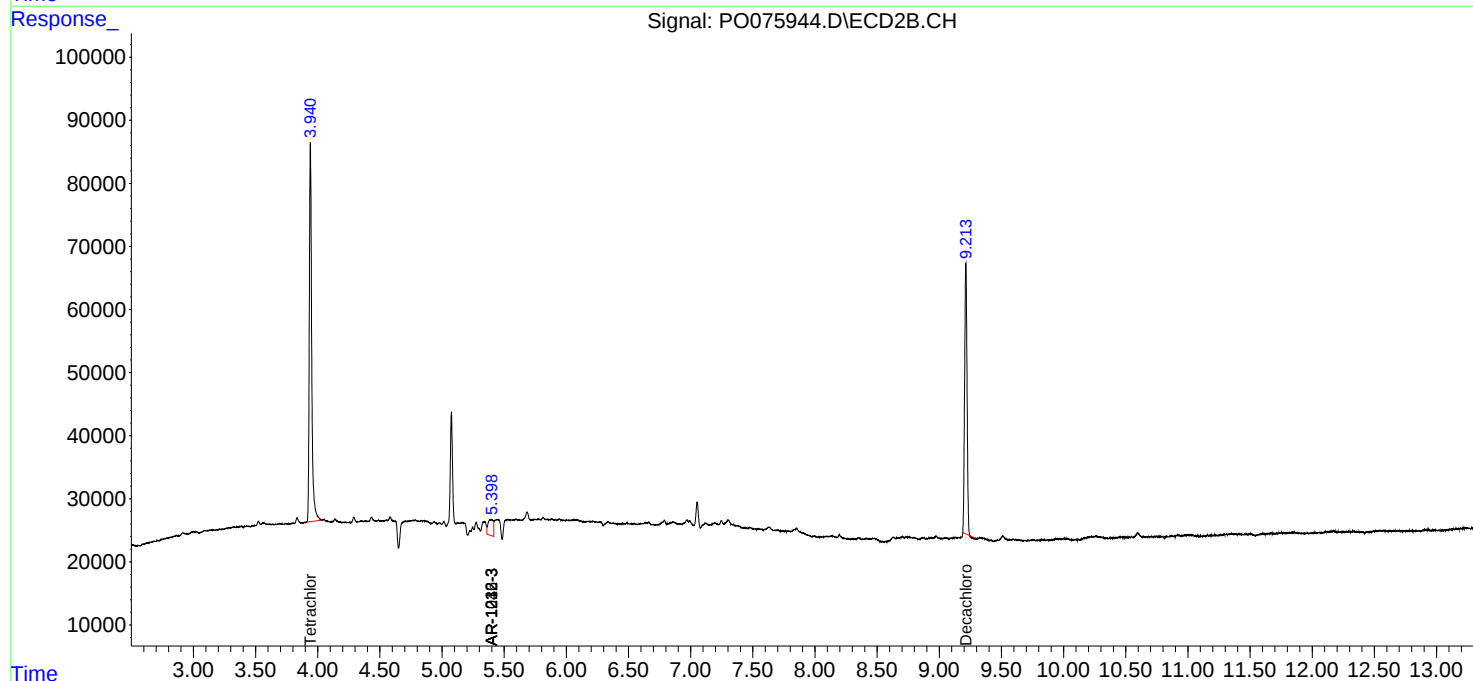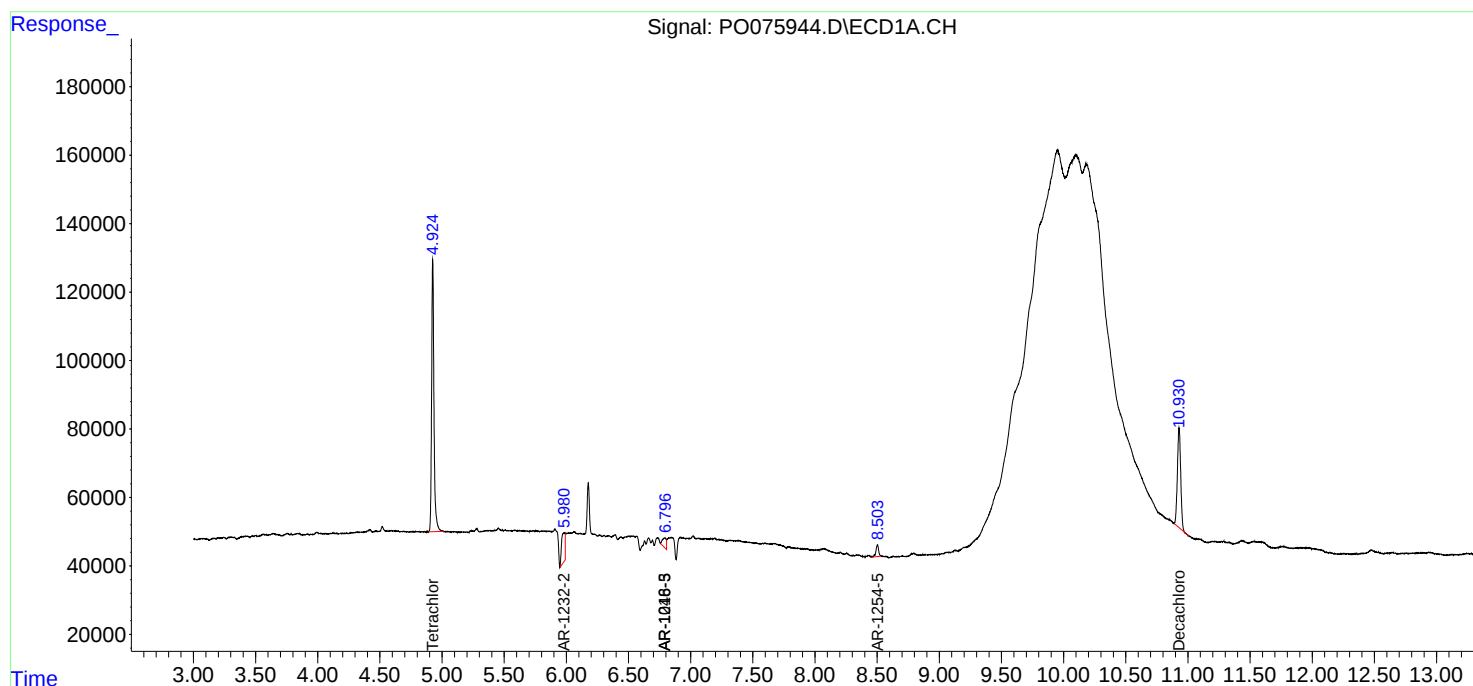


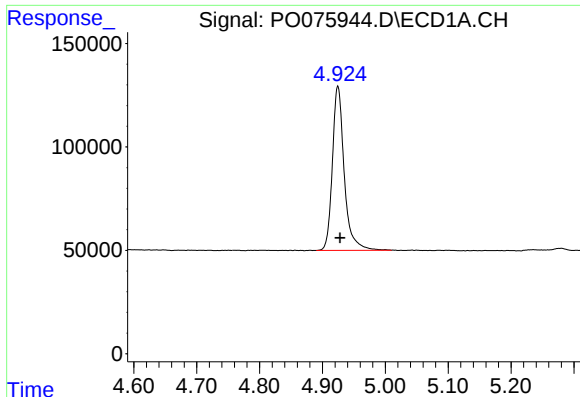

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.003 min
Response: 1039655
Conc: 17.44 ng/ml

Instrument :
ECD_O
ClientSampleId :

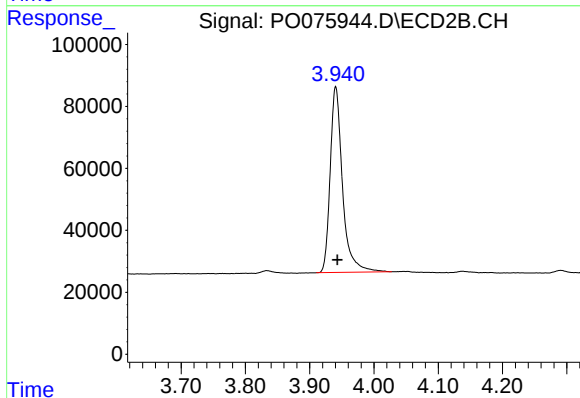


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 800916
Conc: 17.95 ng/ml

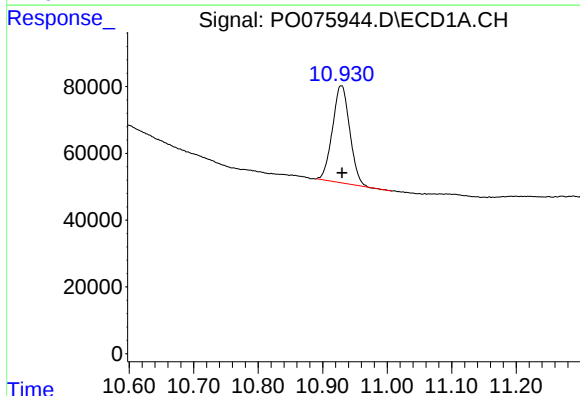


#2 Decachlorobiphenyl

R.T.: 10.929 min
Delta R.T.: -0.001 min
Response: 540274
Conc: 16.45 ng/ml

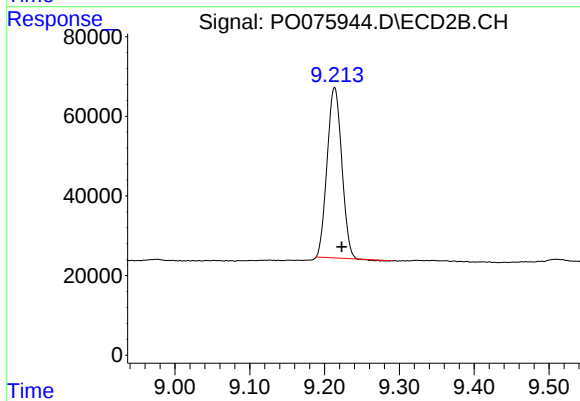

#2 Decachlorobiphenyl


R.T.: 9.213 min
Delta R.T.: -0.010 min
Response: 578265
Conc: 15.90 ng/ml

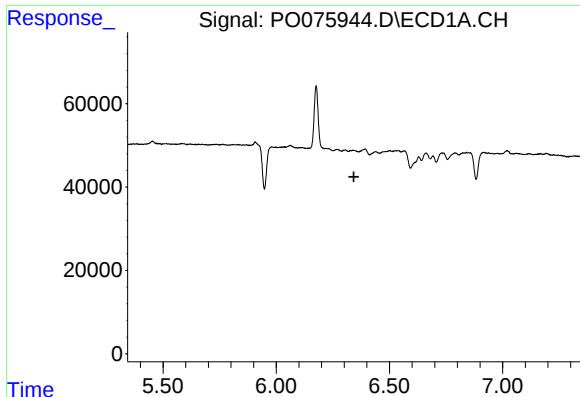

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

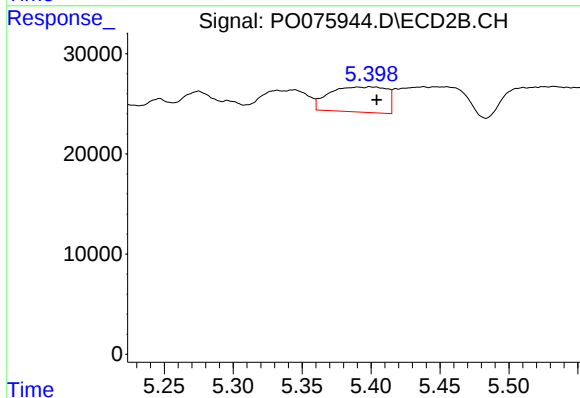


#5 AR-1016-3

R.T.: 5.399 min
Delta R.T.: -0.005 min
Response: 72525
Conc: 60.06 ng/ml

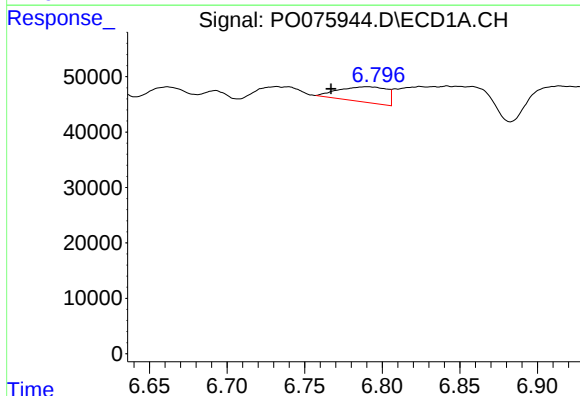


#7 AR-1016-5

R.T.: 6.790 min
Delta R.T.: 0.023 min
Response: 58618
Conc: 44.52 ng/ml

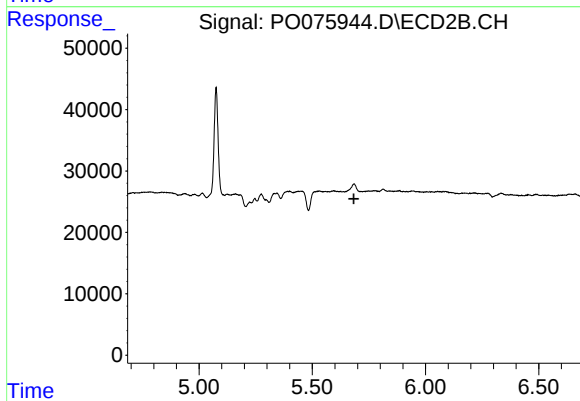

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.684 min
Response: 0
Conc: N.D.

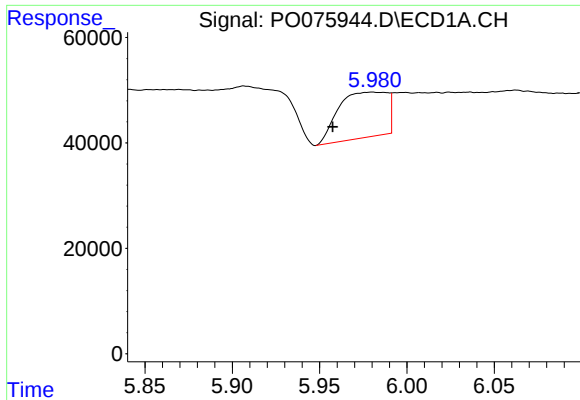

#12 AR-1232-2


R.T.: 5.980 min
Delta R.T.: 0.023 min
Response: 167634
Conc: 268.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

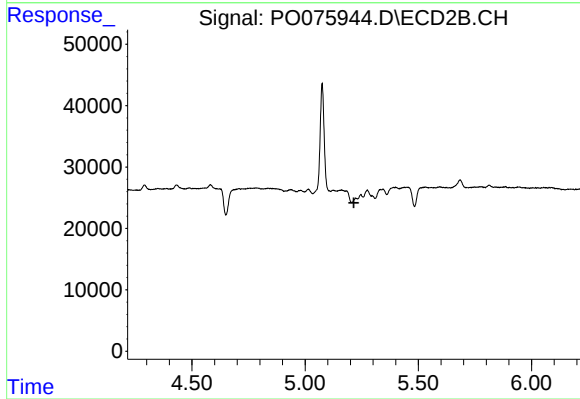


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.216 min
Response: 0
Conc: N.D.

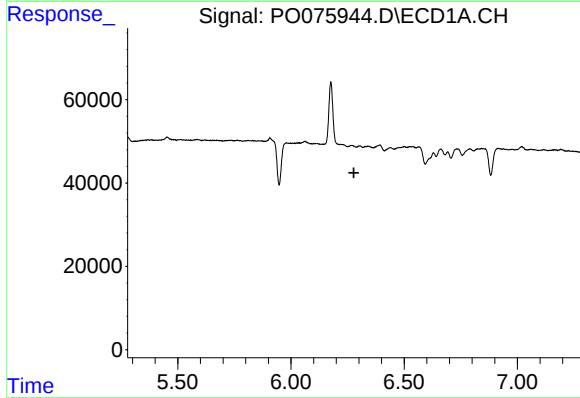


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 6.278 min
Response: 0
Conc: N.D.

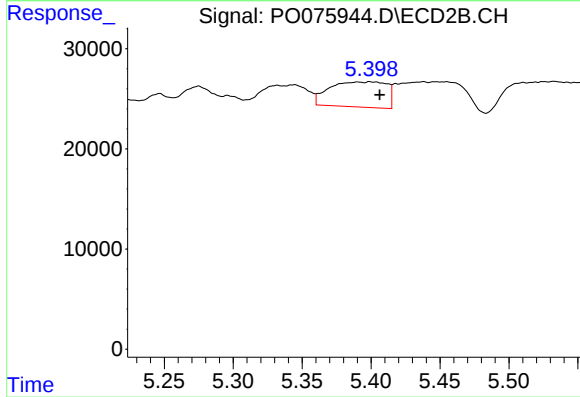

#13 AR-1232-3


R.T.: 5.399 min
Delta R.T.: -0.007 min
Response: 72525
Conc: 142.56 ng/ml

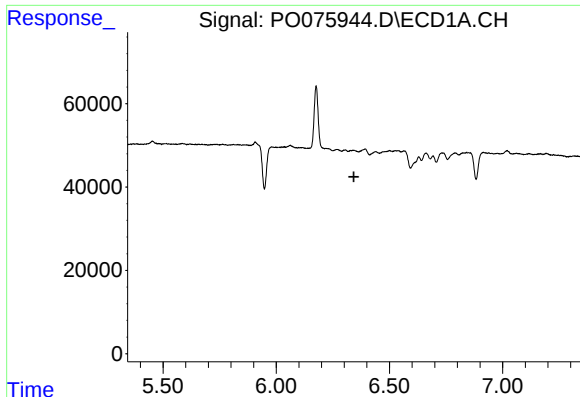

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

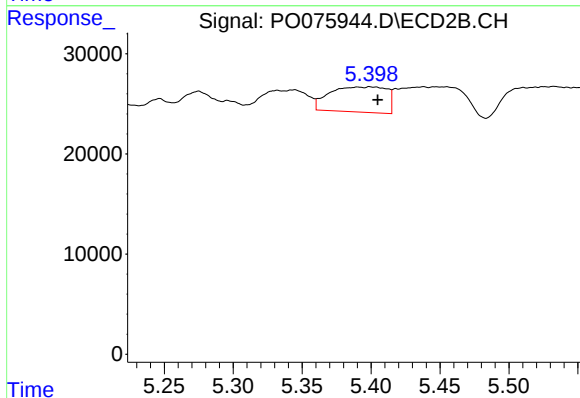


#18 AR-1242-3

R.T.: 5.399 min
Delta R.T.: -0.006 min
Response: 72525
Conc: 74.09 ng/ml

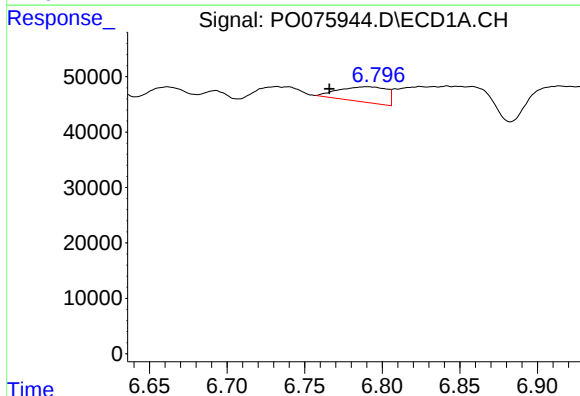


#23 AR-1248-3

R.T.: 6.790 min
Delta R.T.: 0.024 min
Response: 58618
Conc: 32.63 ng/ml

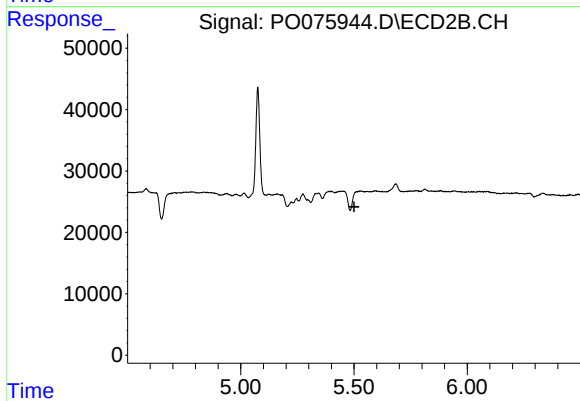

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.500 min
Response: 0
Conc: N.D.

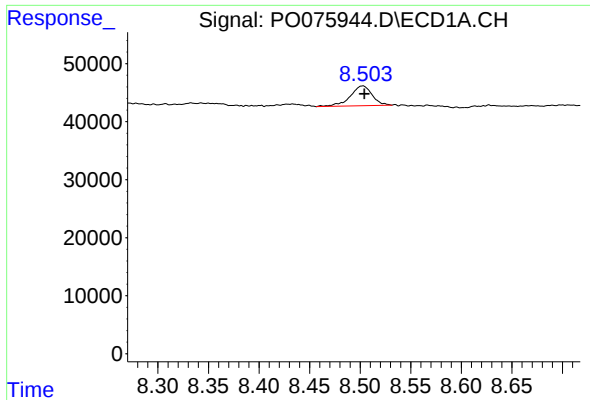

#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.001 min
Response: 51236
Conc: 22.51 ng/ml

Instrument :
ECD_O
ClientSampleId :

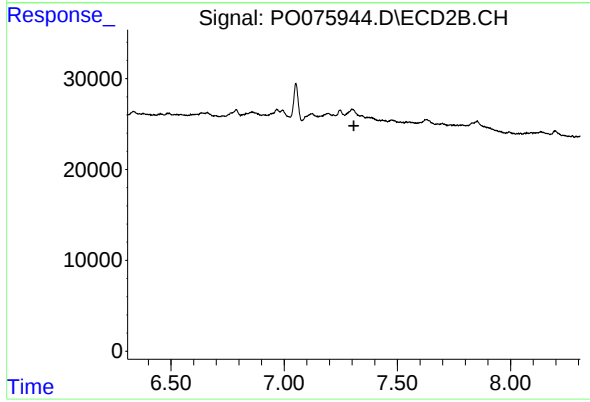

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.308 min
Response: 0
Conc: N.D.