

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
 Data File : P0075969.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2021 11:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 13:42:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.931	3.941	1316042	977099	22.079	21.904
2)	SA Decachlor...	10.937	9.217	854443	872916	26.009	24.007
Target Compounds							
9)	L2 AR-1221-2	5.284	0.000	14215	0	30.994	N.D. #
20)	L4 AR-1242-5	7.210f	0.000	6669	0	6.223	N.D. #
24)	L5 AR-1248-4	7.183	0.000	15740	0	8.238	N.D. #
25)	L5 AR-1248-5	7.210f	0.000	6669	0	3.523	N.D. #
26)	L6 AR-1254-1	7.164	0.000	30999	0	14.912	N.D. #
29)	L6 AR-1254-4	8.069	0.000	13535	0	6.191	N.D. #
30)	L6 AR-1254-5	8.497	0.000	14062	0	6.178	N.D. #
34)	L7 AR-1260-4	8.803	0.000	15698	0	7.221	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
Data File : P0075969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2021 11:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 13:42:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

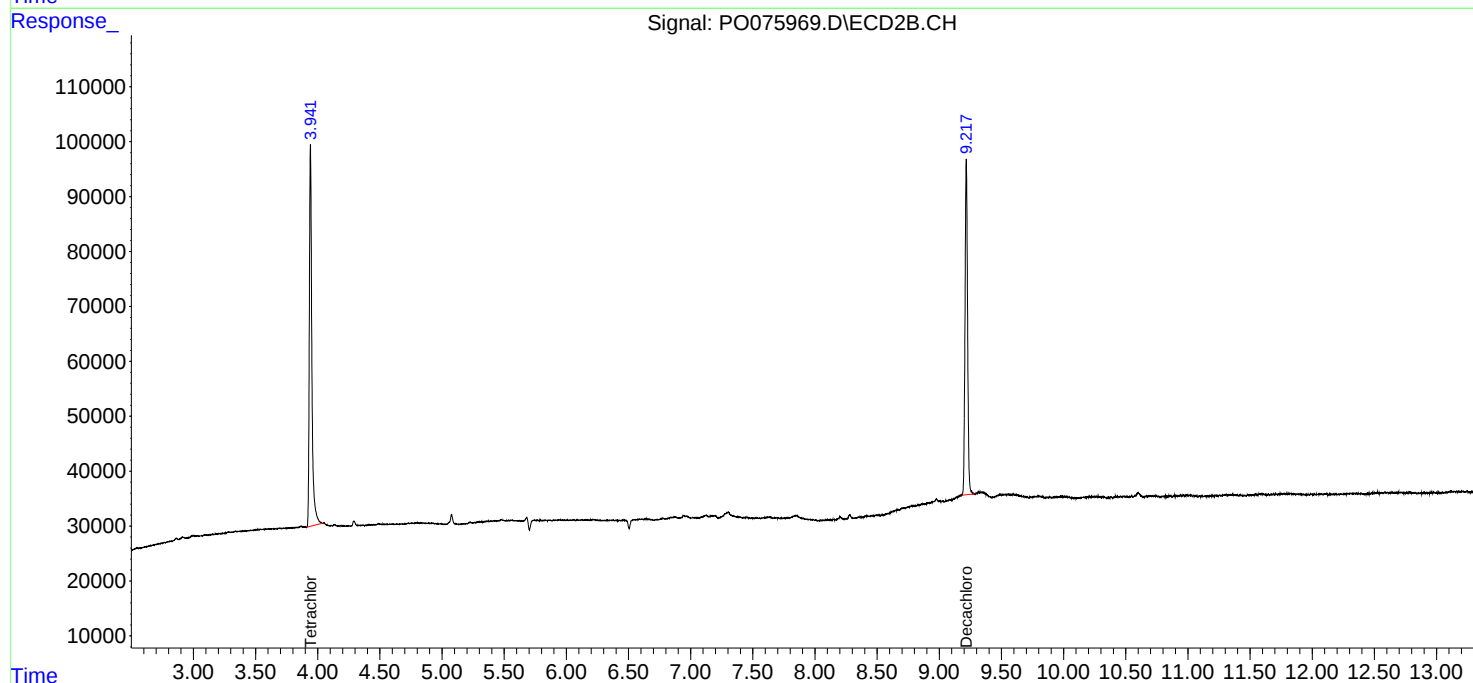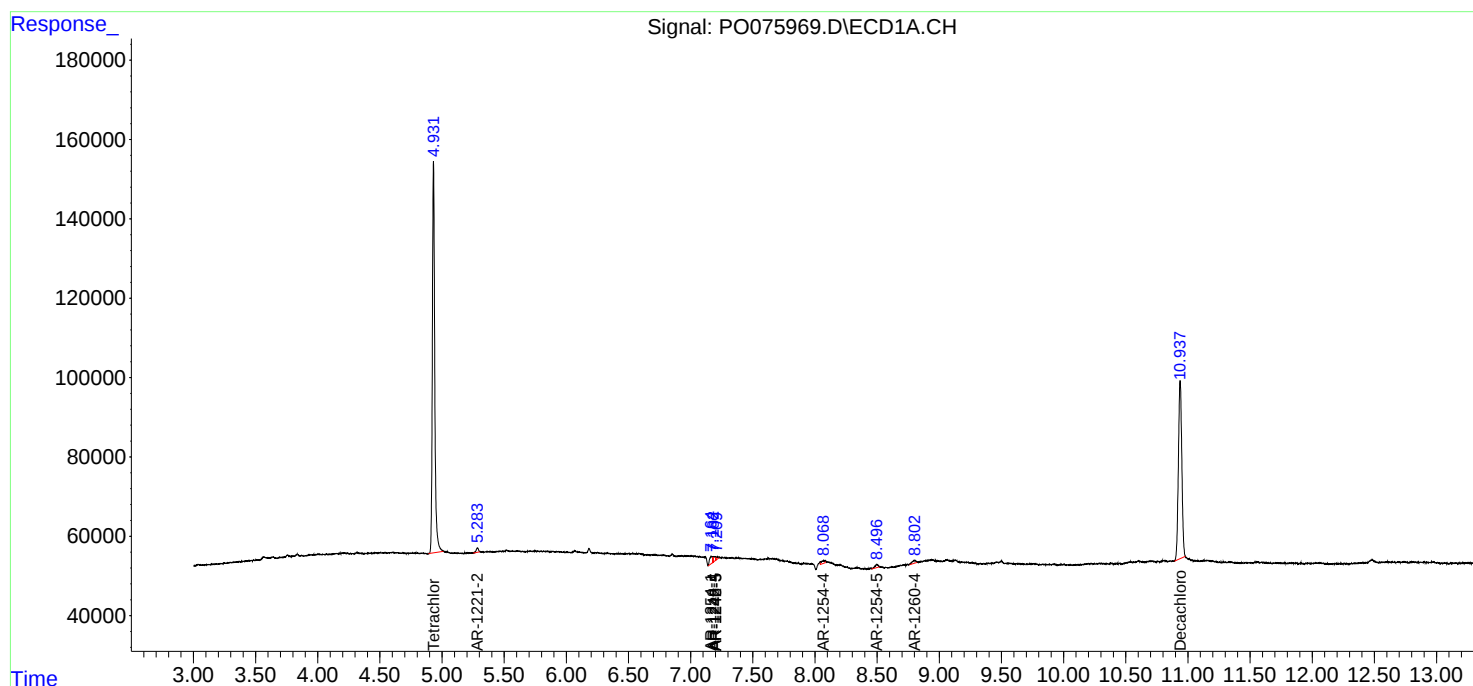


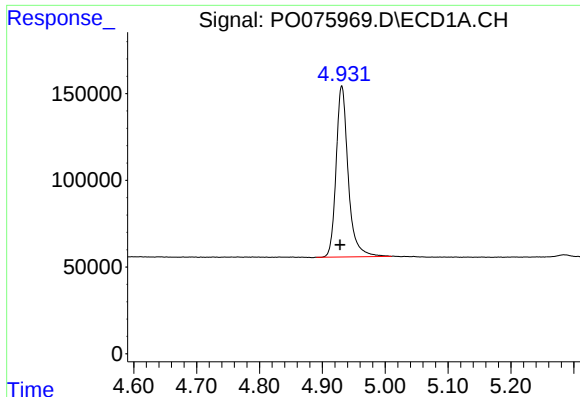

#1 Tetrachloro-m-xylene


R.T.: 4.931 min
Delta R.T.: 0.003 min
Response: 1316042
Conc: 22.08 ng/ml

Instrument :
ECD_O
ClientSampleId :

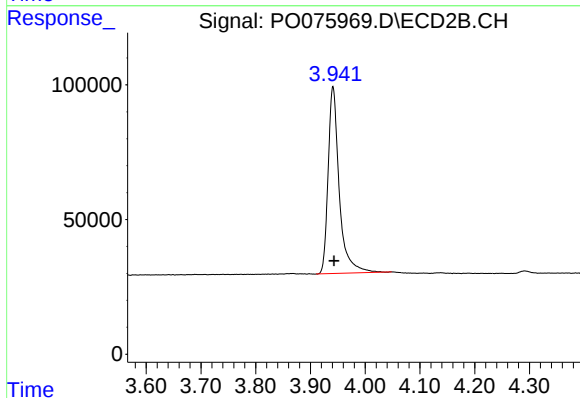


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 977099
Conc: 21.90 ng/ml

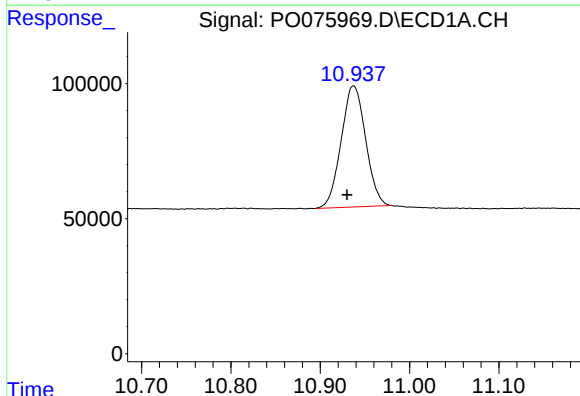


#2 Decachlorobiphenyl

R.T.: 10.937 min
Delta R.T.: 0.007 min
Response: 854443
Conc: 26.01 ng/ml

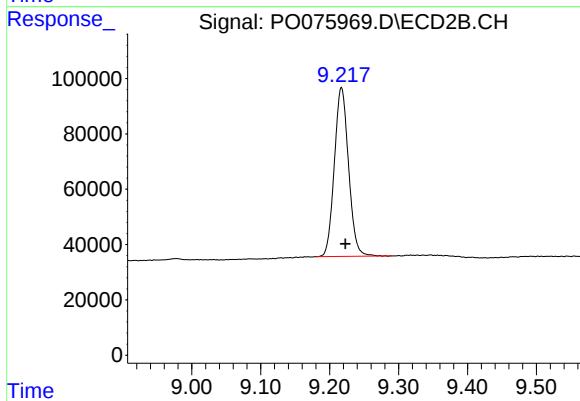

#2 Decachlorobiphenyl


R.T.: 9.217 min
Delta R.T.: -0.006 min
Response: 872916
Conc: 24.01 ng/ml

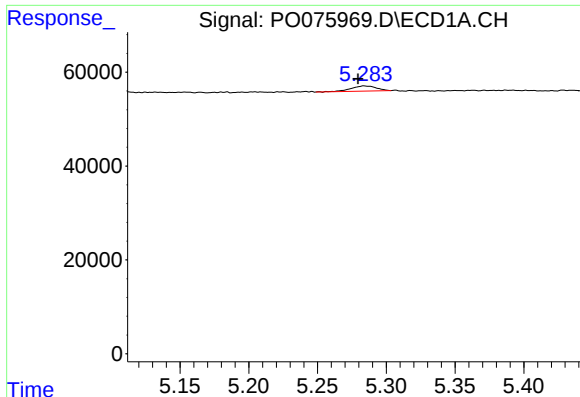

#9 AR-1221-2


R.T.: 5.284 min
Delta R.T.: 0.004 min
Response: 14215
Conc: 30.99 ng/ml

Instrument :
ECD_O
ClientSampleId :

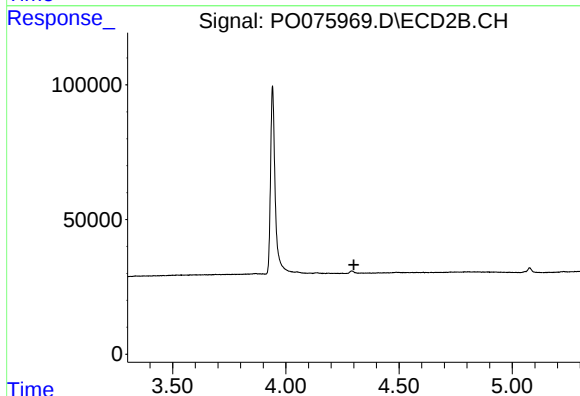


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.

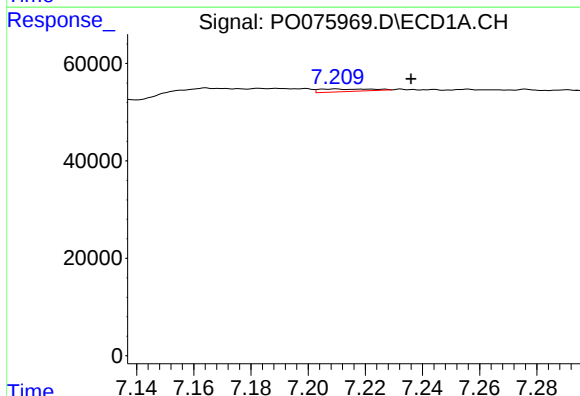


#20 AR-1242-5

R.T.: 7.210 min
Delta R.T.: -0.026 min
Response: 6669
Conc: 6.22 ng/ml

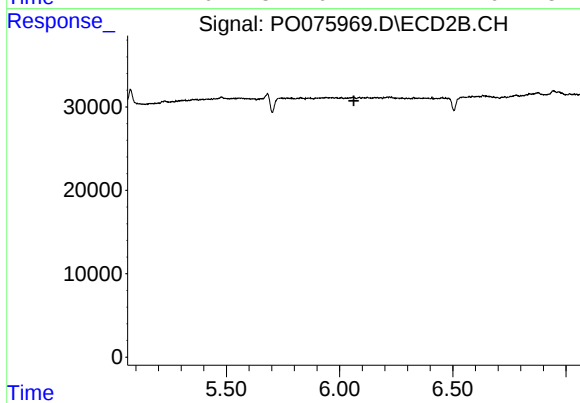

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.063 min
Response: 0
Conc: N.D.

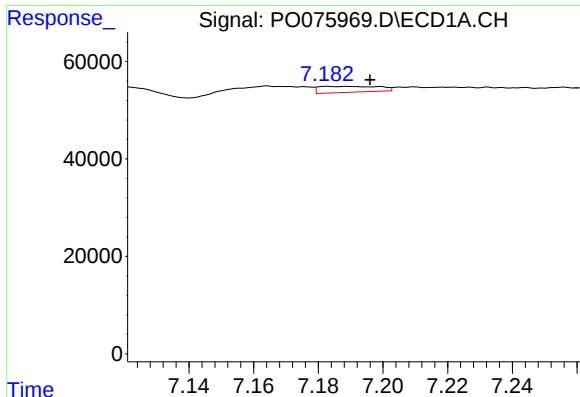

#24 AR-1248-4


R.T.: 7.183 min
Delta R.T.: -0.013 min
Response: 15740
Conc: 8.24 ng/ml

Instrument :
ECD_O
ClientSampleId :

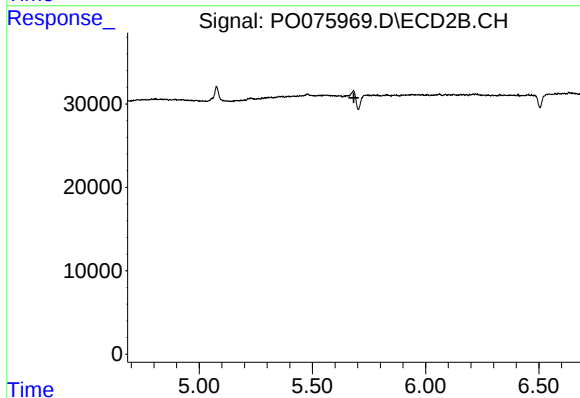


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.683 min
Response: 0
Conc: N.D.

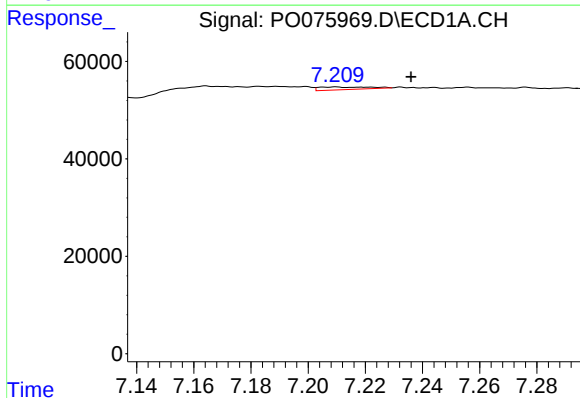


#25 AR-1248-5

R.T.: 7.210 min
Delta R.T.: -0.026 min
Response: 6669
Conc: 3.52 ng/ml

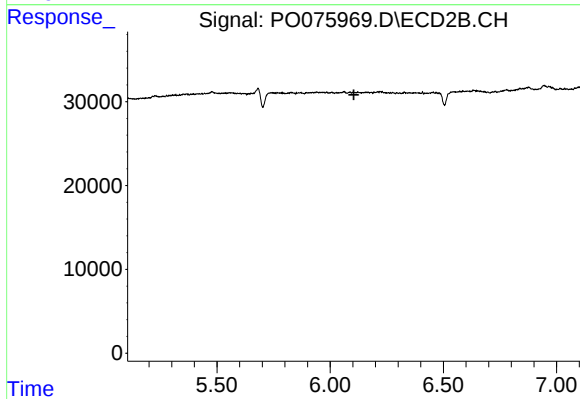

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.105 min
Response: 0
Conc: N.D.

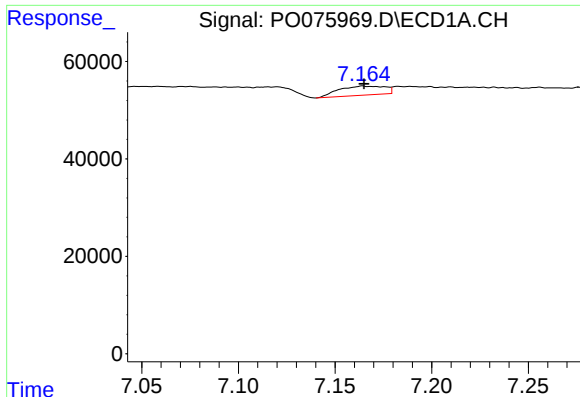

#26 AR-1254-1


R.T.: 7.164 min
Delta R.T.: 0.000 min
Response: 30999
Conc: 14.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

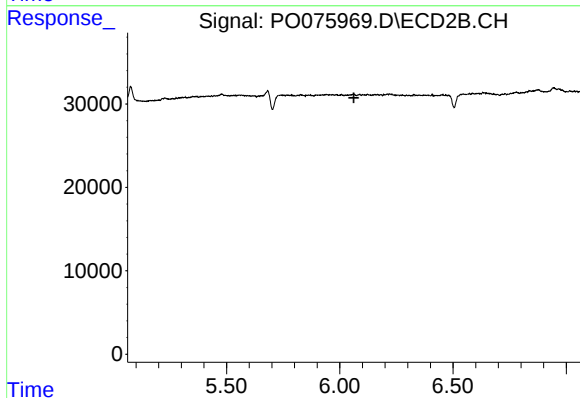


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

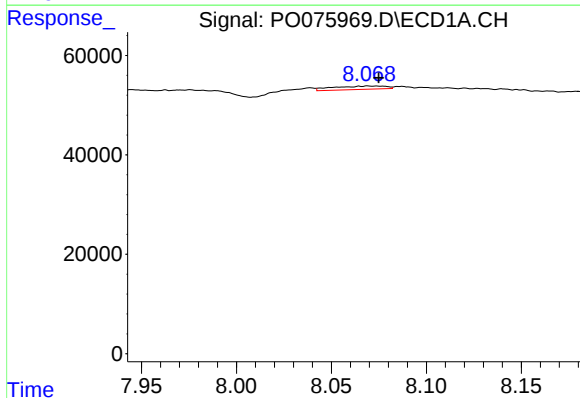


#29 AR-1254-4

R.T.: 8.069 min
Delta R.T.: -0.006 min
Response: 13535
Conc: 6.19 ng/ml

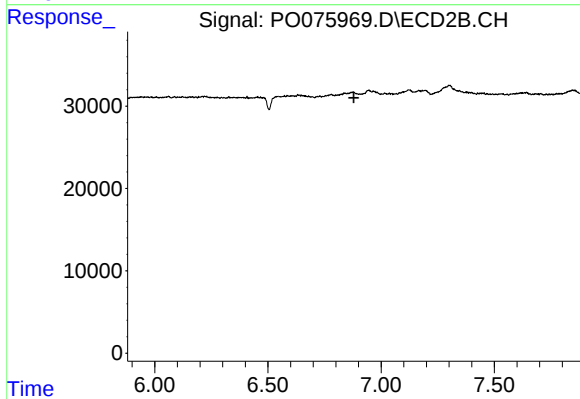

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.880 min
Response: 0
Conc: N.D.

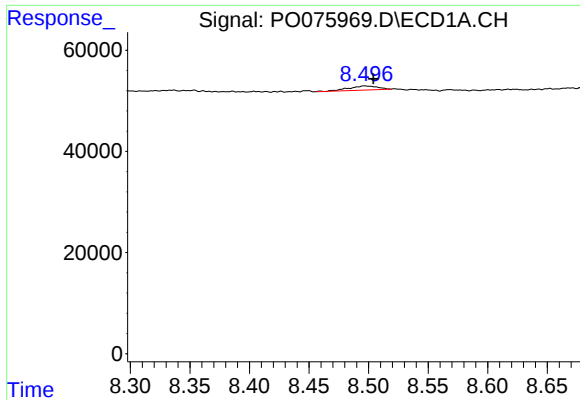

#30 AR-1254-5


R.T.: 8.497 min
Delta R.T.: -0.007 min
Response: 14062
Conc: 6.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

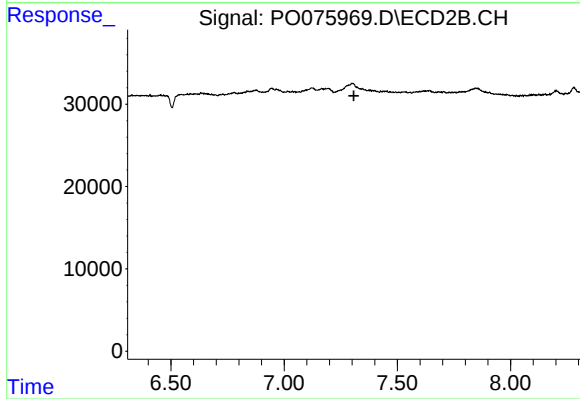


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.308 min
Response: 0
Conc: N.D.

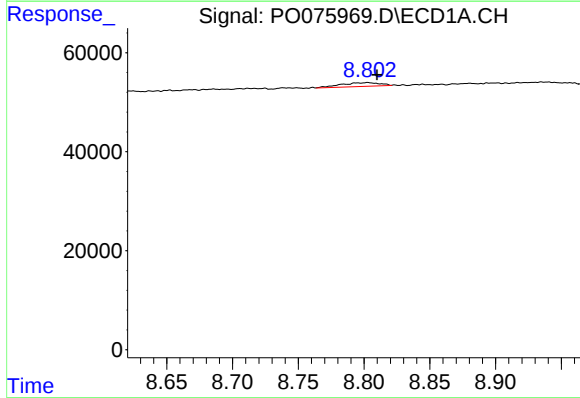

#34 AR-1260-4

R.T.: 8.803 min
Delta R.T.: -0.007 min
Response: 15698
Conc: 7.22 ng/ml

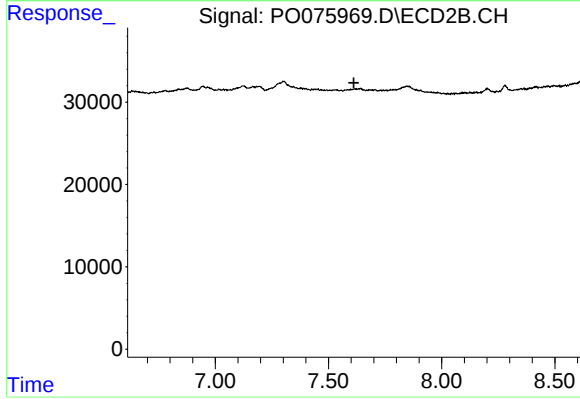

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.612 min
Response: 0
Conc: N.D.