

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
 Data File : P0075989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2021 18:21
 Operator : DD\AJ
 Sample : PB135069BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 02:53:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.941	1180429	934550	19.804	20.950
2) SA Decachlor...	10.930	9.214	732593	749041	22.300	20.600
Target Compounds						
8) L2 AR-1221-1	5.184	0.000	24846	0	41.178	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
Data File : P0075989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2021 18:21
Operator : DD\AJ
Sample : PB135069BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 02:53:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

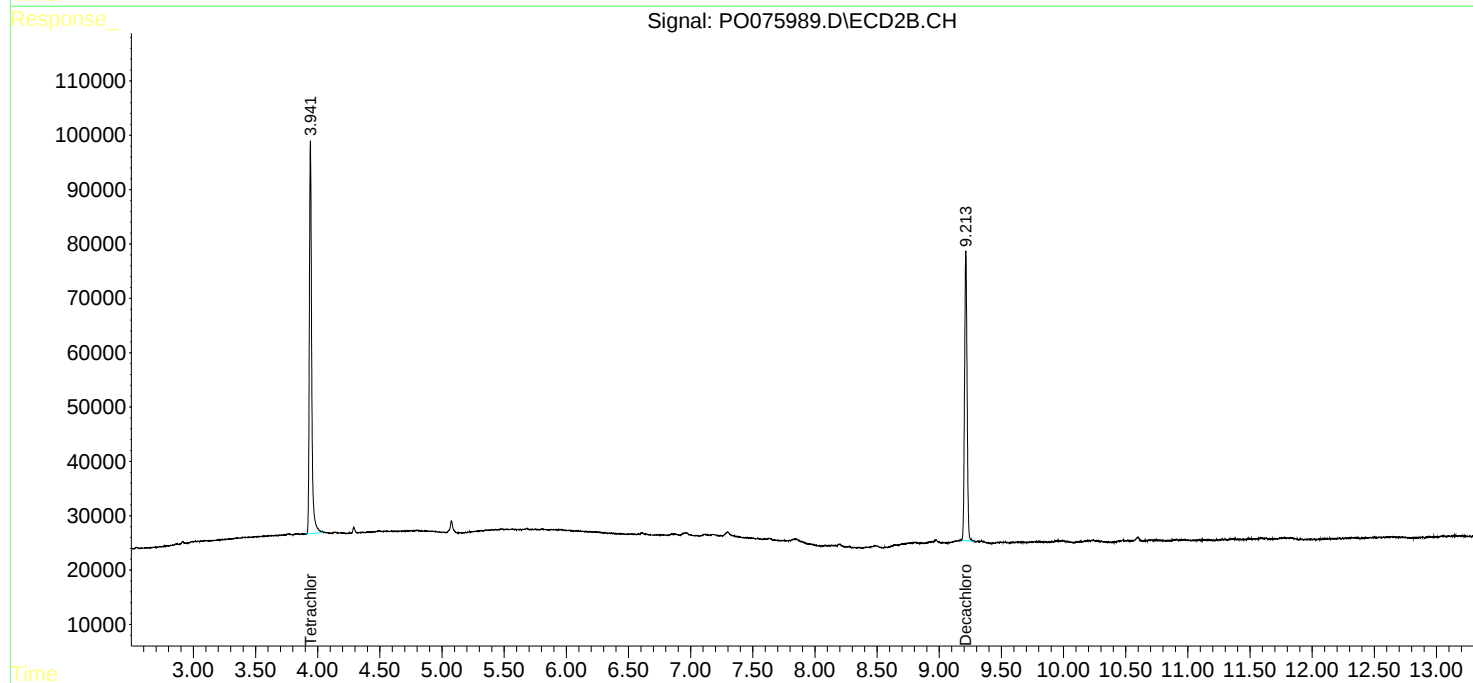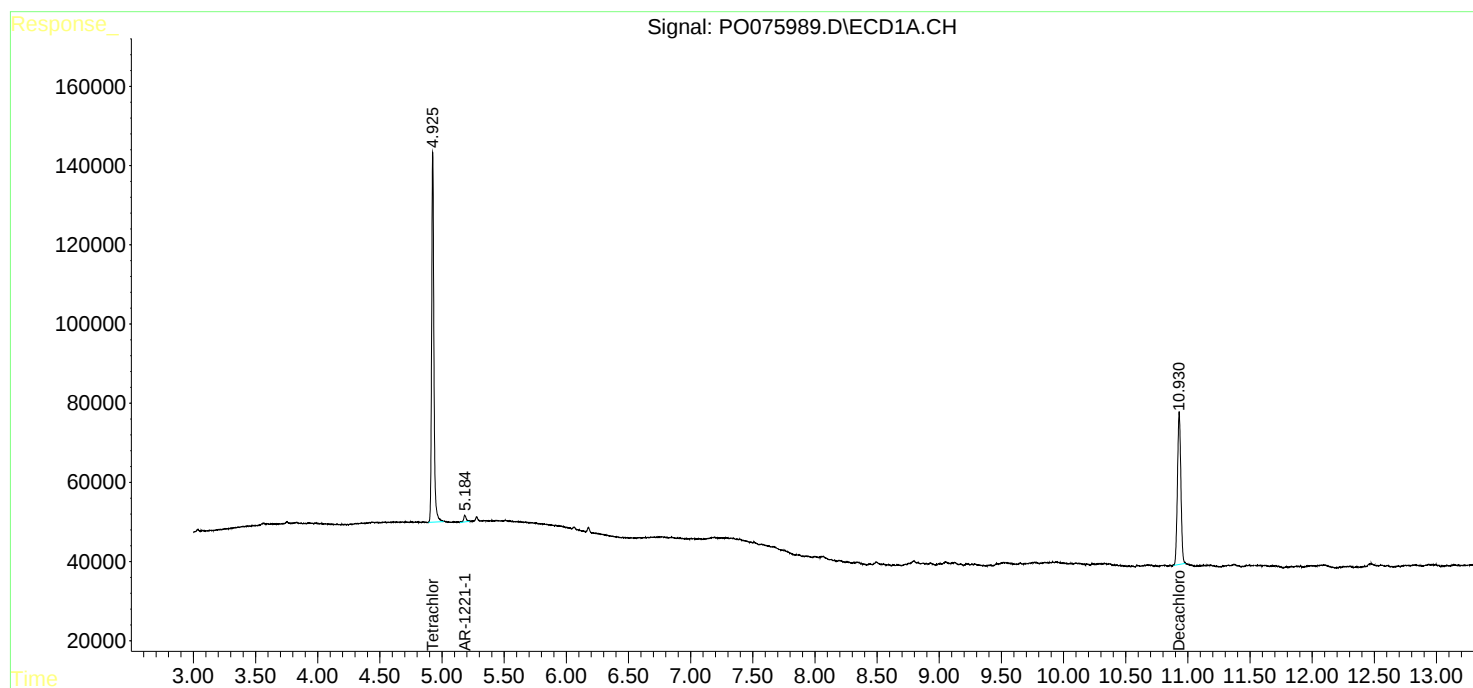


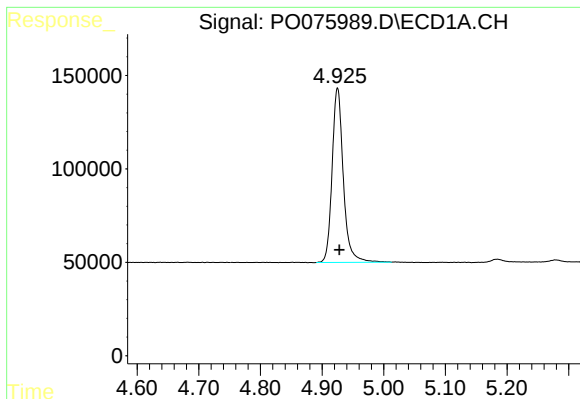

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.003 min
Response: 1180429
Conc: 19.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

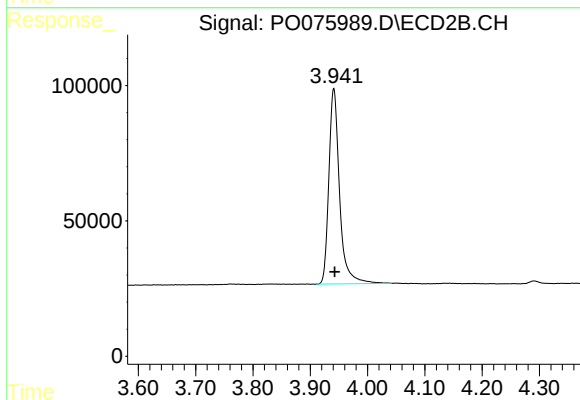


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 934550
Conc: 20.95 ng/ml

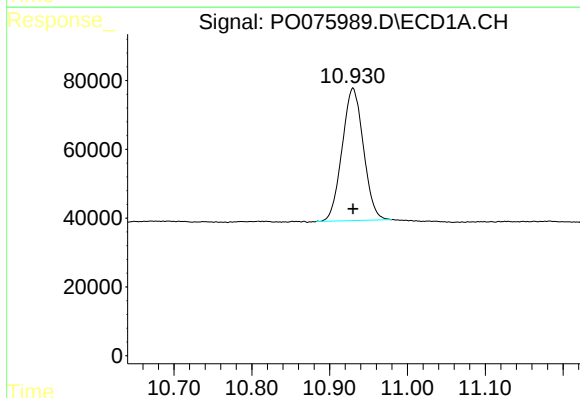


#2 Decachlorobiphenyl

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 732593
Conc: 22.30 ng/ml

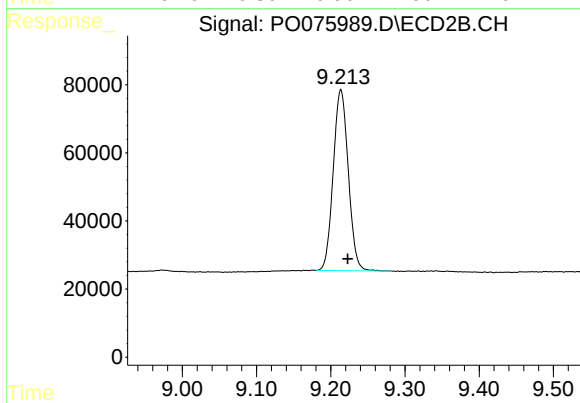

#2 Decachlorobiphenyl


R.T.: 9.214 min
Delta R.T.: -0.009 min
Response: 749041
Conc: 20.60 ng/ml

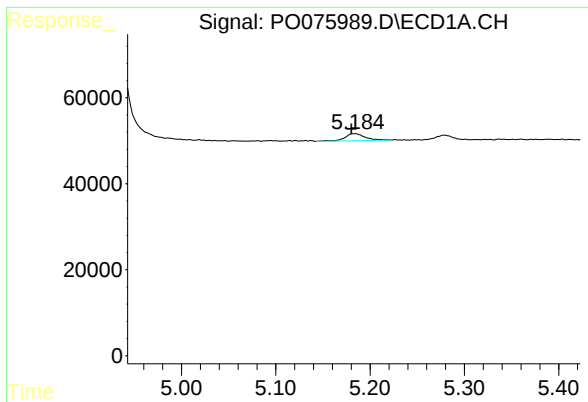

#8 AR-1221-1

R.T.: 5.184 min
Delta R.T.: 0.004 min
Response: 24846
Conc: 41.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

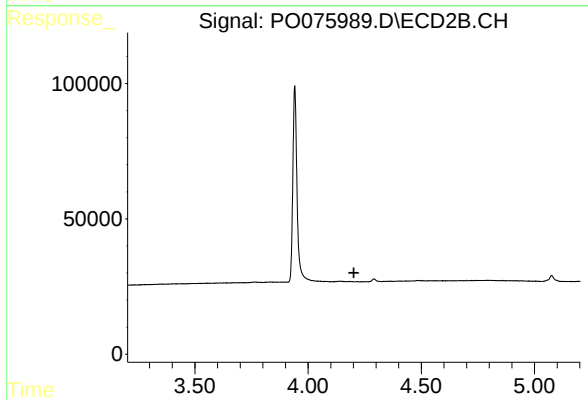

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.