

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
 Data File : P0075973.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2021 12:35
 Operator : DD\AJ
 Sample : M1589-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-067-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 13:44:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.939	1429351	1037899	23.980	23.267
2) SA Decachlor...	10.929	9.214	814604	764108	24.797	21.015

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
Data File : P0075973.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2021 12:35
Operator : DD\AJ
Sample : M1589-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-067-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 13:44:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

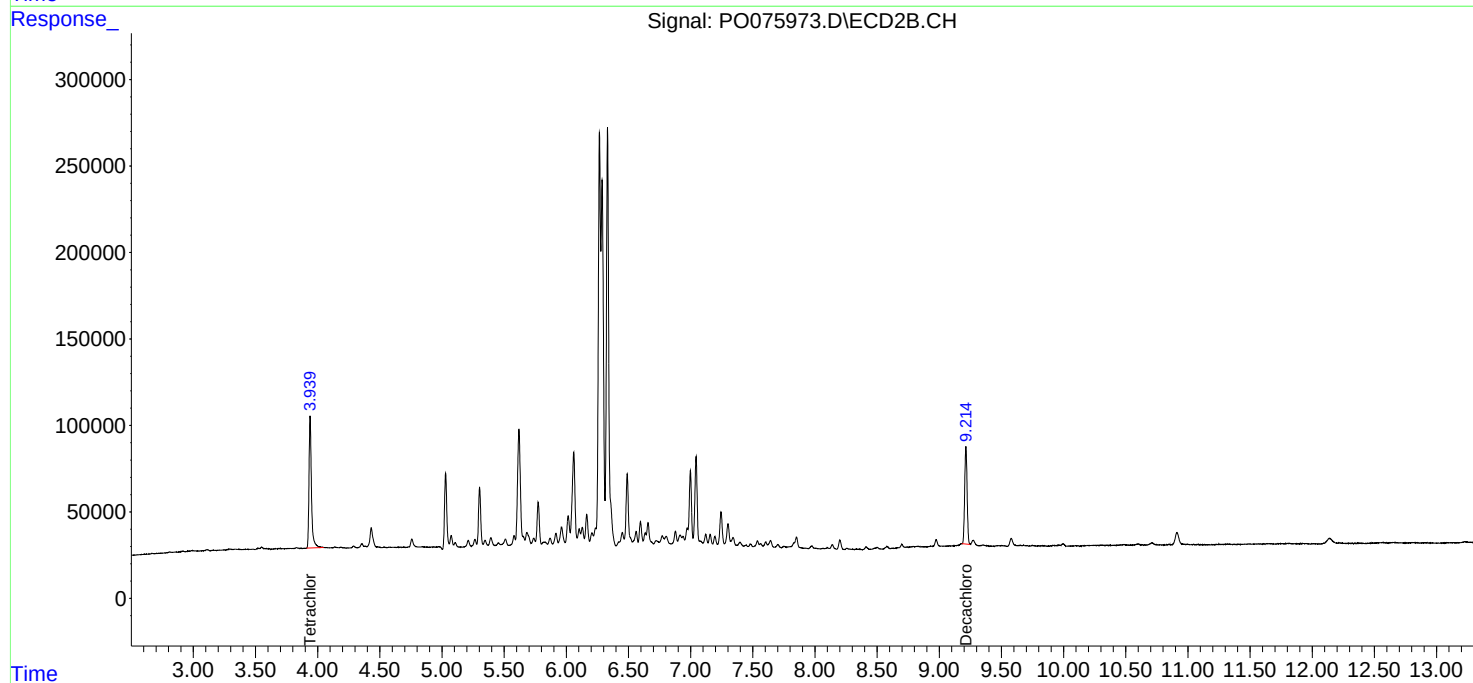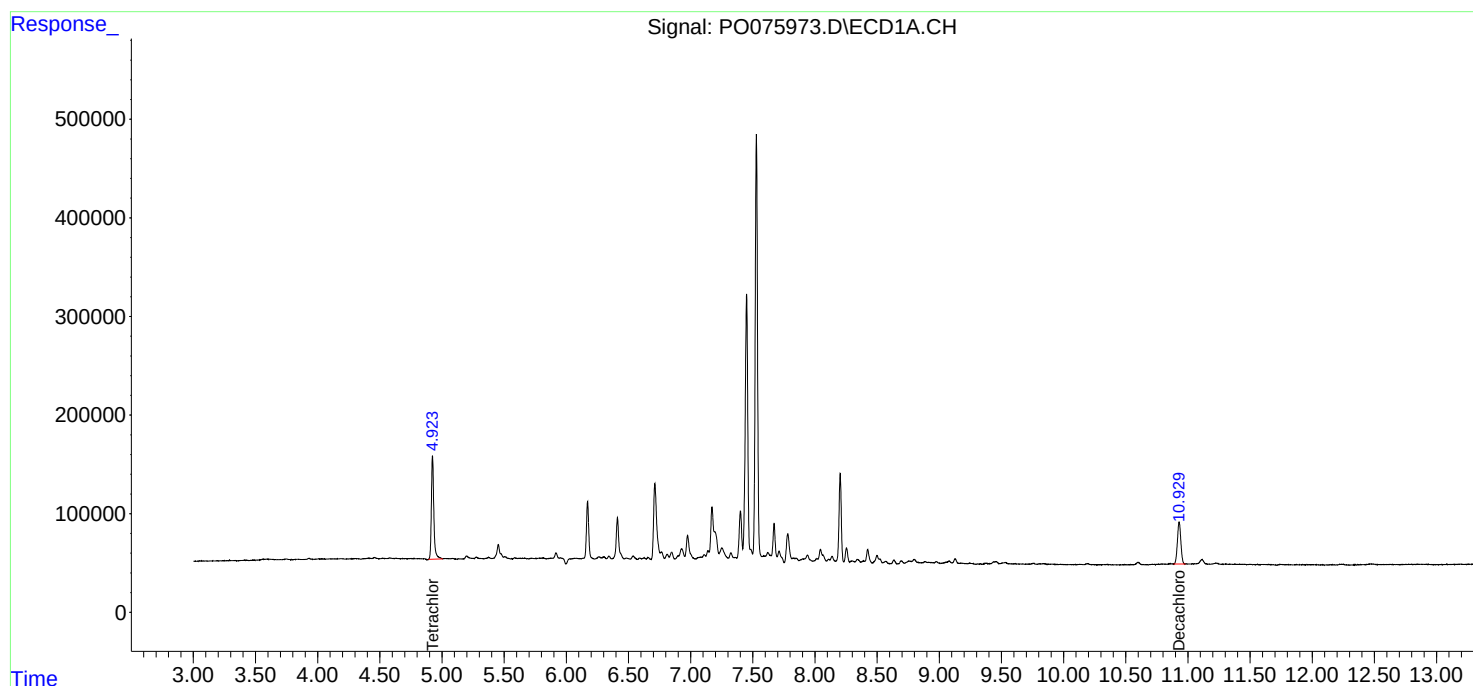


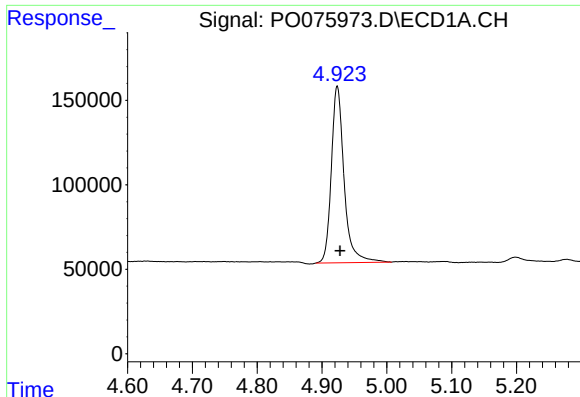

#1 Tetrachloro-m-xylene


R.T.: 4.923 min
Delta R.T.: -0.005 min
Response: 1429351
Conc: 23.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-067-A

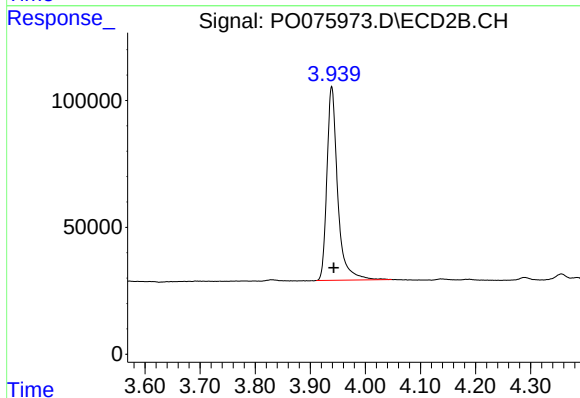


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.004 min
Response: 1037899
Conc: 23.27 ng/ml

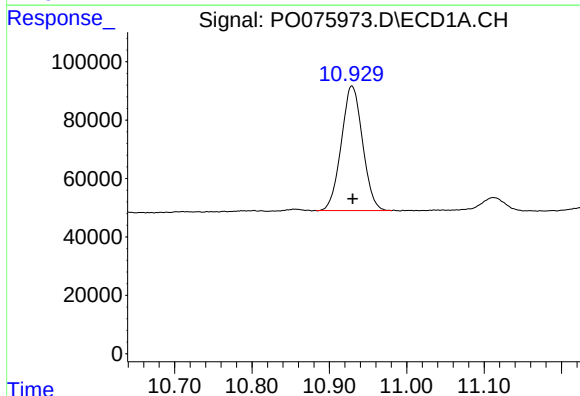

#2 Decachlorobiphenyl

R.T.: 10.929 min
Delta R.T.: 0.000 min
Response: 814604
Conc: 24.80 ng/ml

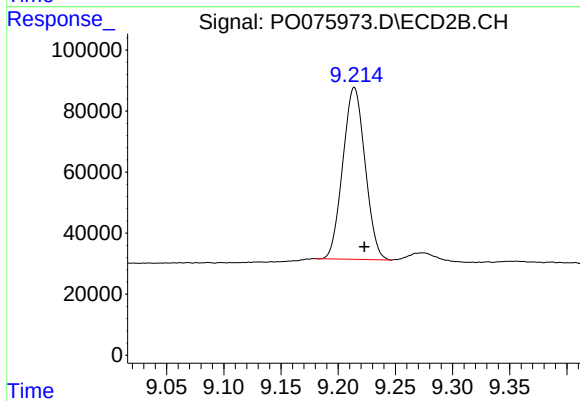

#2 Decachlorobiphenyl

R.T.: 9.214 min
Delta R.T.: -0.009 min
Response: 764108
Conc: 21.01 ng/ml