

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
 Data File : P0075975.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2021 13:09
 Operator : DD\AJ
 Sample : M1590-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-018-ABCD

Manual Integrations
 APPROVED

Ankita
 3/10/2021 2:02:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 13:45:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.939	1404764	1013165	23.567	22.713
2) SA Decachlor...	10.930	9.214	844222	811629	25.698	22.321

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
Data File : P0075975.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2021 13:09
Operator : DD\AJ
Sample : M1590-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-EF-01-018-ABCD


Manual Integrations
APPROVED

Ankita
3/10/2021 2:02:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 13:45:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

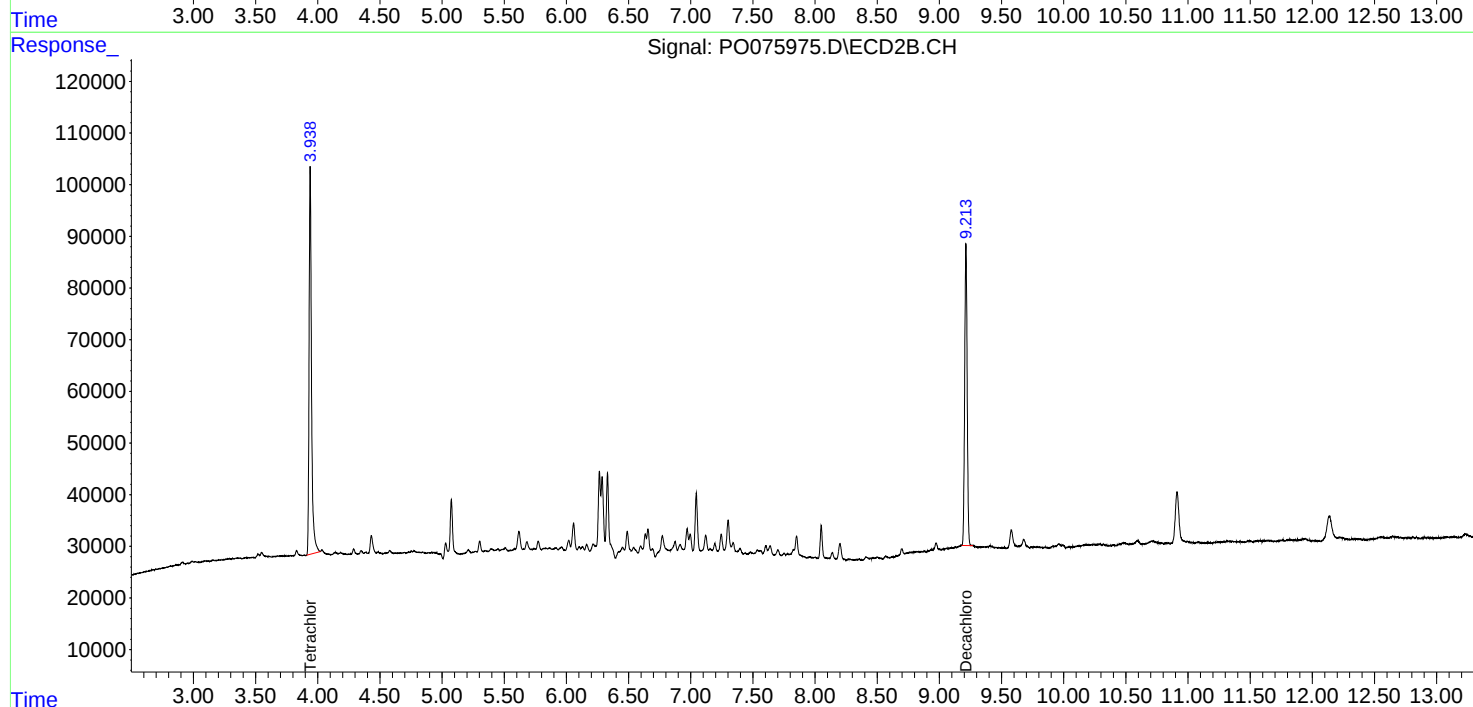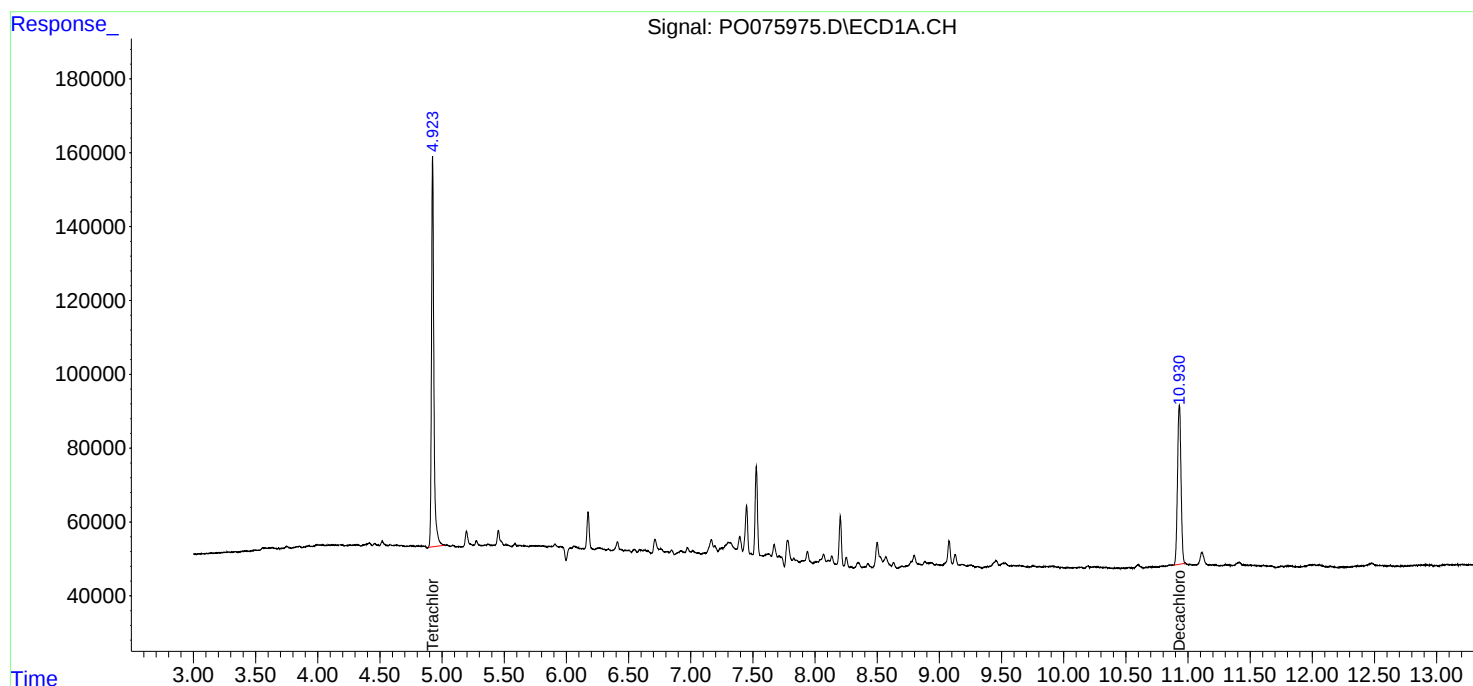

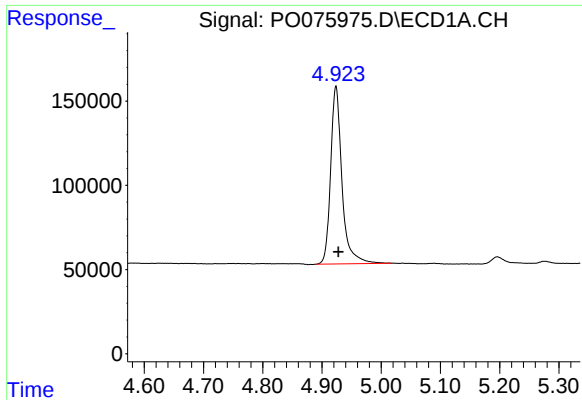


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.004 min
Response: 1404764
Conc: 23.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-018-ABCD


Manual Integrations
APPROVED

Ankita
3/10/2021 2:02:38 PM

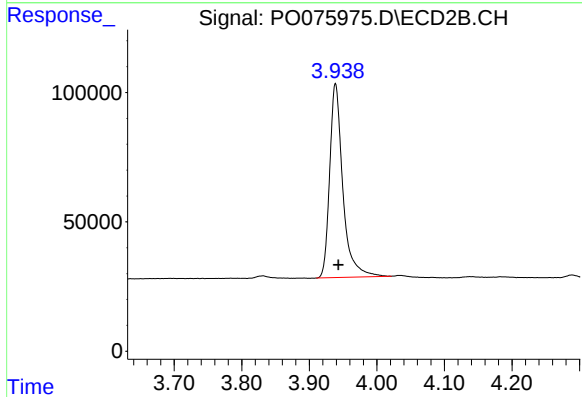


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.004 min
Response: 1013165
Conc: 22.71 ng/ml

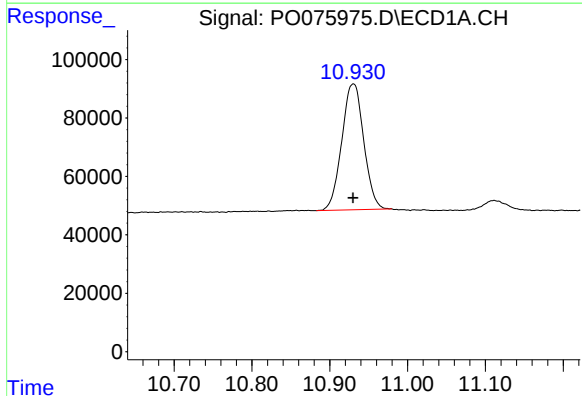

#2 Decachlorobiphenyl

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 844222
Conc: 25.70 ng/ml

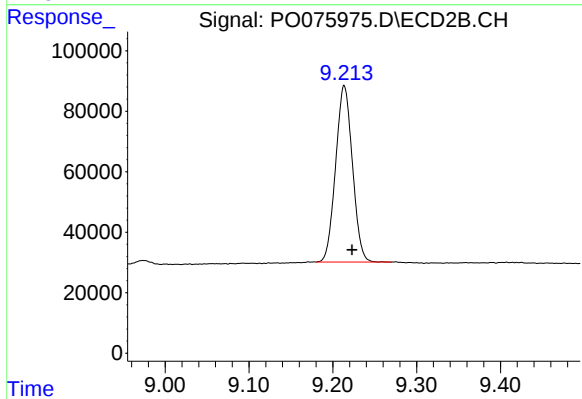

#2 Decachlorobiphenyl

R.T.: 9.214 min
Delta R.T.: -0.009 min
Response: 811629
Conc: 22.32 ng/ml