

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
 Data File : P0075983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2021 15:47
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 3/10/2021 2:02:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 17:05:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	3.940	1491892	1109143	25.029	24.864
2) SA Decachlor...	10.934	9.214	1003581	962532	30.549m	26.472

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030921\
Data File : P0075983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2021 15:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
3/10/2021 2:02:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 17:05:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

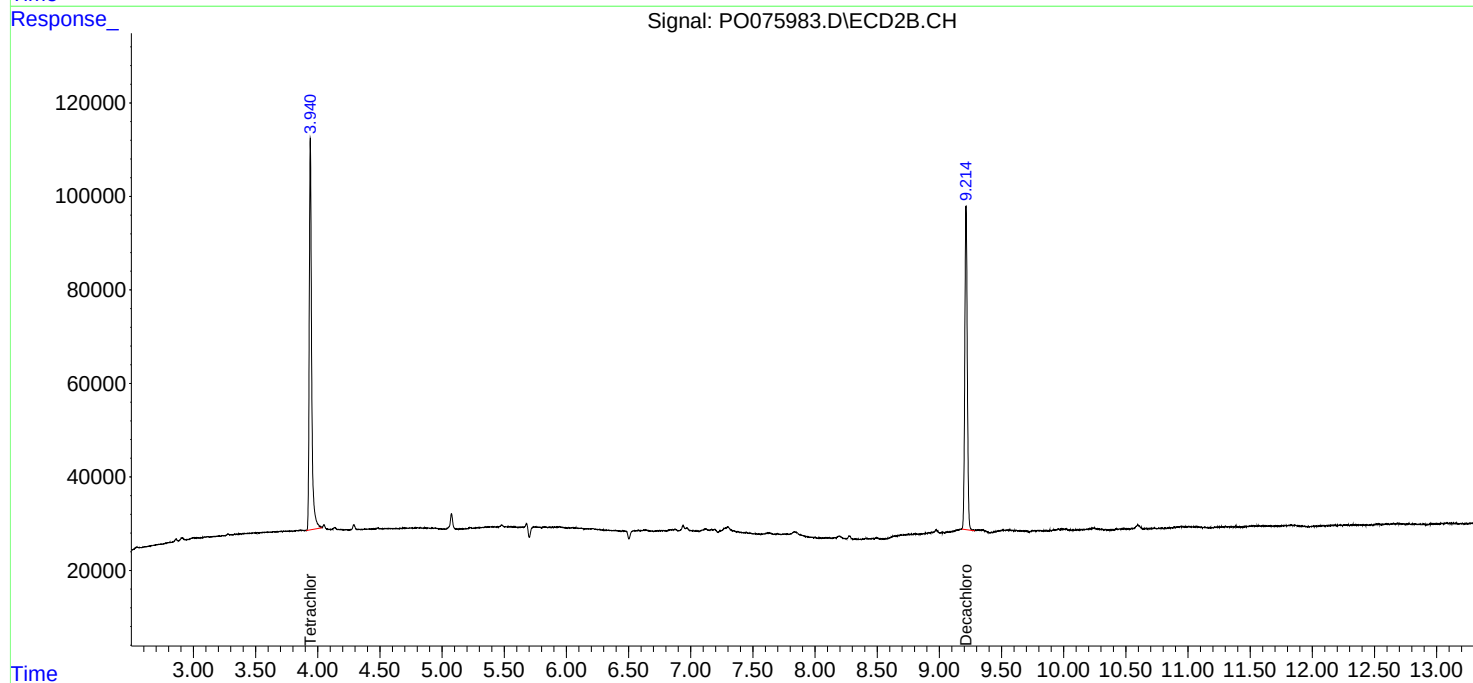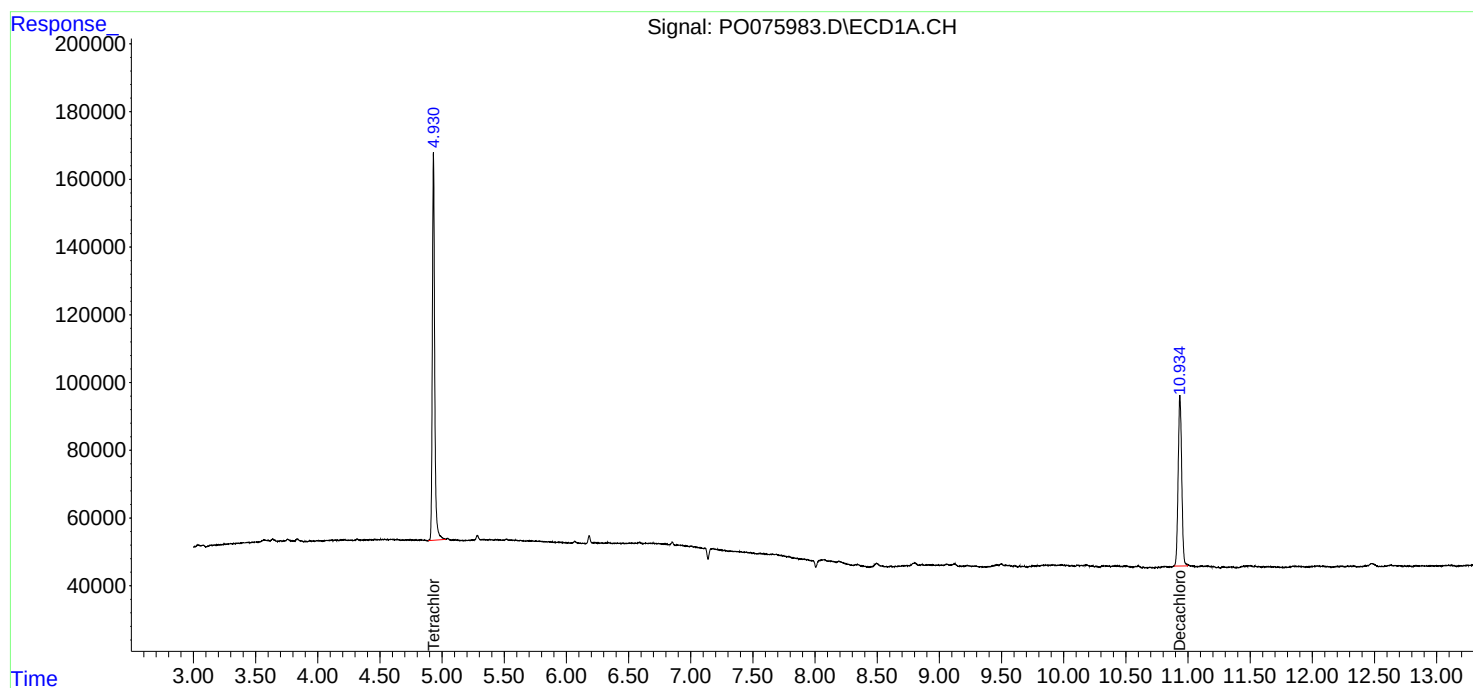

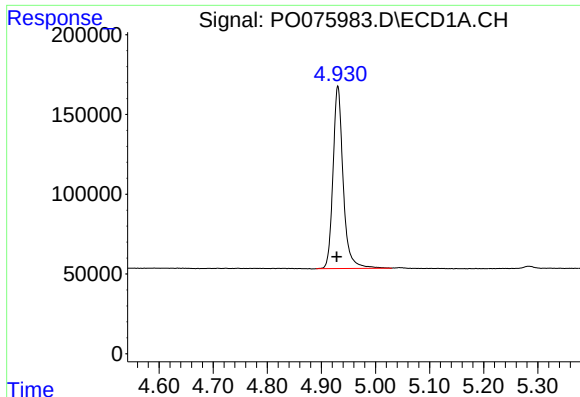


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: 0.002 min
Response: 1491892
Conc: 25.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
3/10/2021 2:02:42 PM

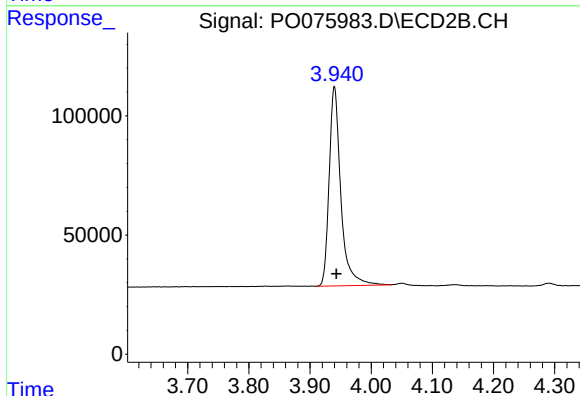


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.003 min
Response: 1109143
Conc: 24.86 ng/ml

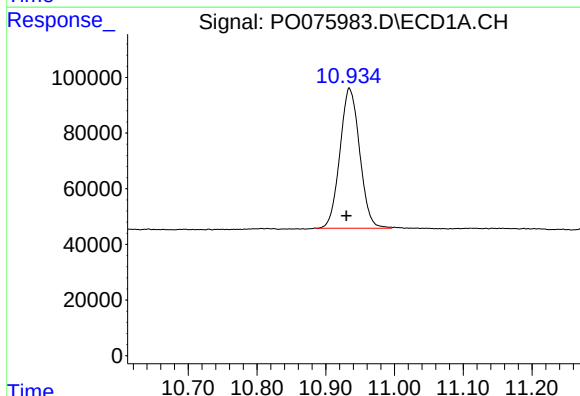

#2 Decachlorobiphenyl

R.T.: 10.934 min
Delta R.T.: 0.004 min
Response: 1003581
Conc: 30.55 ng/ml m

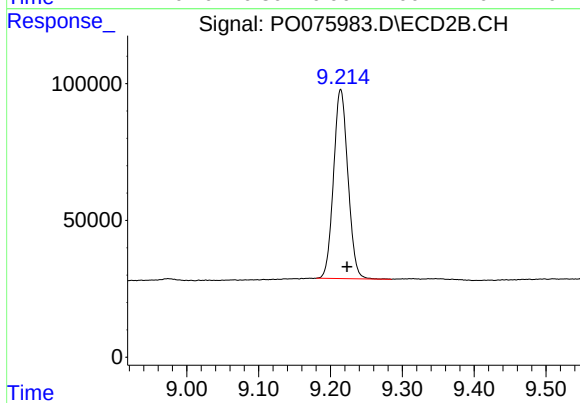

#2 Decachlorobiphenyl

R.T.: 9.214 min
Delta R.T.: -0.009 min
Response: 962532
Conc: 26.47 ng/ml