

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
 Data File : P0085180.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2022 13:45
 Operator : YP\AJ
 Sample : N1645-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 02:04:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.499	3.591	2154032	680954	12.545	14.923
2) SA Decachlor...	10.415	8.611	938764	642465	14.336	16.875
Target Compounds						
8) L2 AR-1221-1	4.710	3.807	126123	8621	68.256	15.640 #
9) L2 AR-1221-2	4.810	3.890	54913	21987	41.282	51.715 #
10) L2 AR-1221-3	4.877	3.967	93828	23121	24.052	17.750 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
Data File : P0085180.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2022 13:45
Operator : YP\AJ
Sample : N1645-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 02:04:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

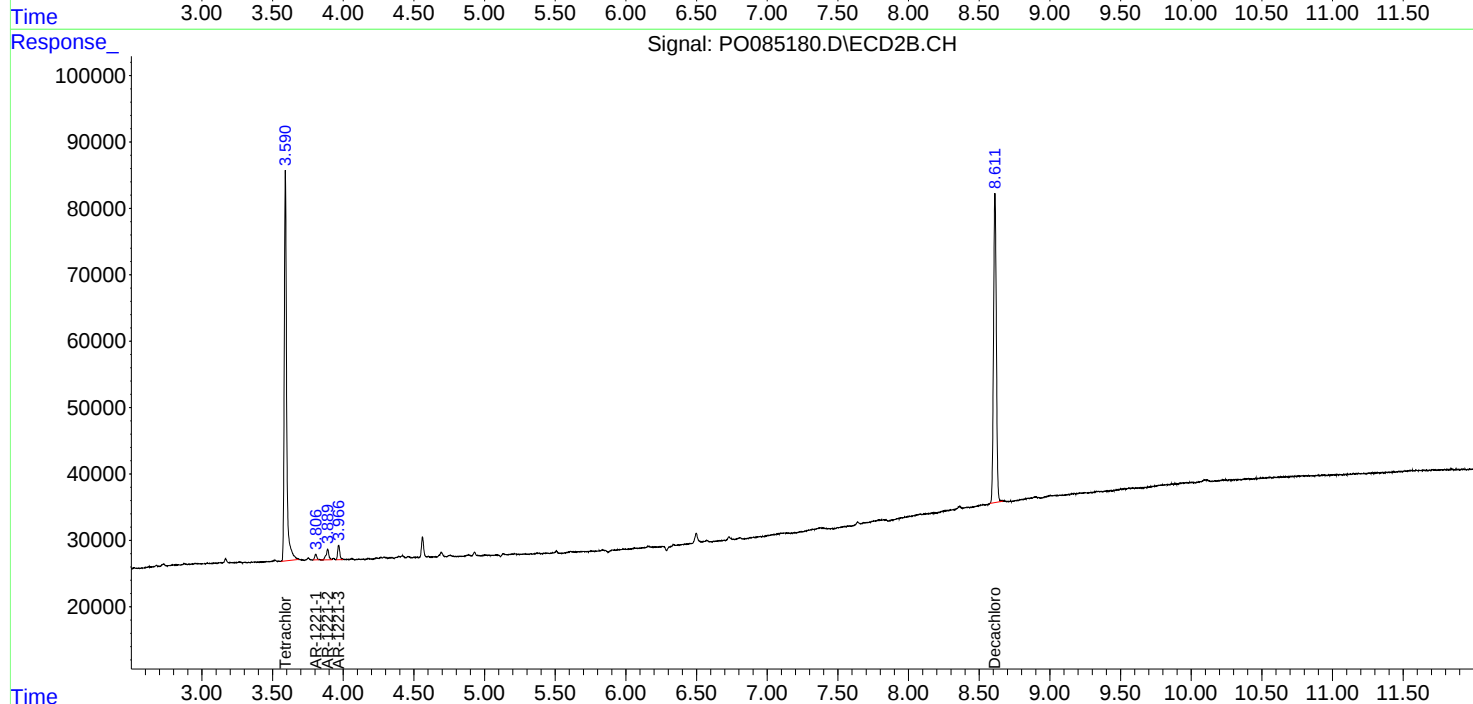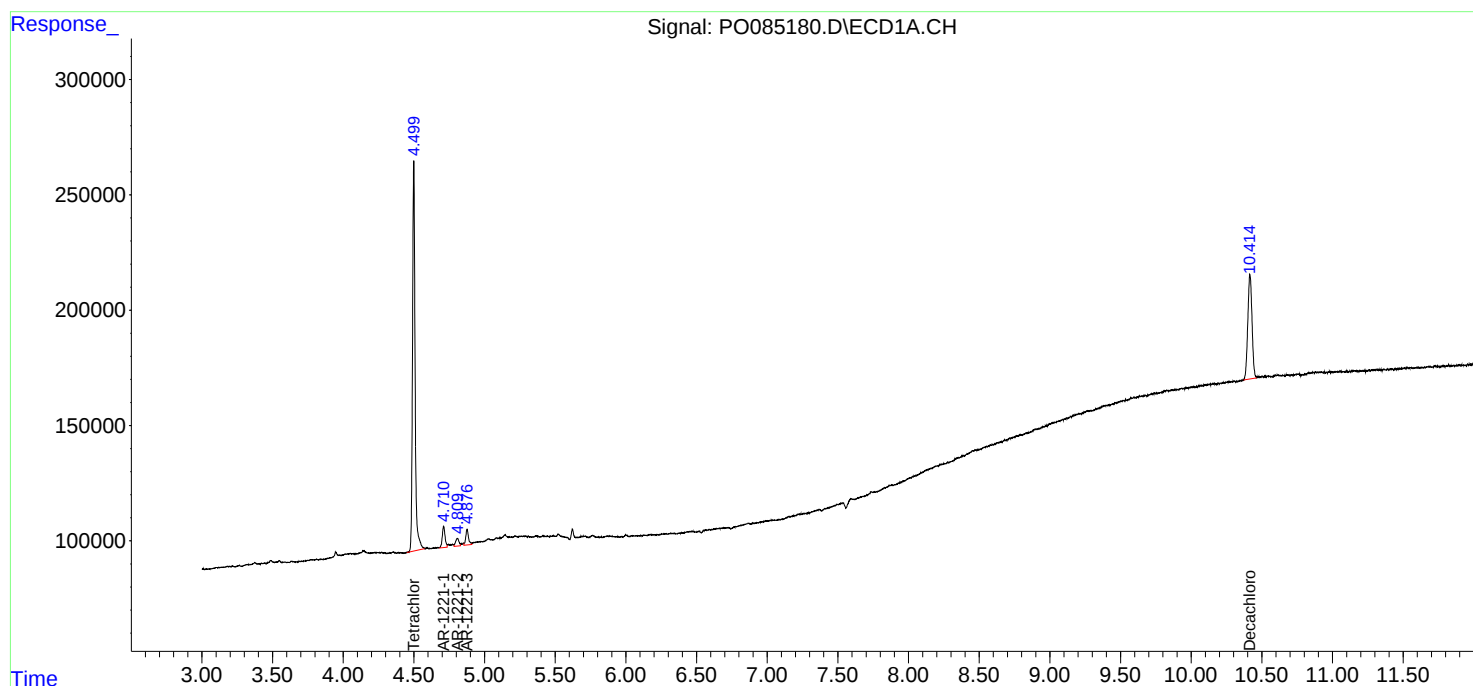


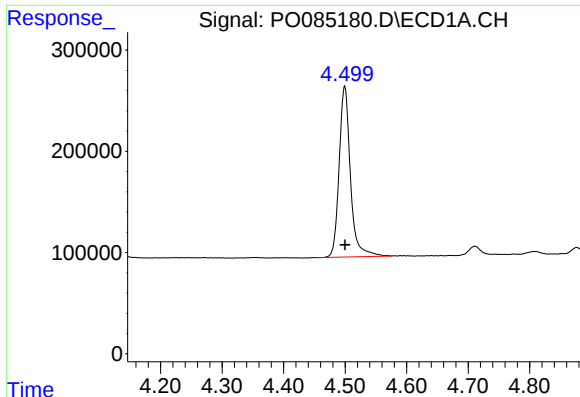

#1 Tetrachloro-m-xylene


R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 2154032
Conc: 12.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

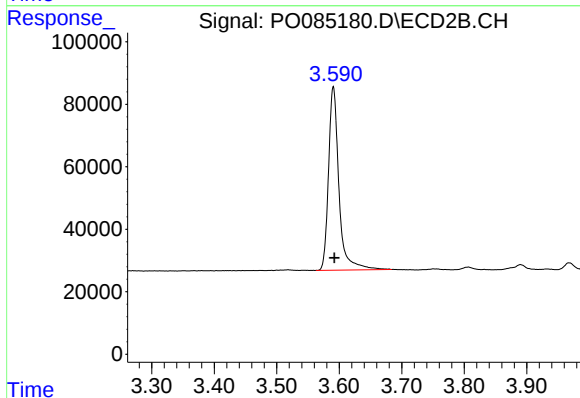


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 680954
Conc: 14.92 ng/ml

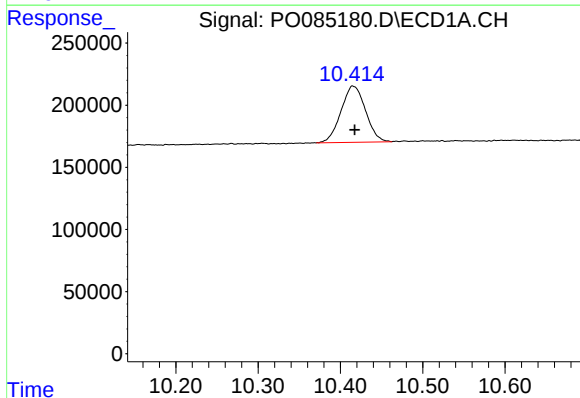


#2 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.003 min
Response: 938764
Conc: 14.34 ng/ml

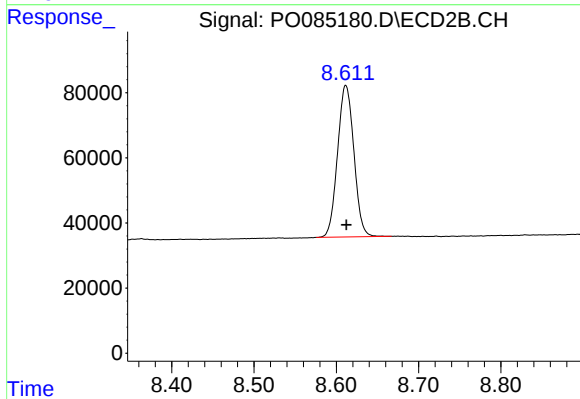

#2 Decachlorobiphenyl


R.T.: 8.611 min
Delta R.T.: 0.000 min
Response: 642465
Conc: 16.87 ng/ml

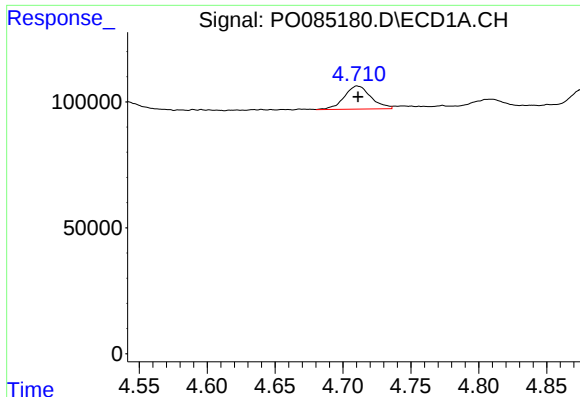

#8 AR-1221-1


R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 126123
Conc: 68.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

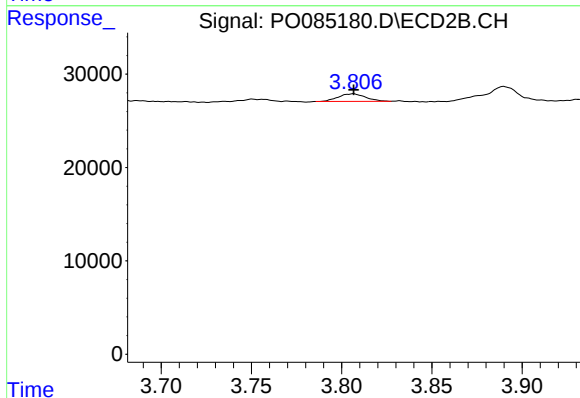


#8 AR-1221-1

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 8621
Conc: 15.64 ng/ml

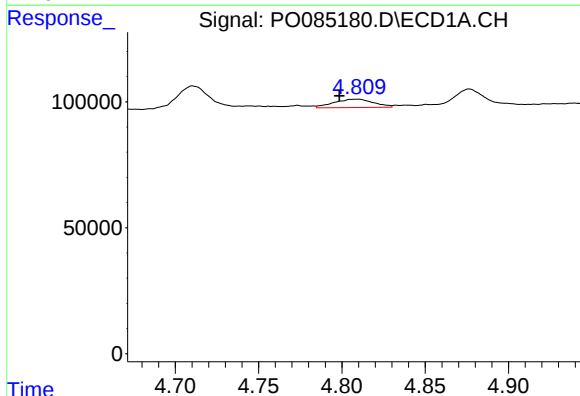


#9 AR-1221-2

R.T.: 4.810 min
Delta R.T.: 0.011 min
Response: 54913
Conc: 41.28 ng/ml

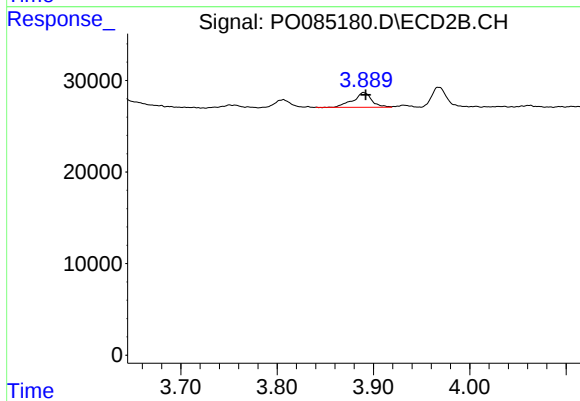

#9 AR-1221-2


R.T.: 3.890 min
Delta R.T.: -0.002 min
Response: 21987
Conc: 51.72 ng/ml

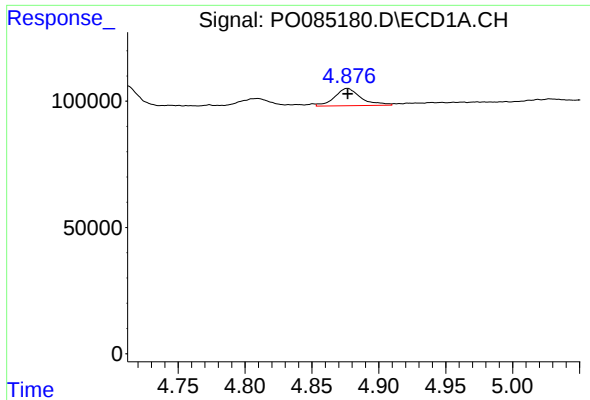

#10 AR-1221-3

R.T.: 4.877 min
Delta R.T.: 0.000 min
Response: 93828
Conc: 24.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

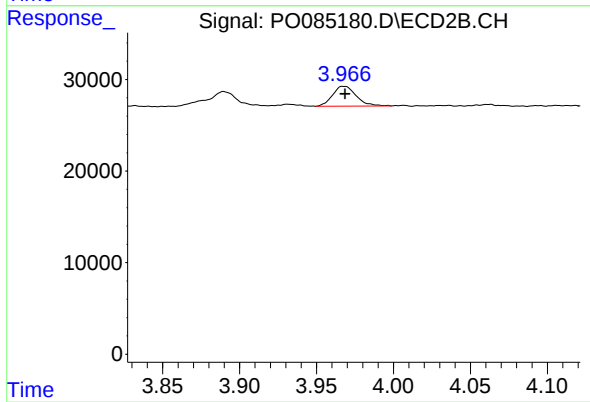

#10 AR-1221-3

R.T.: 3.967 min
Delta R.T.: -0.001 min
Response: 23121
Conc: 17.75 ng/ml