

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
 Data File : P0085189.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2022 16:09
 Operator : YP\AJ
 Sample : PB143214BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB143214BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 02:09:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.499	3.591	3271538	1058835	19.053	23.204
2)	SA Decachlor...	10.416	8.612	1449115	941365	22.129	24.726

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
Data File : P0085189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2022 16:09
Operator : YP\AJ
Sample : PB143214BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB143214BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 02:09:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

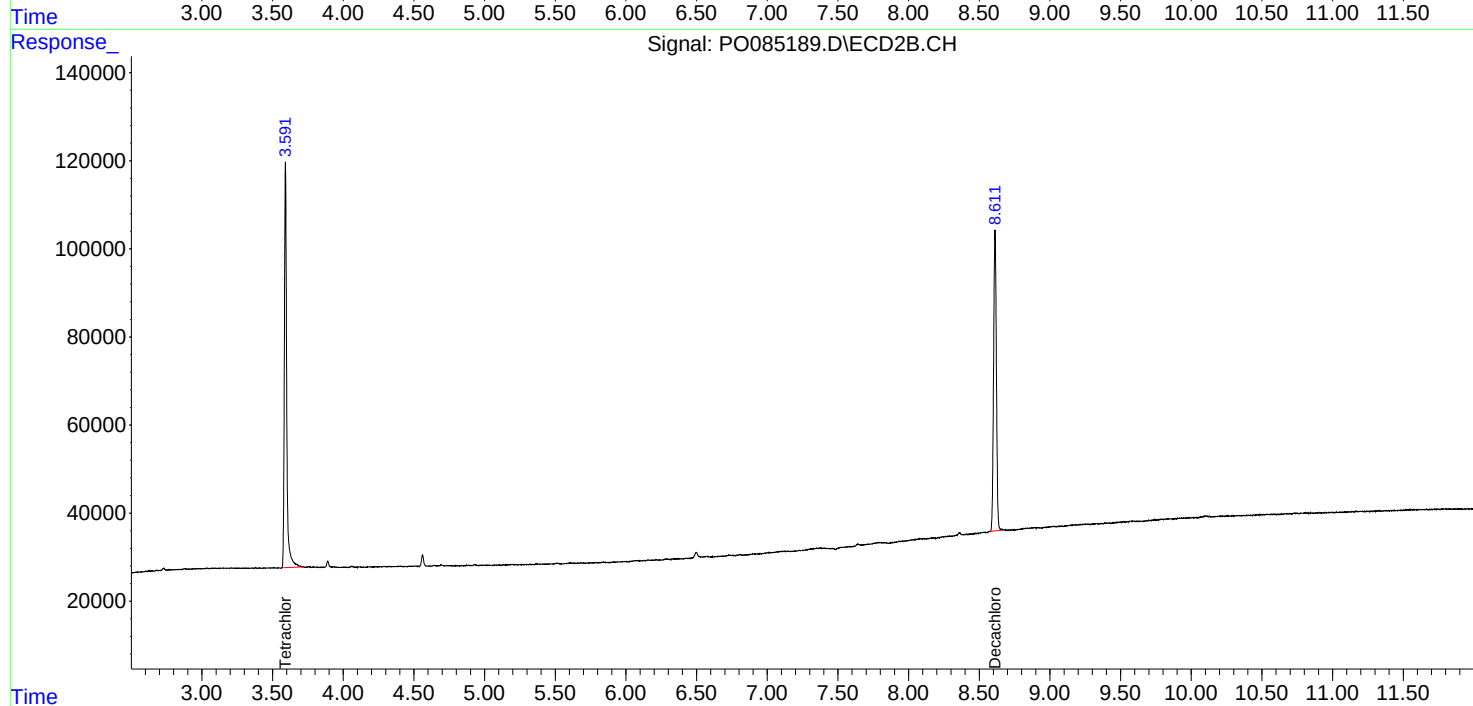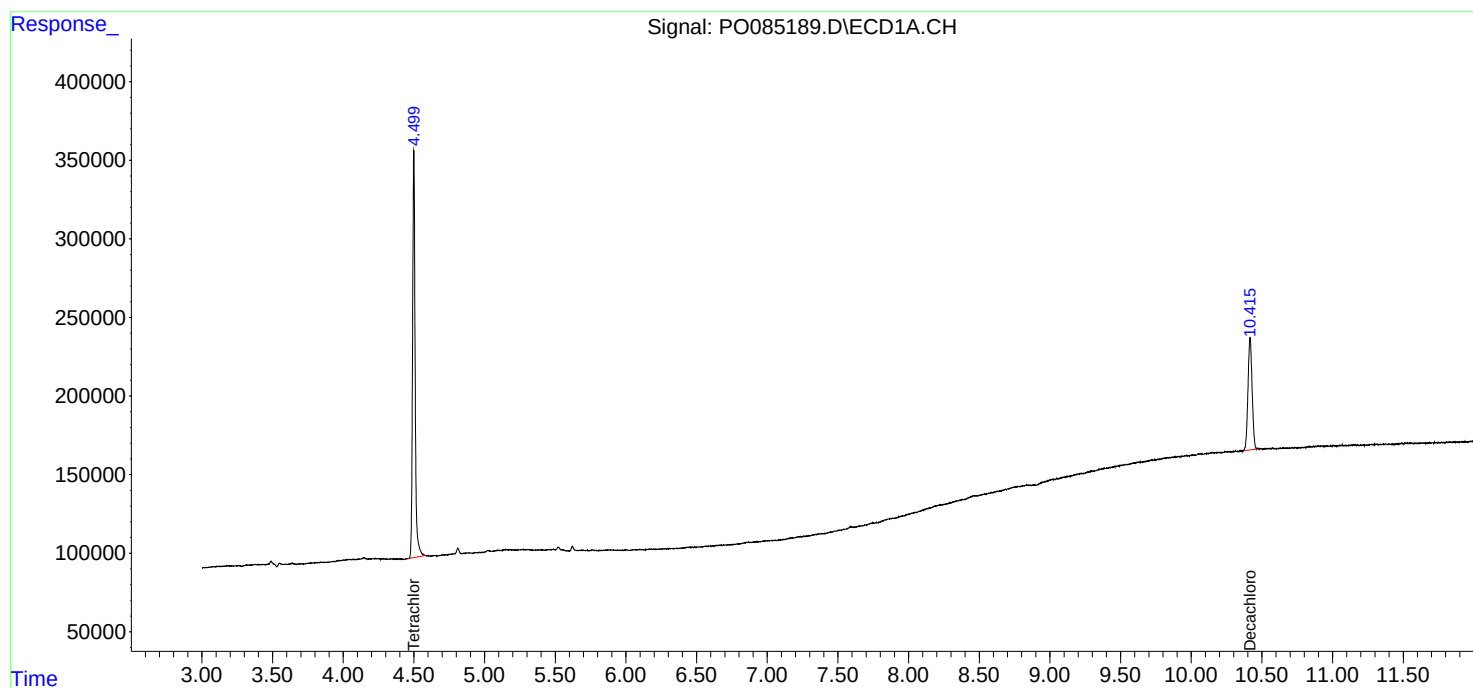


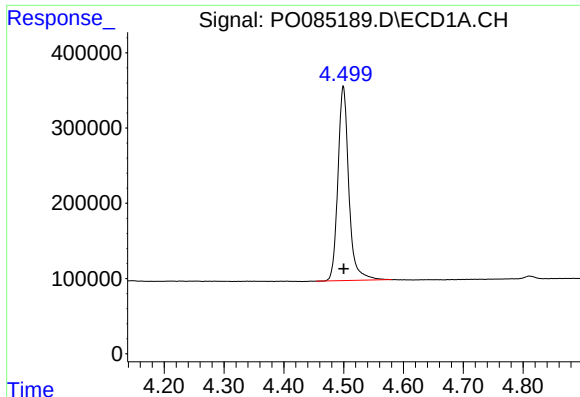

#1 Tetrachloro-m-xylene


R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 3271538
Conc: 19.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB143214BL

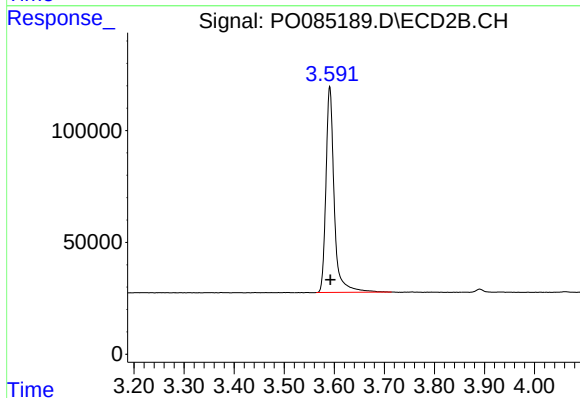


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.001 min
Response: 1058835
Conc: 23.20 ng/ml

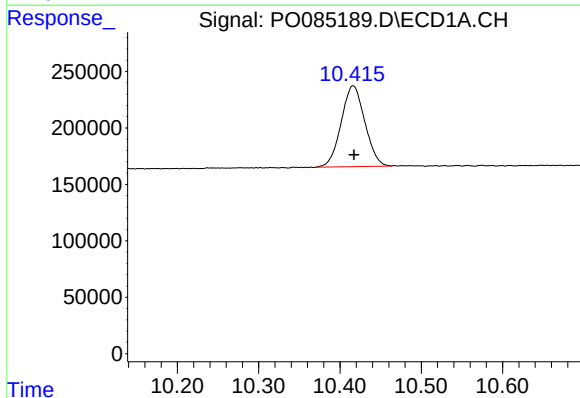

#2 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.001 min
Response: 1449115
Conc: 22.13 ng/ml

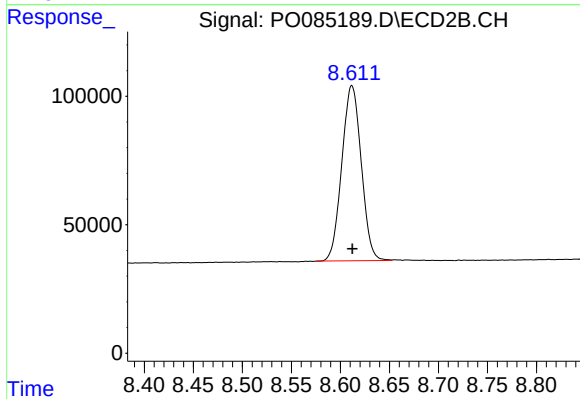

#2 Decachlorobiphenyl

R.T.: 8.612 min
Delta R.T.: 0.000 min
Response: 941365
Conc: 24.73 ng/ml