

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
 Data File : P0085243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2022 7:32
 Operator : YP\AJ
 Sample : N1645-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 07:53:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.589	2873695	902330	16.736	19.774
2) SA Decachlor...	10.409	8.606	1271882	824803	19.423	21.664
Target Compounds						
11) L3 AR-1232-1	4.874	3.966	80069	24881	28.360m	25.050
12) L3 AR-1232-2	5.413	4.695	39720	35741	24.656m	34.146 #
13) L3 AR-1232-3	5.708	4.871	57312	14756	20.247	25.917 #
14) L3 AR-1232-4	5.872	4.957	28238	11937	20.706	22.603
15) L3 AR-1232-5	5.965	5.127	15868	13041	15.425m	22.072 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
Data File : P0085243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2022 7:32
Operator : YP\AJ
Sample : N1645-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 07:53:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

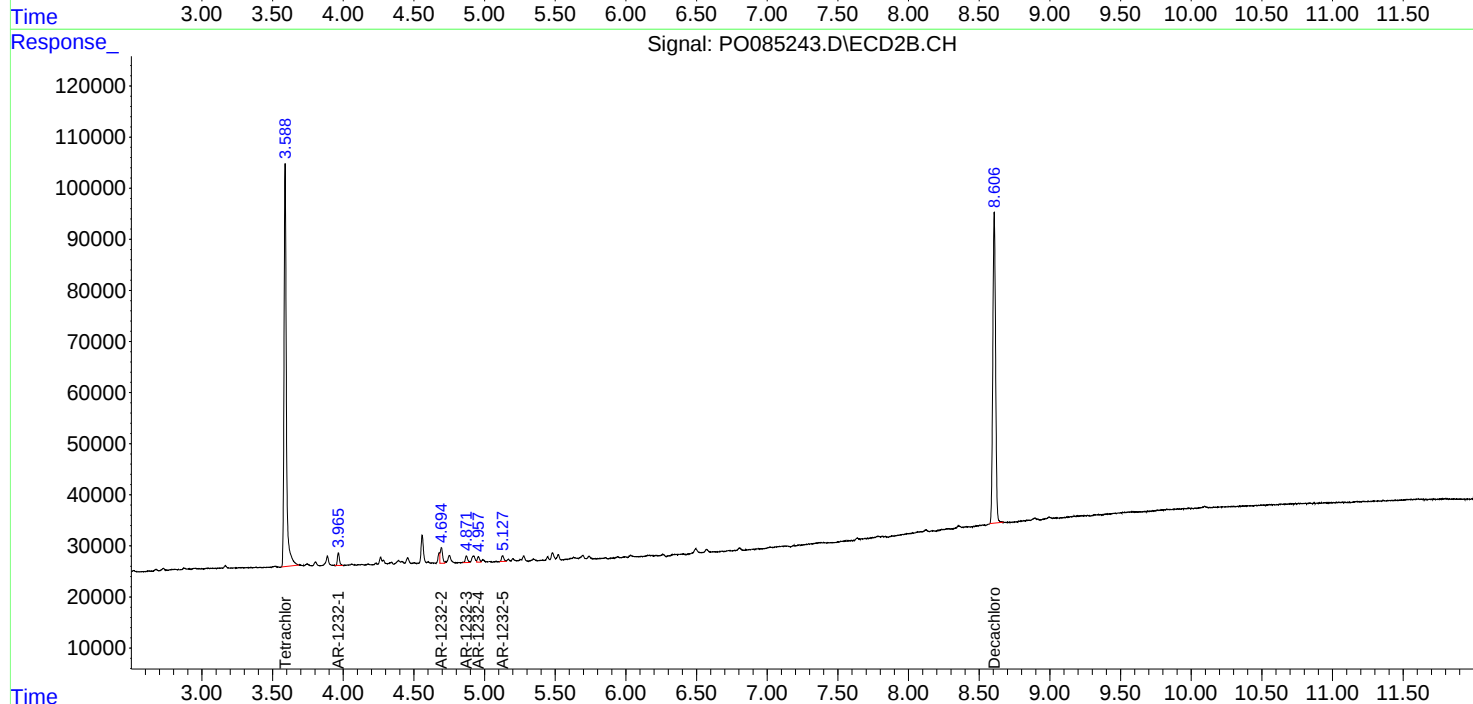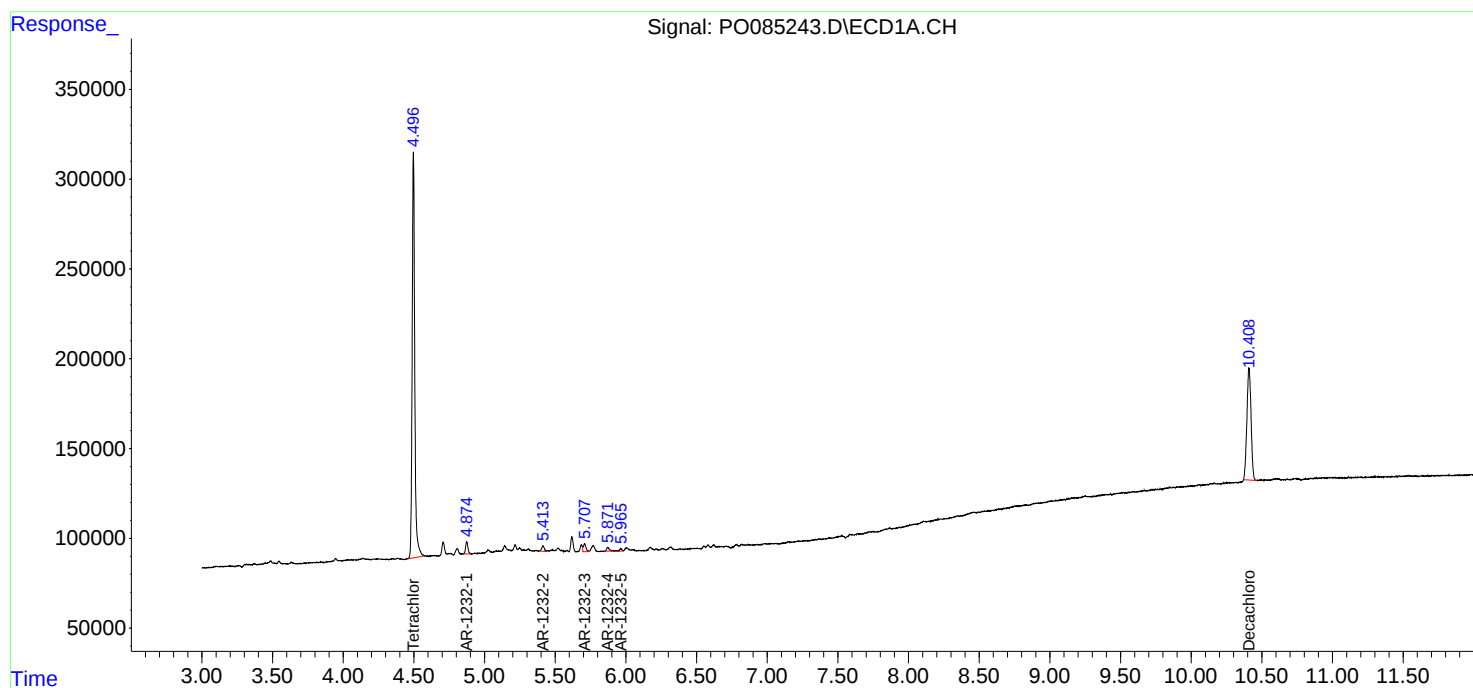


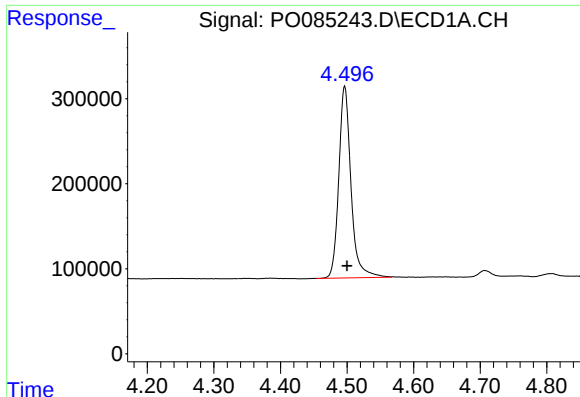

#1 Tetrachloro-m-xylene


R.T.: 4.497 min
Delta R.T.: -0.003 min
Response: 2873695
Conc: 16.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

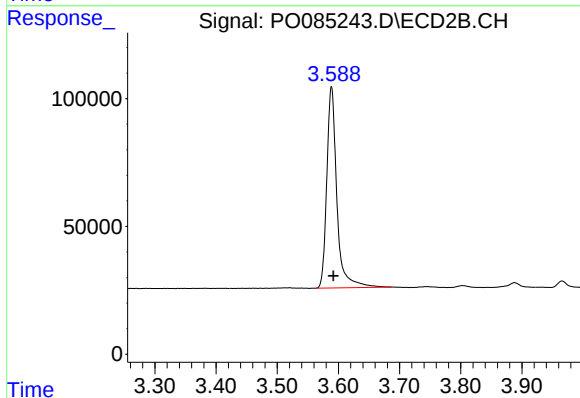


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.003 min
Response: 902330
Conc: 19.77 ng/ml

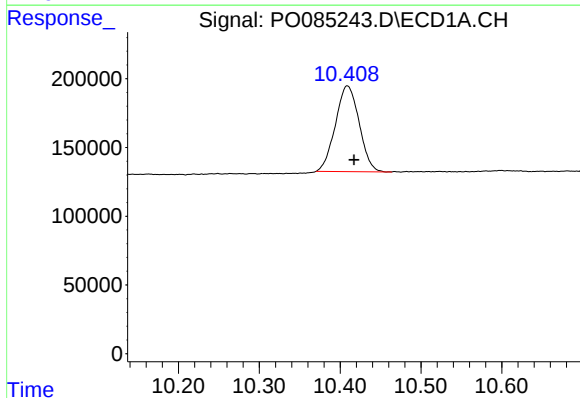


#2 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: -0.008 min
Response: 1271882
Conc: 19.42 ng/ml

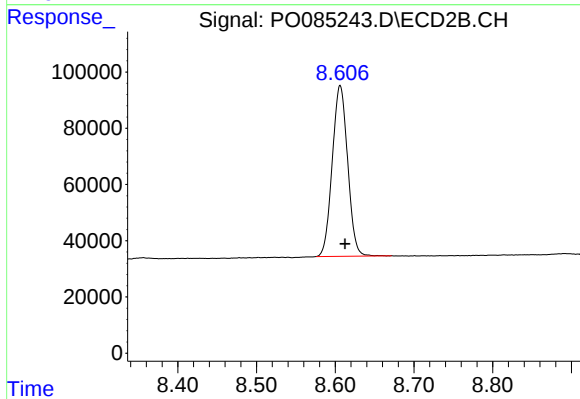

#2 Decachlorobiphenyl


R.T.: 8.606 min
Delta R.T.: -0.006 min
Response: 824803
Conc: 21.66 ng/ml

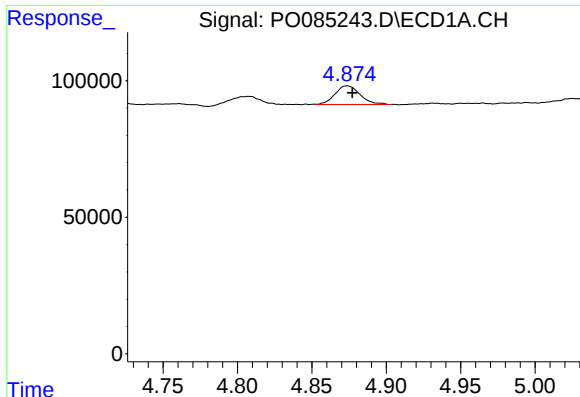

#11 AR-1232-1


R.T.: 4.874 min
Delta R.T.: -0.004 min
Response: 80069
Conc: 28.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

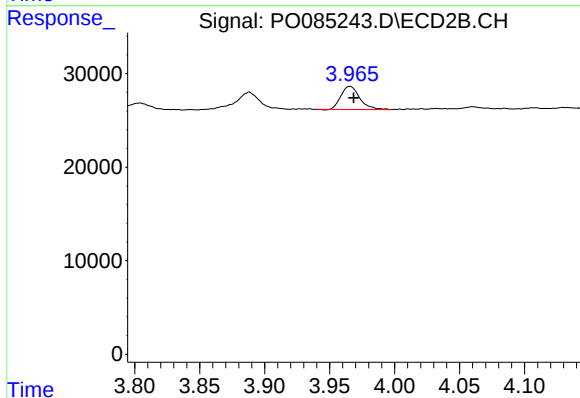


#11 AR-1232-1

R.T.: 3.966 min
Delta R.T.: -0.003 min
Response: 24881
Conc: 25.05 ng/ml

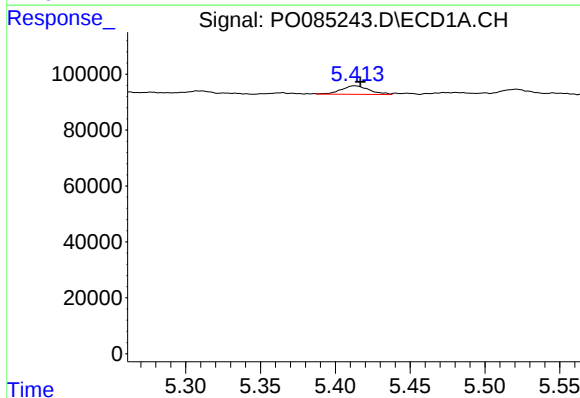


#12 AR-1232-2

R.T.: 5.413 min
Delta R.T.: -0.004 min
Response: 39720
Conc: 24.66 ng/ml m

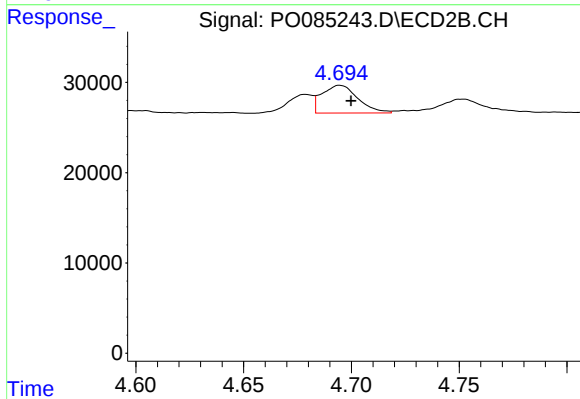

#12 AR-1232-2


R.T.: 4.695 min
Delta R.T.: -0.005 min
Response: 35741
Conc: 34.15 ng/ml

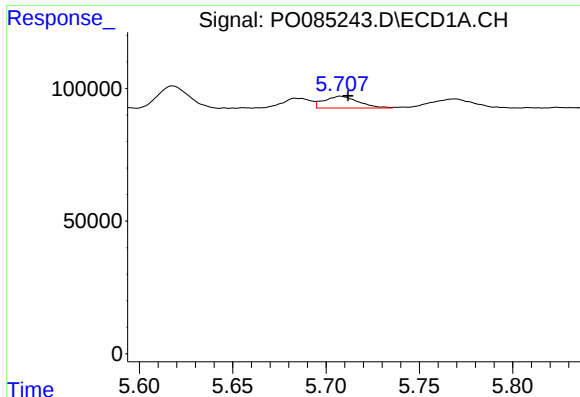

#13 AR-1232-3


R.T.: 5.708 min
Delta R.T.: -0.004 min
Response: 57312
Conc: 20.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

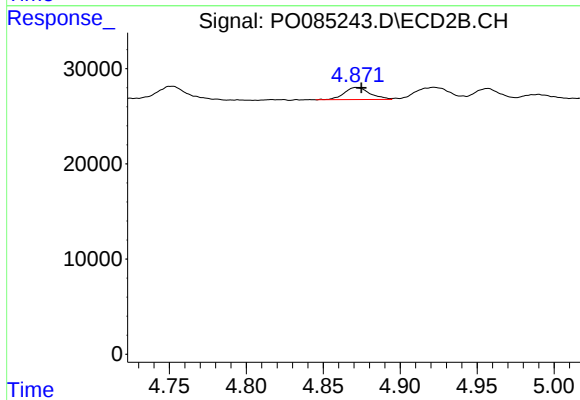


#13 AR-1232-3

R.T.: 4.871 min
Delta R.T.: -0.003 min
Response: 14756
Conc: 25.92 ng/ml

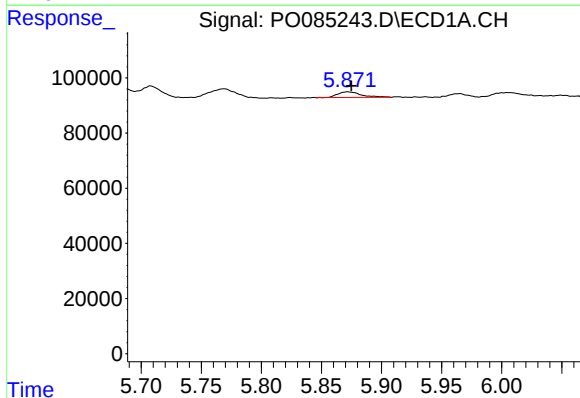


#14 AR-1232-4

R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 28238
Conc: 20.71 ng/ml

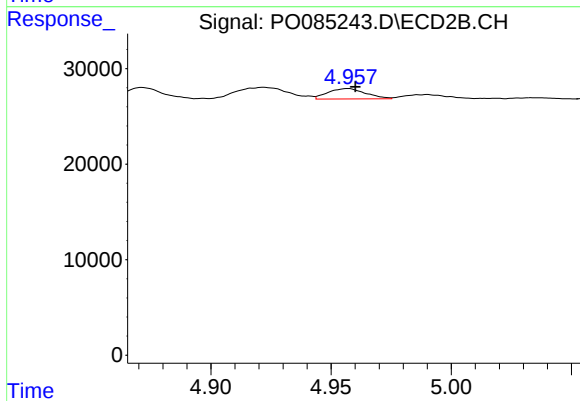

#14 AR-1232-4


R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 11937
Conc: 22.60 ng/ml

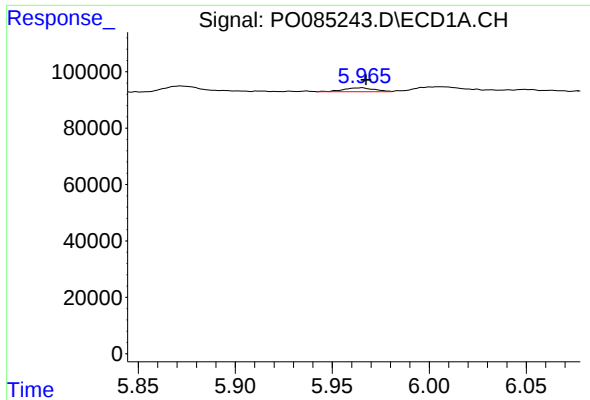

#15 AR-1232-5

R.T.: 5.965 min
Delta R.T.: -0.002 min
Response: 15868
Conc: 15.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

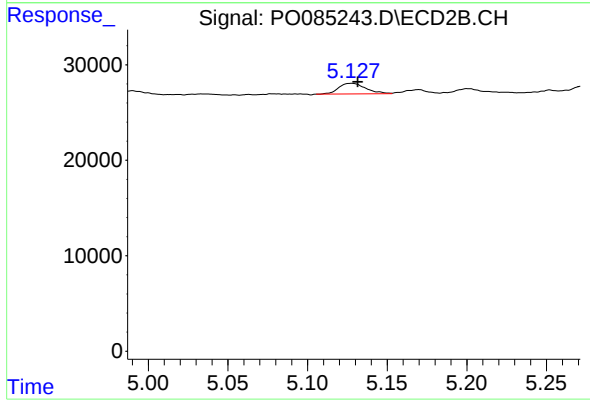

#15 AR-1232-5

R.T.: 5.127 min
Delta R.T.: -0.004 min
Response: 13041
Conc: 22.07 ng/ml