

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
 Data File : P0085247.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2022 8:35
 Operator : YP\AJ
 Sample : N1645-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:29:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.496	3.589	2808766	880820	16.358	19.303
2) SA Decachlor...	10.405	8.606	1297637	817296	19.816m	21.467
Target Compounds						
36) L8 AR-1262-1	7.937	6.681	113751	46616	24.966	27.136
37) L8 AR-1262-2	8.500	6.980	205574	78895	25.044	27.395
38) L8 AR-1262-3	8.824	7.509	112697	64685	21.068	28.626 #
39) L8 AR-1262-4	8.923	7.572	53575	108905	21.539	26.473
40) L8 AR-1262-5	9.607	8.069	67493	49238	24.392	26.438



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
Data File : P0085247.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2022 8:35
Operator : YP\AJ
Sample : N1645-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:29:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

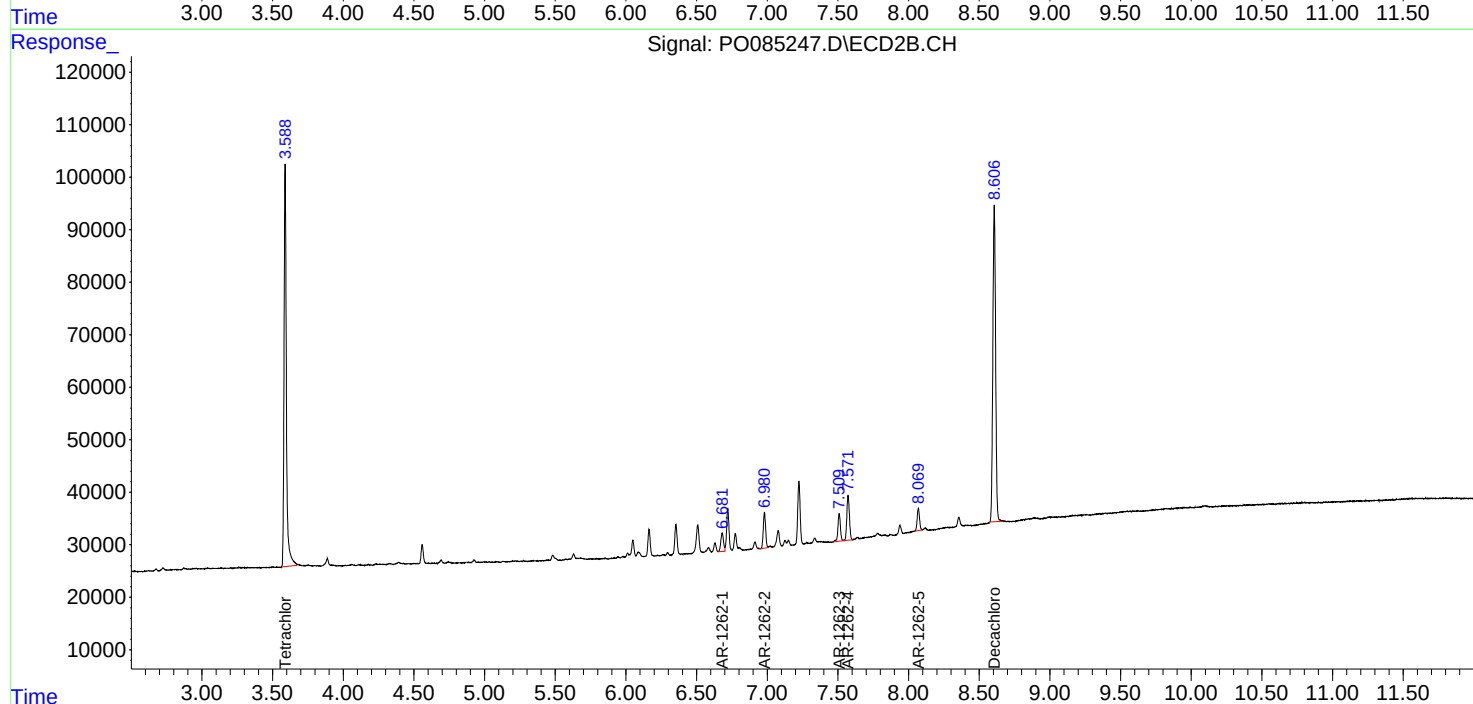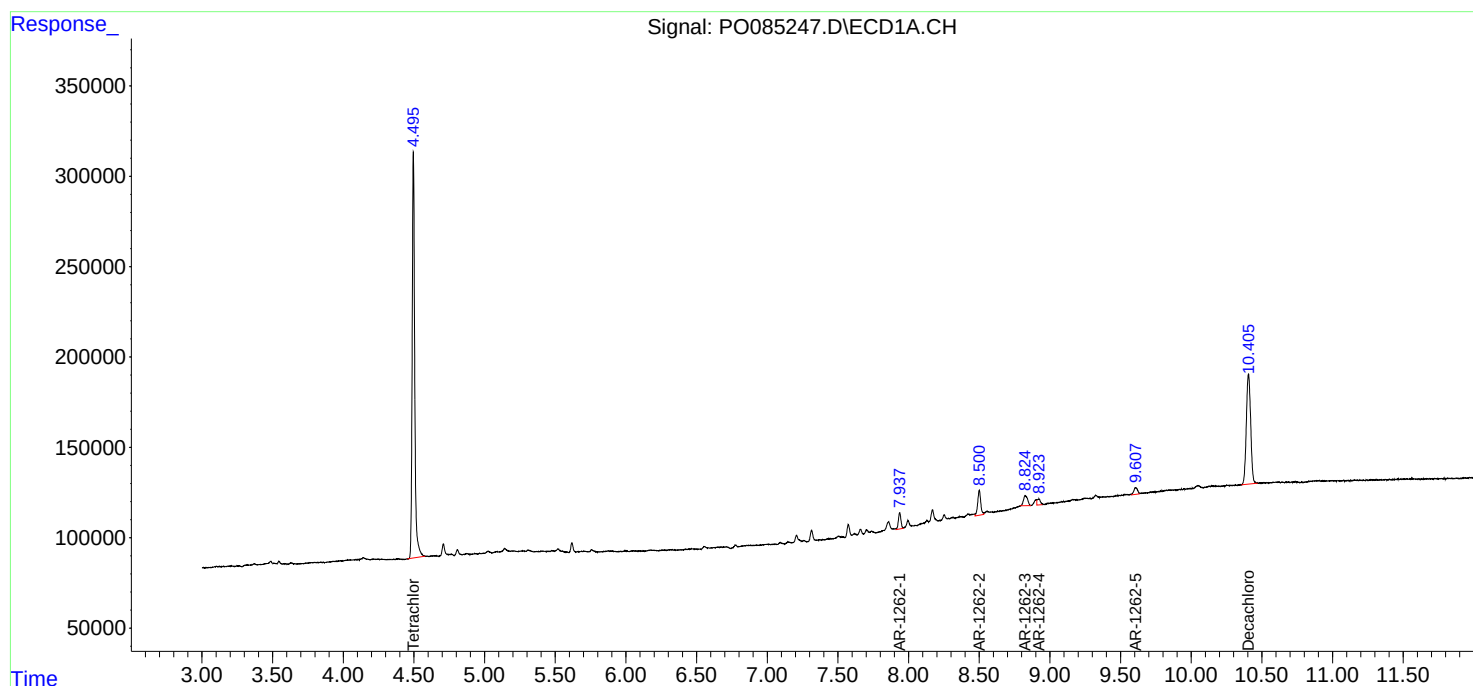


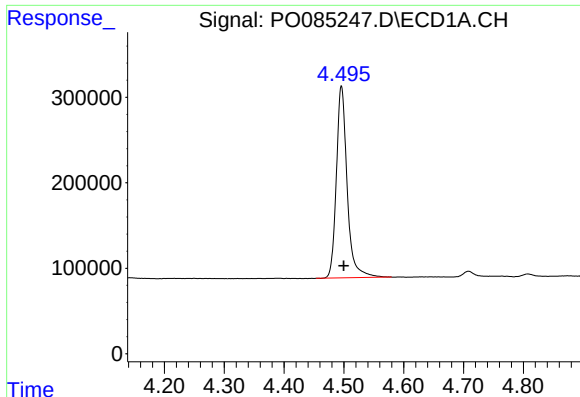

#1 Tetrachloro-m-xylene


R.T.: 4.496 min
Delta R.T.: -0.004 min
Response: 2808766
Conc: 16.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

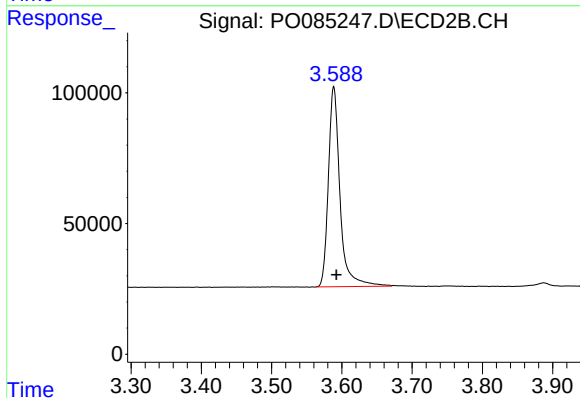


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 880820
Conc: 19.30 ng/ml

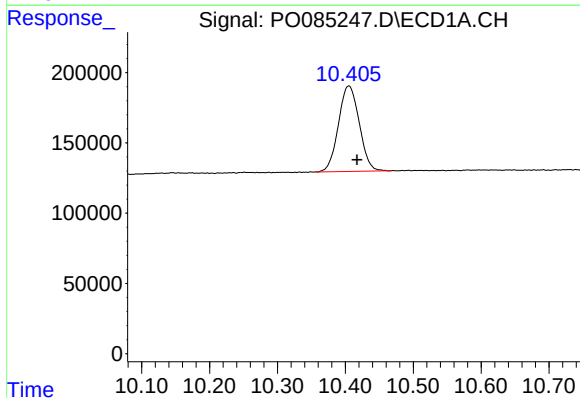


#2 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.012 min
Response: 1297637
Conc: 19.82 ng/ml m

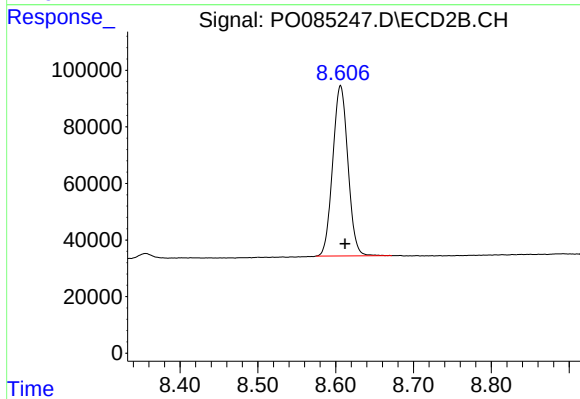

#2 Decachlorobiphenyl


R.T.: 8.606 min
Delta R.T.: -0.006 min
Response: 817296
Conc: 21.47 ng/ml

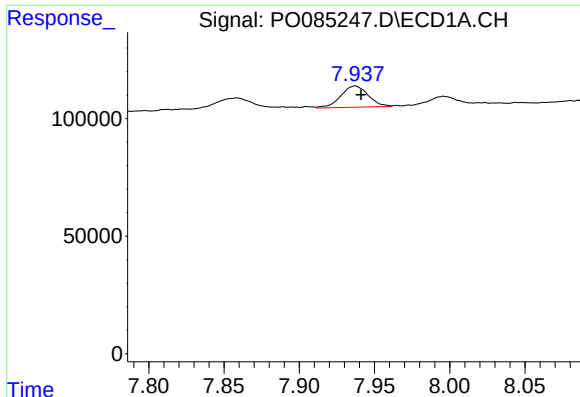

#36 AR-1262-1


R.T.: 7.937 min
Delta R.T.: -0.004 min
Response: 113751
Conc: 24.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

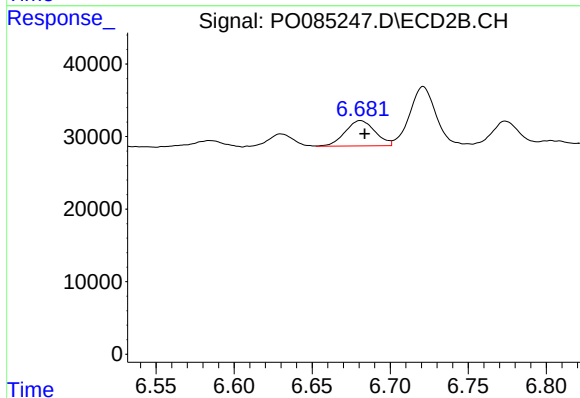


#36 AR-1262-1

R.T.: 6.681 min
Delta R.T.: -0.003 min
Response: 46616
Conc: 27.14 ng/ml

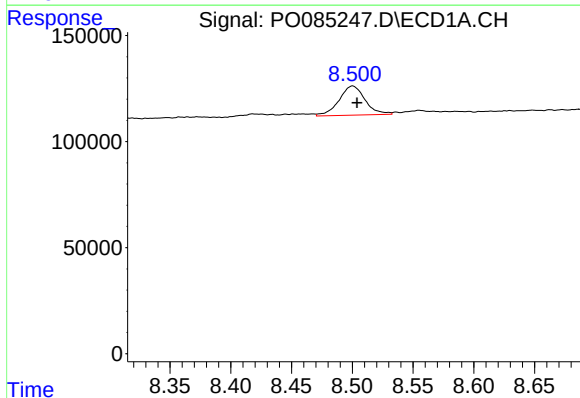


#37 AR-1262-2

R.T.: 8.500 min
Delta R.T.: -0.003 min
Response: 205574
Conc: 25.04 ng/ml

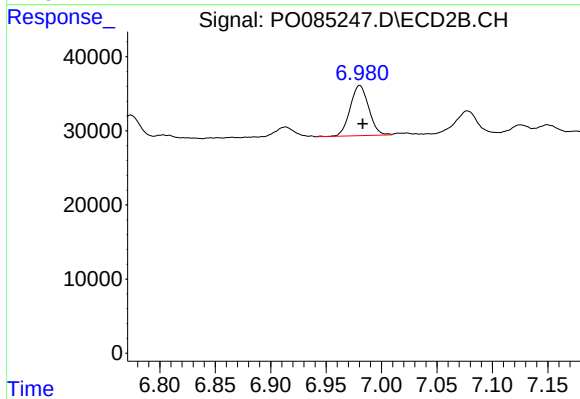

#37 AR-1262-2


R.T.: 6.980 min
Delta R.T.: -0.003 min
Response: 78895
Conc: 27.39 ng/ml

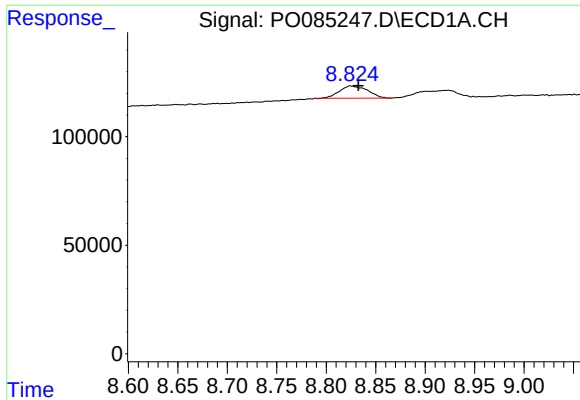

#38 AR-1262-3


R.T.: 8.824 min
Delta R.T.: -0.008 min
Response: 112697
Conc: 21.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

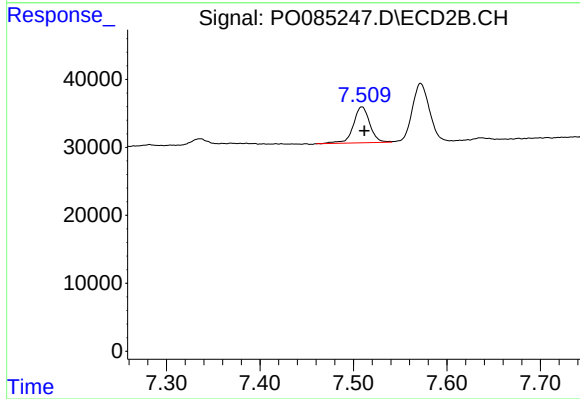


#38 AR-1262-3

R.T.: 7.509 min
Delta R.T.: -0.003 min
Response: 64685
Conc: 28.63 ng/ml

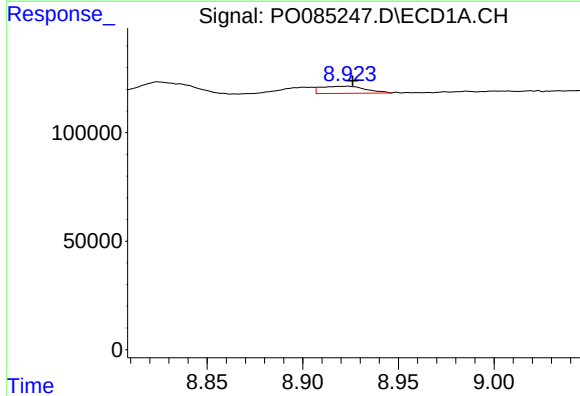


#39 AR-1262-4

R.T.: 8.923 min
Delta R.T.: -0.003 min
Response: 53575
Conc: 21.54 ng/ml

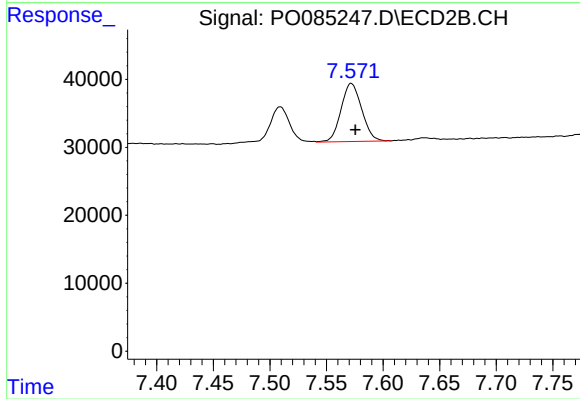

#39 AR-1262-4


R.T.: 7.572 min
Delta R.T.: -0.004 min
Response: 108905
Conc: 26.47 ng/ml

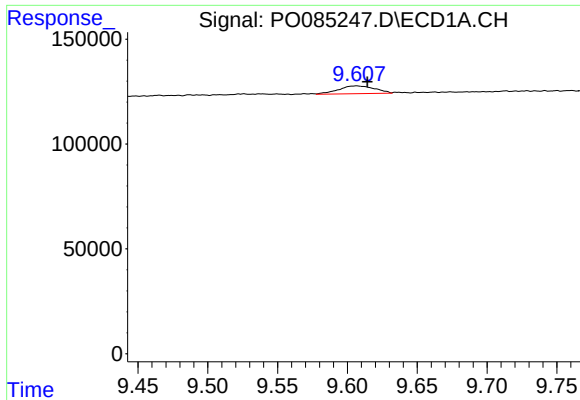

#40 AR-1262-5

R.T.: 9.607 min
Delta R.T.: -0.008 min
Response: 67493
Conc: 24.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

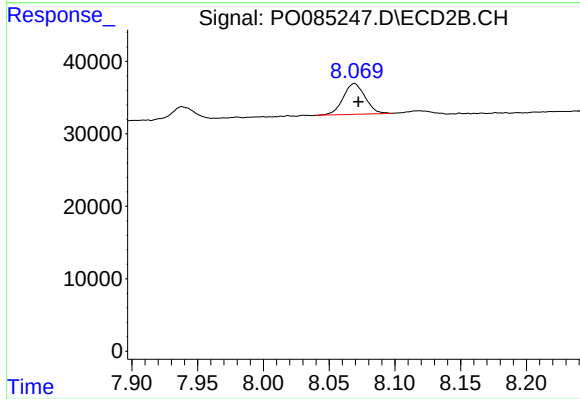

#40 AR-1262-5

R.T.: 8.069 min
Delta R.T.: -0.003 min
Response: 49238
Conc: 26.44 ng/ml