

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
 Data File : P0085248.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2022 8:51
 Operator : YP\AJ
 Sample : N1645-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:30:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.496	3.589	2892603	913587	16.846	20.021
2) SA Decachlor...	10.407	8.606	1439302	898592	21.980m	23.602
Target Compounds						
41) L9 AR-1268-1	8.824	7.509	226887	175518	24.206	26.756
42) L9 AR-1268-2	8.923	7.573	212944	154786	25.091	26.462
43) L9 AR-1268-3	9.163	7.781	184103	135307	25.672	27.288
44) L9 AR-1268-4	9.607	8.069	75234	56227	24.579	26.495
45) L9 AR-1268-5	10.047	8.355	553948	386819	23.230	26.951



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030922\
Data File : P0085248.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2022 8:51
Operator : YP\AJ
Sample : N1645-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:30:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

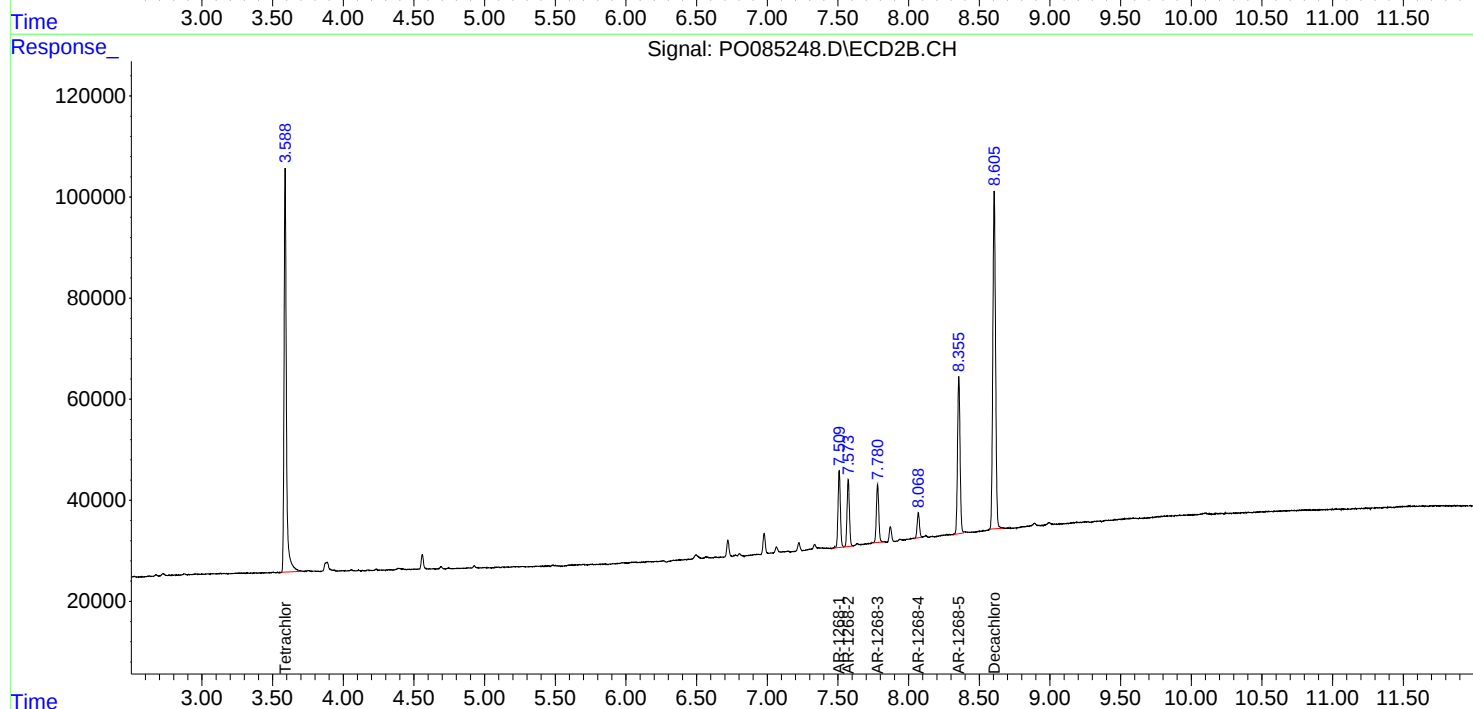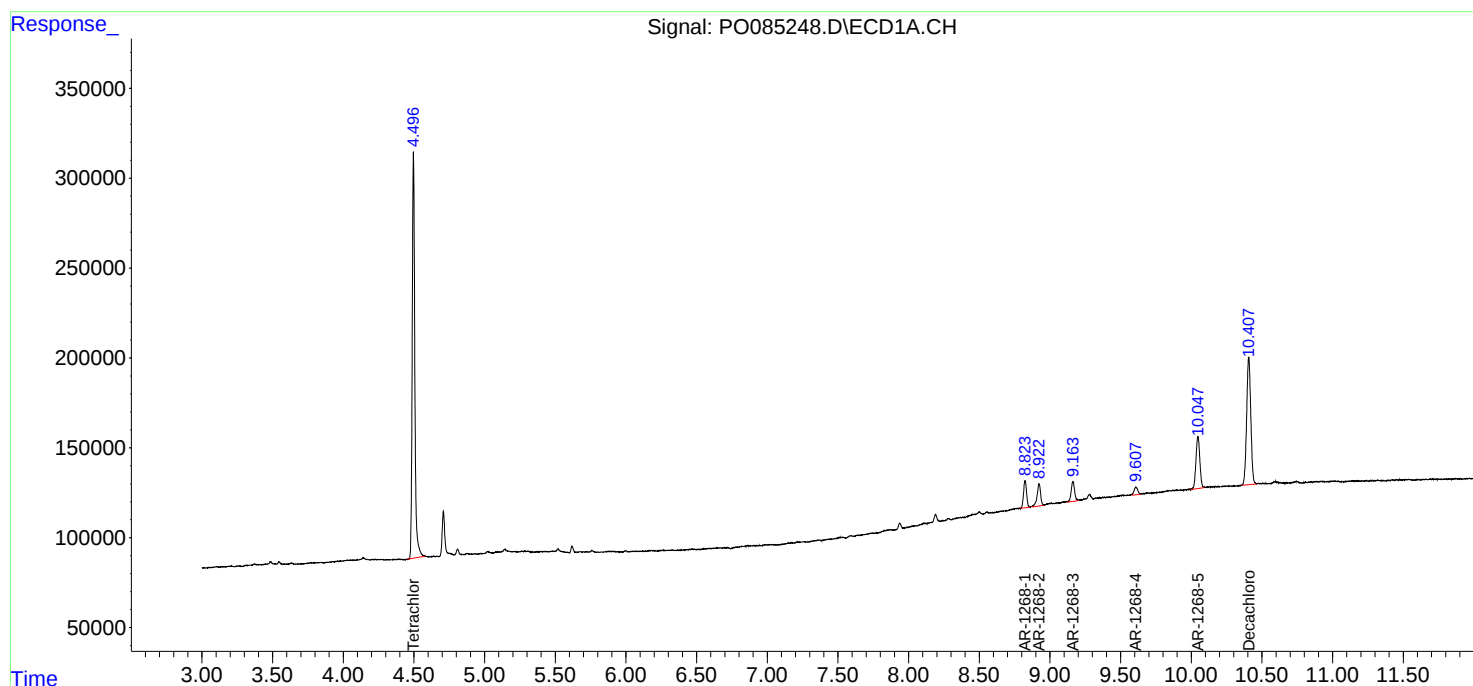


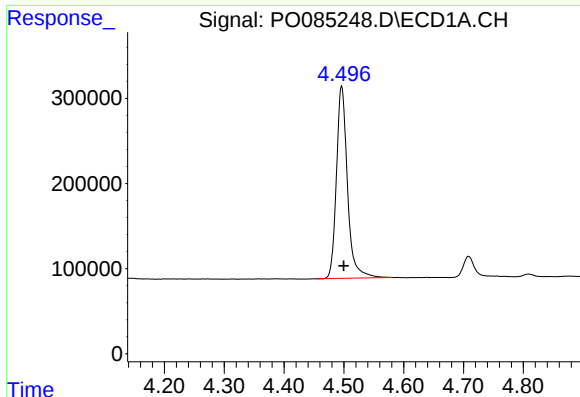

#1 Tetrachloro-m-xylene


R.T.: 4.496 min
Delta R.T.: -0.004 min
Response: 2892603
Conc: 16.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

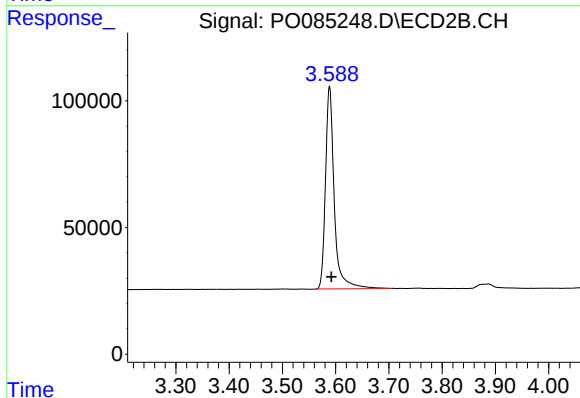


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 913587
Conc: 20.02 ng/ml

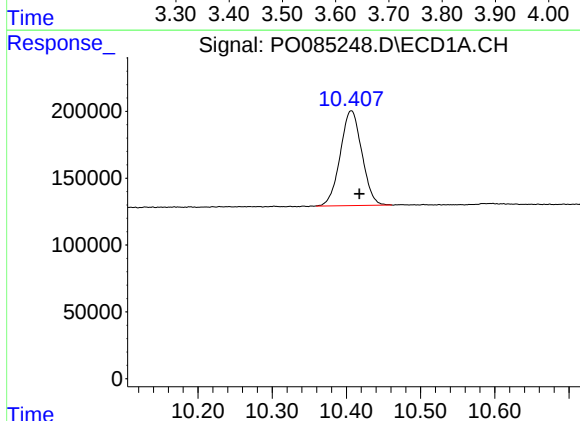


#2 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.011 min
Response: 1439302
Conc: 21.98 ng/ml m

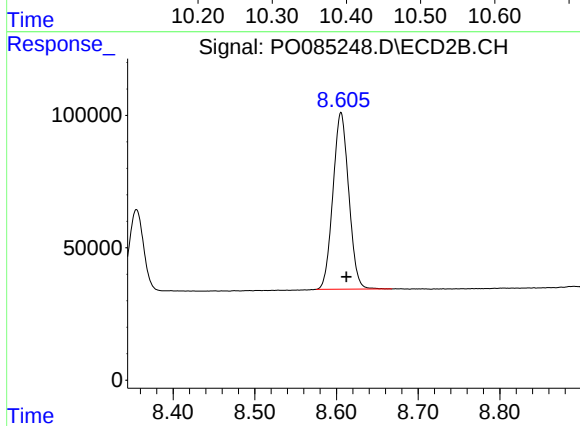

#2 Decachlorobiphenyl


R.T.: 8.606 min
Delta R.T.: -0.007 min
Response: 898592
Conc: 23.60 ng/ml

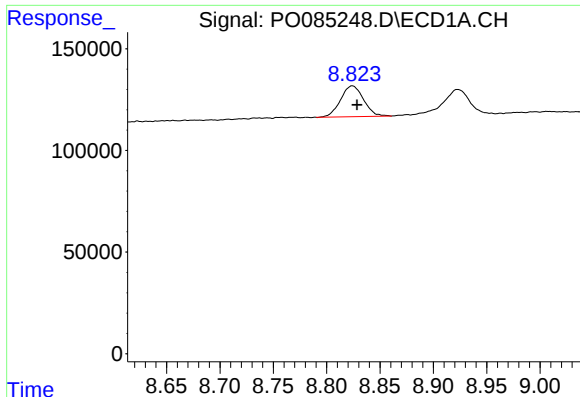

#41 AR-1268-1


R.T.: 8.824 min
Delta R.T.: -0.004 min
Response: 226887
Conc: 24.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

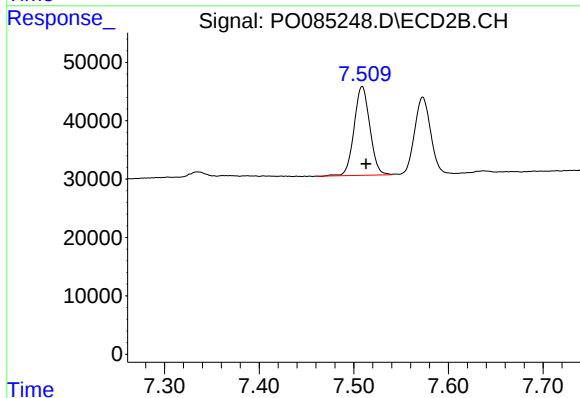


#41 AR-1268-1

R.T.: 7.509 min
Delta R.T.: -0.004 min
Response: 175518
Conc: 26.76 ng/ml

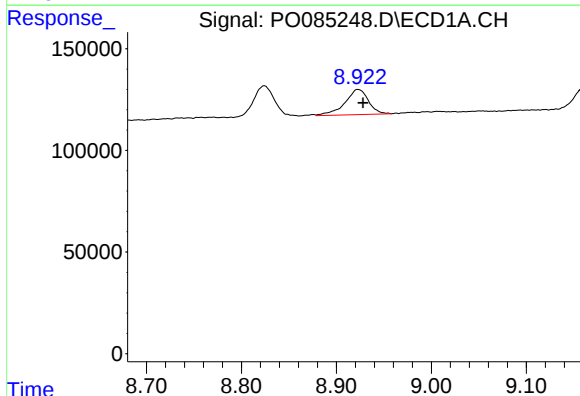


#42 AR-1268-2

R.T.: 8.923 min
Delta R.T.: -0.005 min
Response: 212944
Conc: 25.09 ng/ml

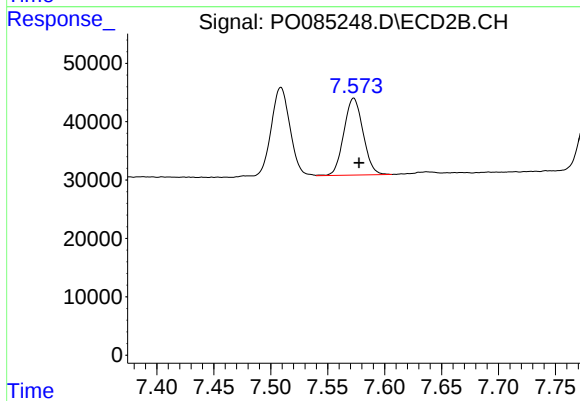

#42 AR-1268-2


R.T.: 7.573 min
Delta R.T.: -0.005 min
Response: 154786
Conc: 26.46 ng/ml

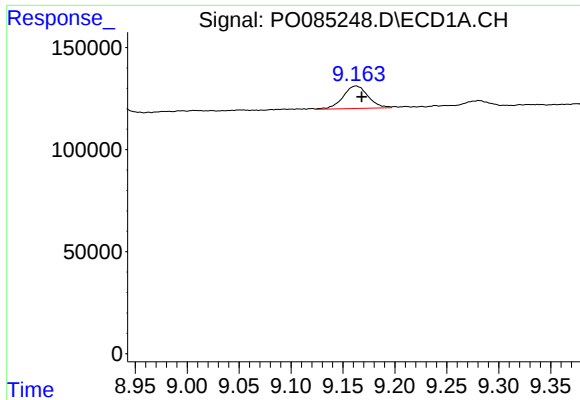

#43 AR-1268-3


R.T.: 9.163 min
Delta R.T.: -0.005 min
Response: 184103
Conc: 25.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

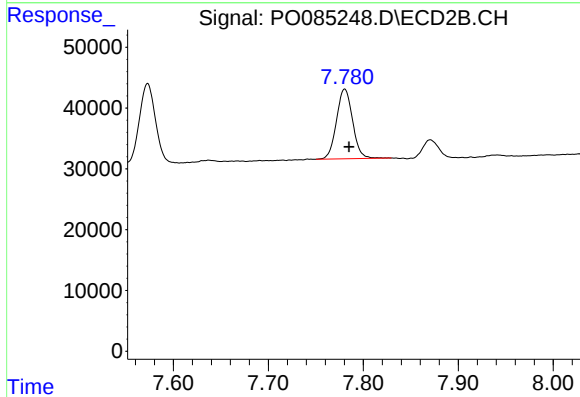


#43 AR-1268-3

R.T.: 7.781 min
Delta R.T.: -0.004 min
Response: 135307
Conc: 27.29 ng/ml

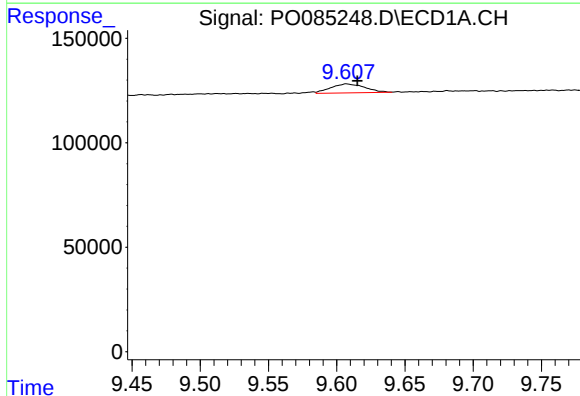


#44 AR-1268-4

R.T.: 9.607 min
Delta R.T.: -0.008 min
Response: 75234
Conc: 24.58 ng/ml

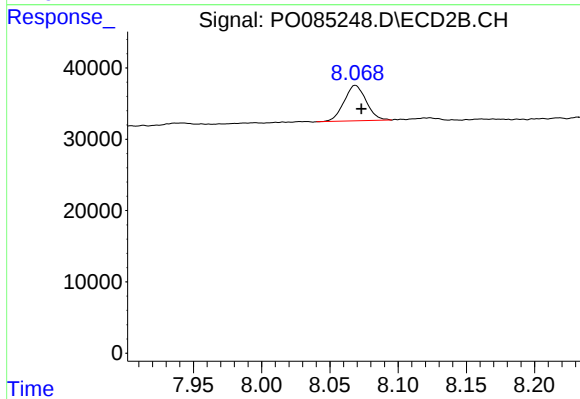

#44 AR-1268-4


R.T.: 8.069 min
Delta R.T.: -0.004 min
Response: 56227
Conc: 26.50 ng/ml

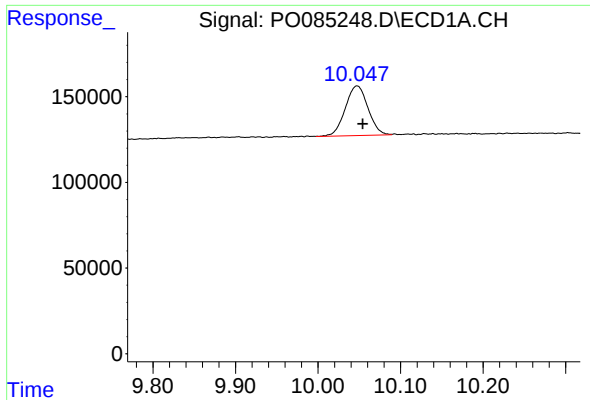

#45 AR-1268-5

R.T.: 10.047 min
Delta R.T.: -0.007 min
Response: 553948
Conc: 23.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

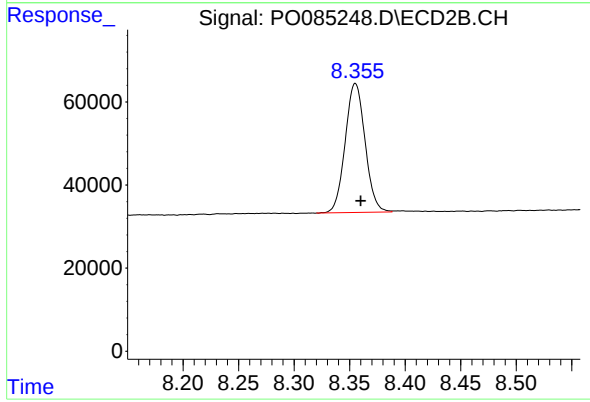

#45 AR-1268-5

R.T.: 8.355 min
Delta R.T.: -0.005 min
Response: 386819
Conc: 26.95 ng/ml