

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031021\
 Data File : P0076021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2021 16:26
 Operator : DD\AJ
 Sample : M1615-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-04-015-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:24:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.940	1471776	1139570	24.691	25.546
2) SA Decachlor...	10.927	9.211	898251	915080	27.343	25.167

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031021\
Data File : P0076021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2021 16:26
Operator : DD\AJ
Sample : M1615-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-04-015-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:24:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

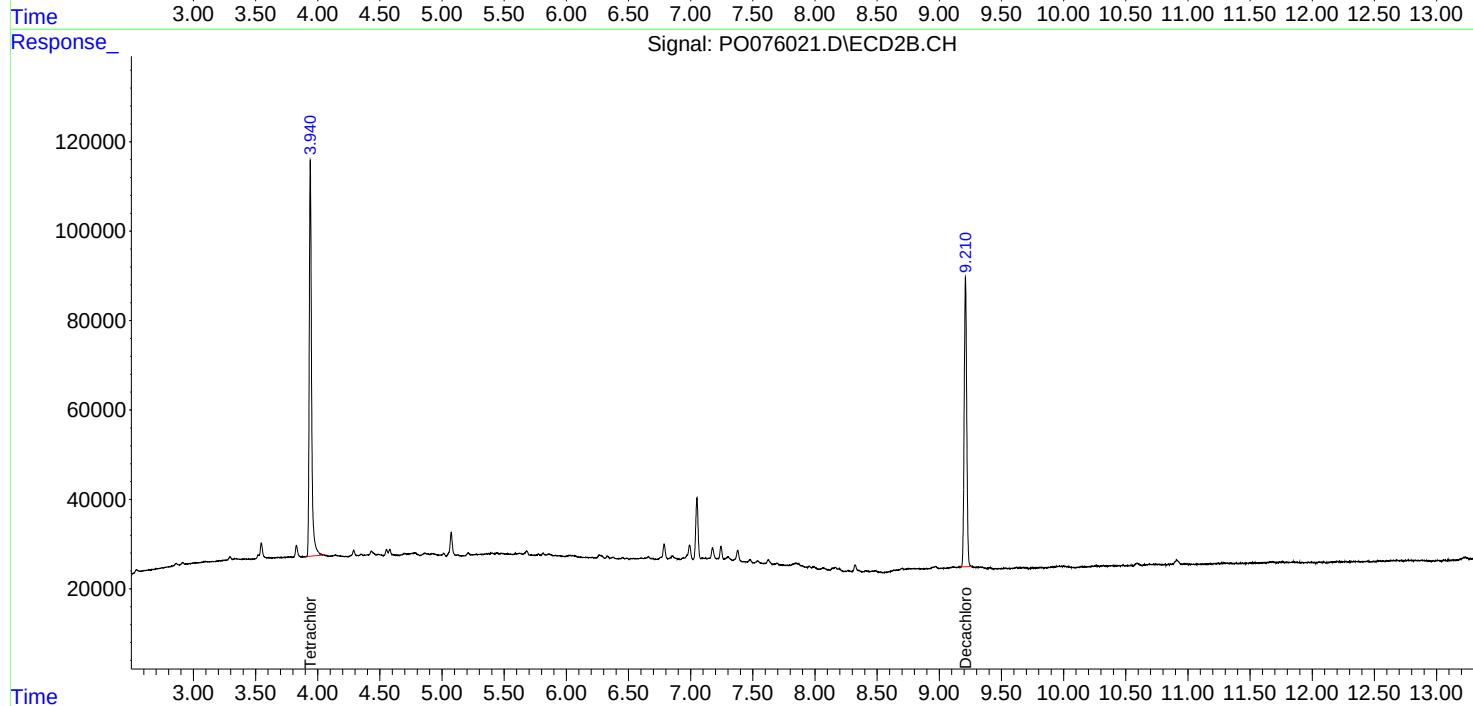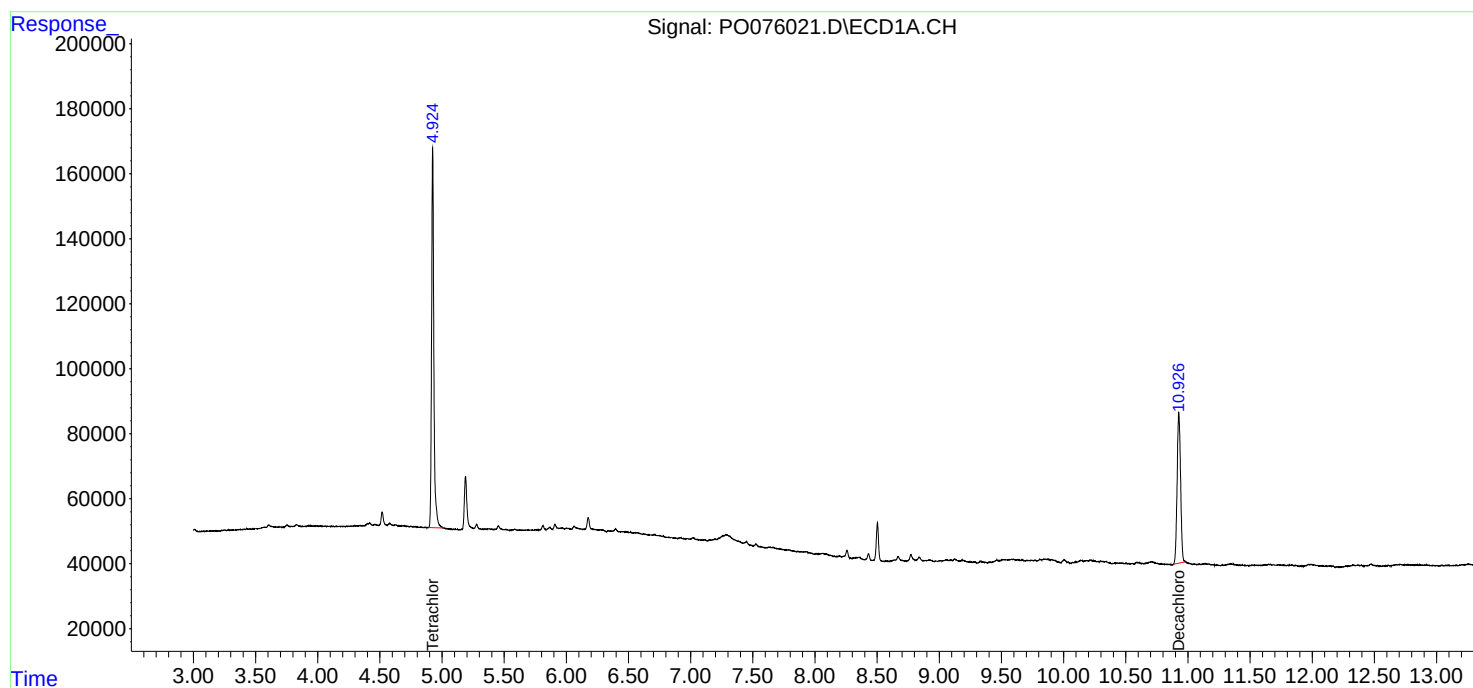


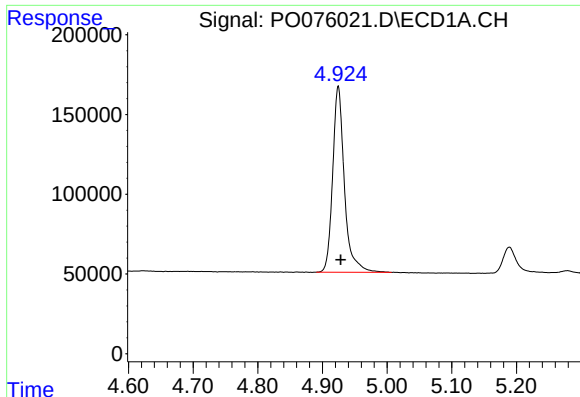

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.003 min
Response: 1471776
Conc: 24.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-04-015-ABCD

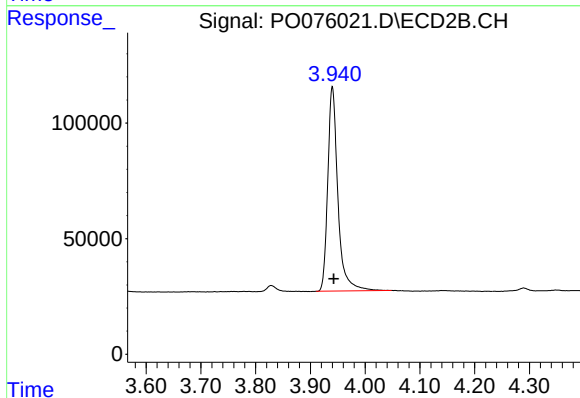


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.003 min
Response: 1139570
Conc: 25.55 ng/ml

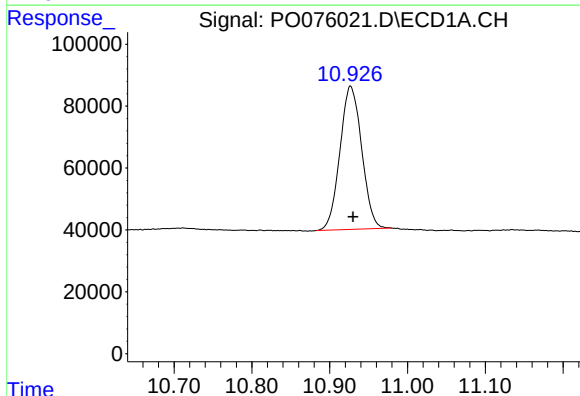

#2 Decachlorobiphenyl

R.T.: 10.927 min
Delta R.T.: -0.003 min
Response: 898251
Conc: 27.34 ng/ml

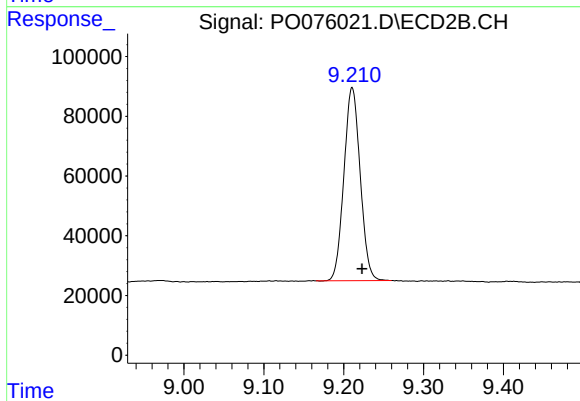

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.012 min
Response: 915080
Conc: 25.17 ng/ml