

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031021\
 Data File : P0076032.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2021 19:34
 Operator : DD\AJ
 Sample : M1605-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 13-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:28:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	3.942	1132519	873363	19.000	19.579
2) SA Decachlor...	10.924	9.210	464239	489243	14.131	13.455

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031021\
Data File : P0076032.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2021 19:34
Operator : DD\AJ
Sample : M1605-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
13-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:28:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

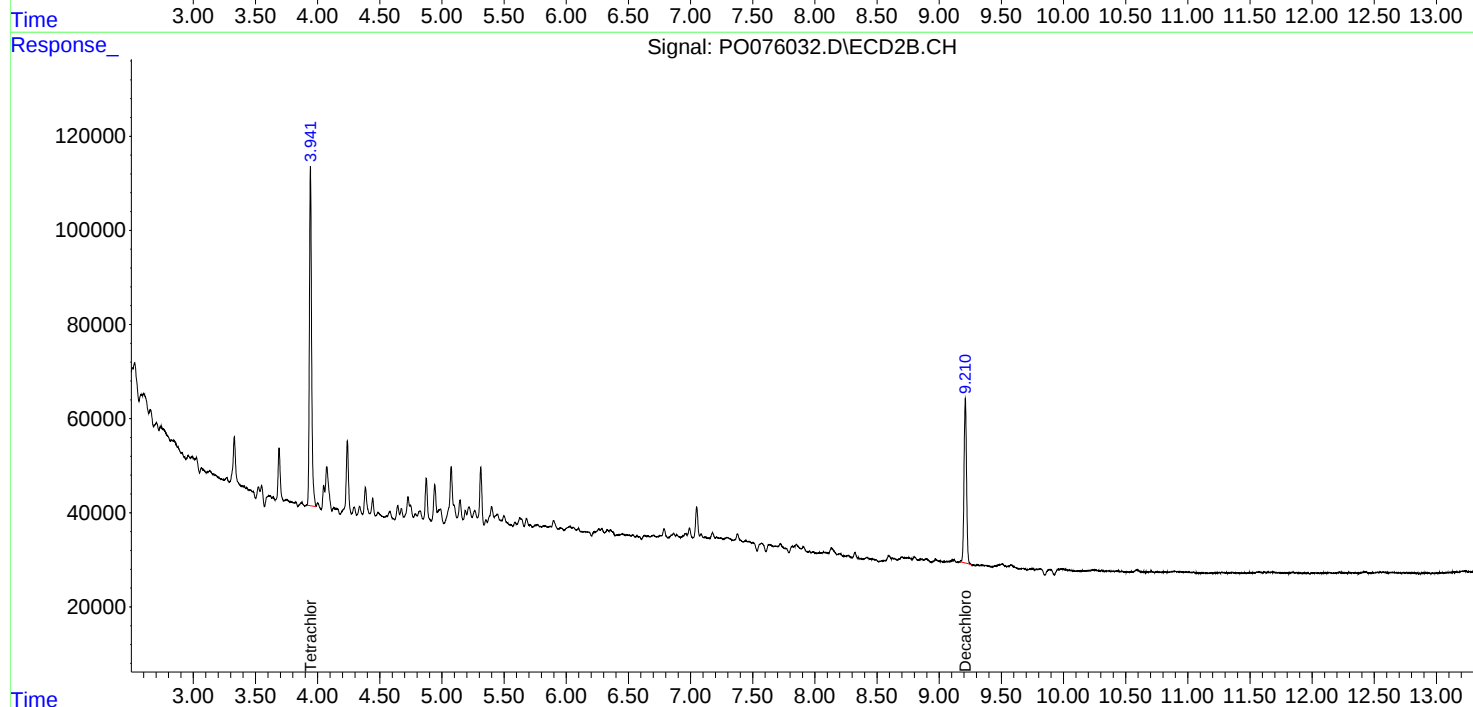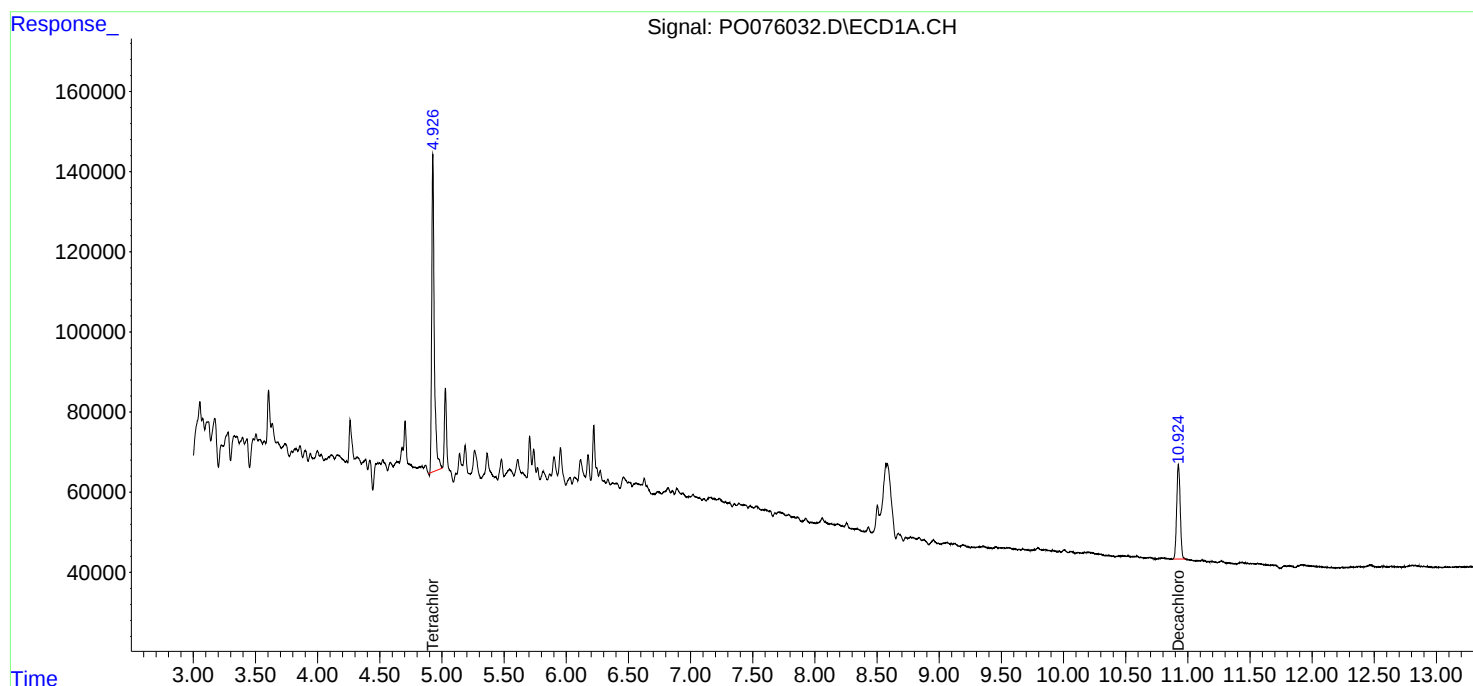


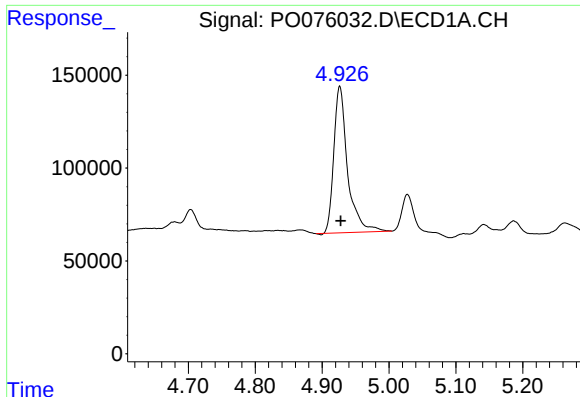

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.002 min
Response: 1132519
Conc: 19.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
13-14

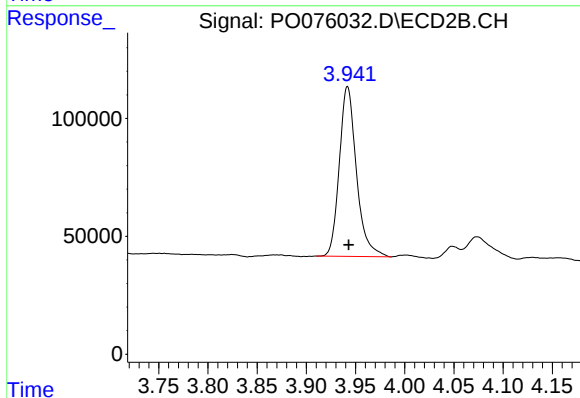


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.001 min
Response: 873363
Conc: 19.58 ng/ml

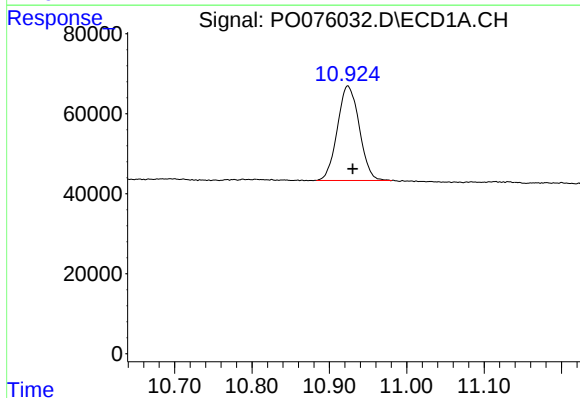

#2 Decachlorobiphenyl

R.T.: 10.924 min
Delta R.T.: -0.006 min
Response: 464239
Conc: 14.13 ng/ml

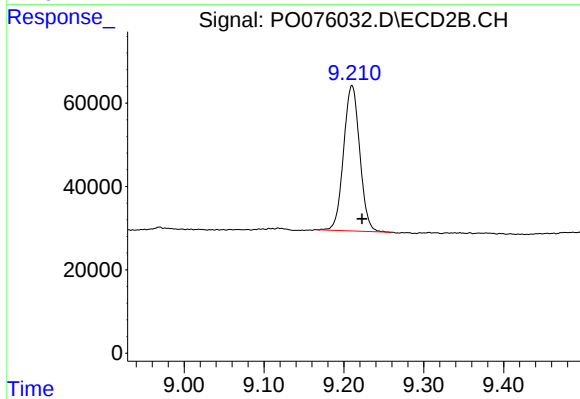

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: -0.013 min
Response: 489243
Conc: 13.46 ng/ml