

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031021\
 Data File : P0076034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2021 20:09
 Operator : DD\AJ
 Sample : M1606-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OW-SEPARATOR-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:29:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	3.941	800263	663319	13.426	14.870
2) SA Decachlor...	10.926	9.210	294322	316247	8.959	8.697

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031021\
Data File : P0076034.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2021 20:09
Operator : DD\AJ
Sample : M1606-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OW-SEPARATOR-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:29:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

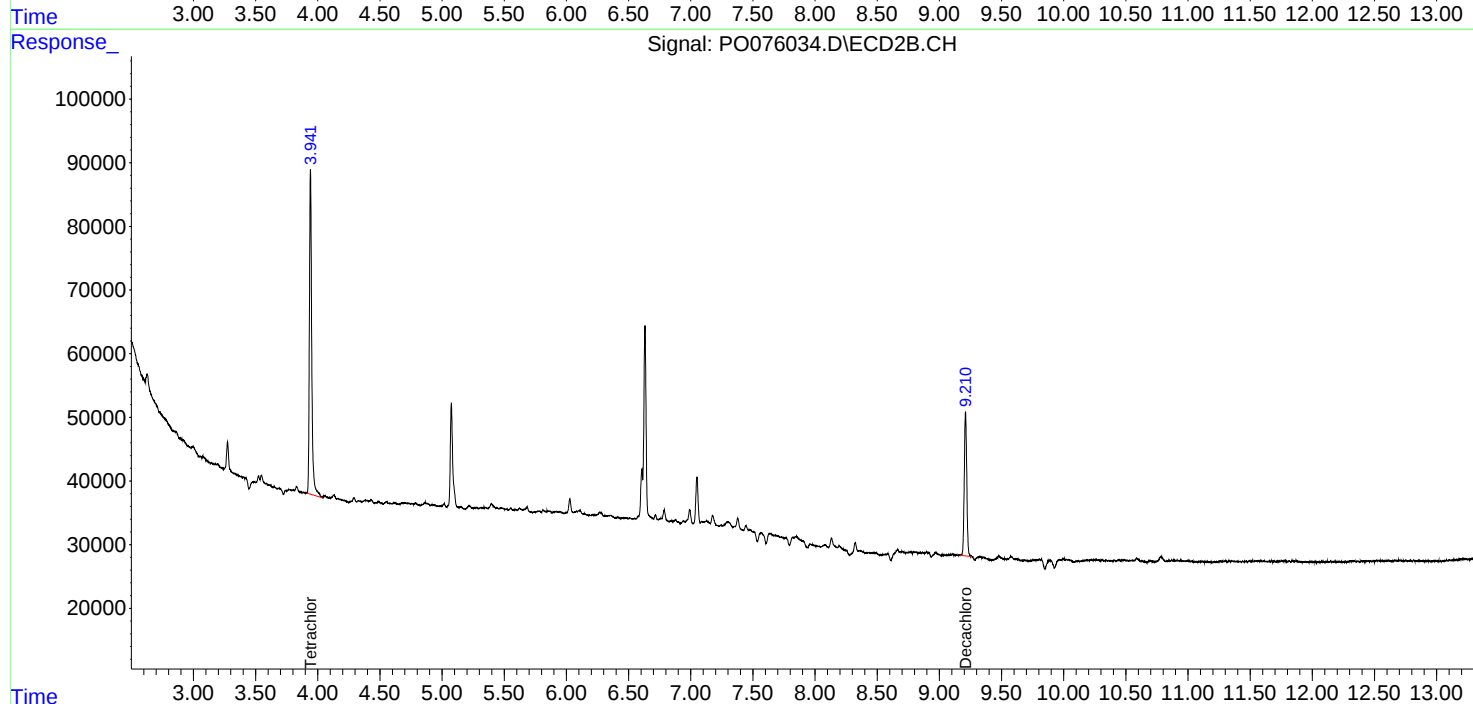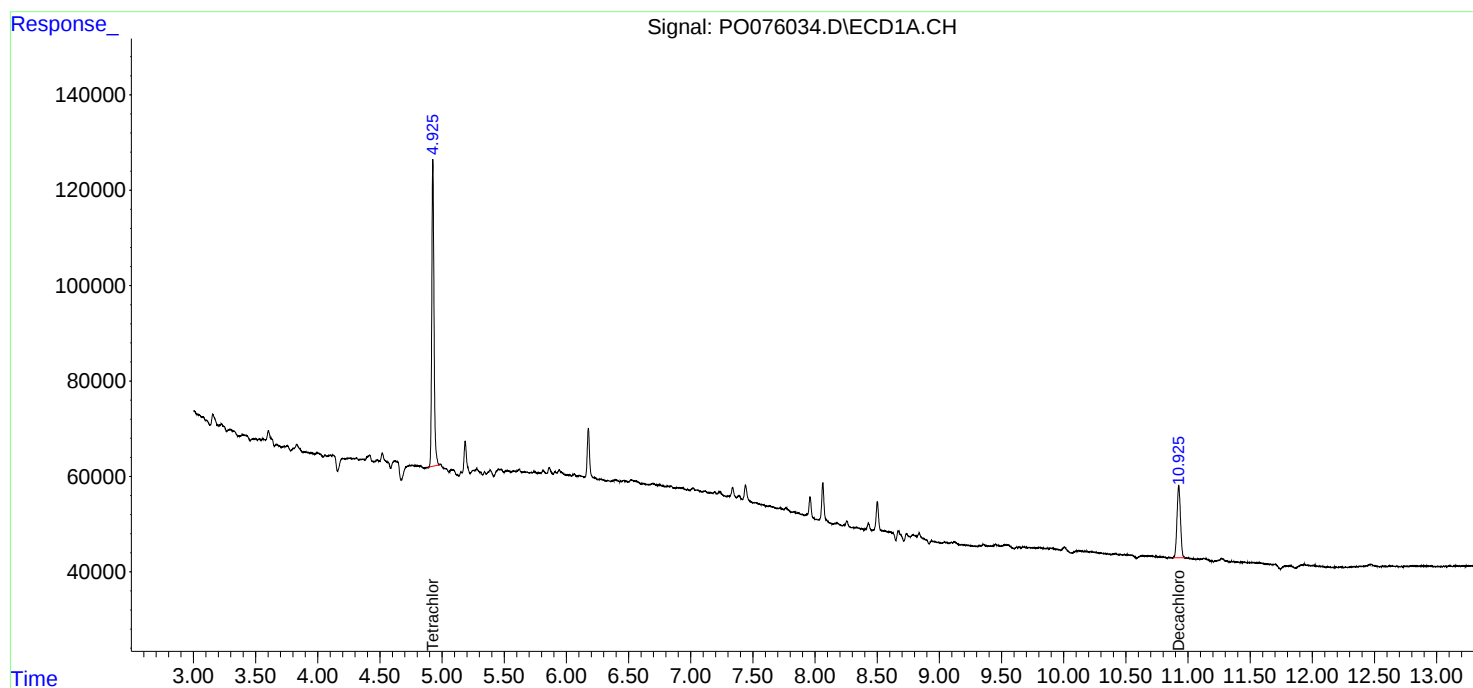


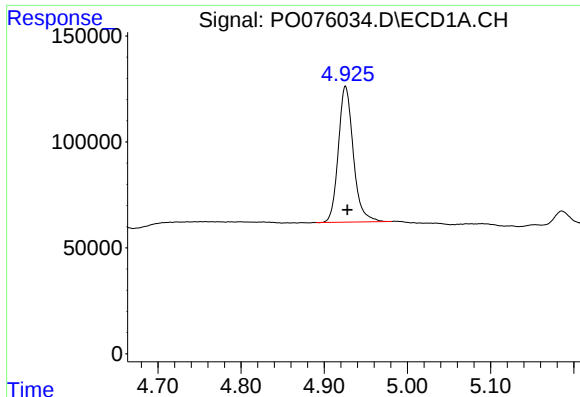

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.002 min
Response: 800263
Conc: 13.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
OW-SEPARATOR-PIT

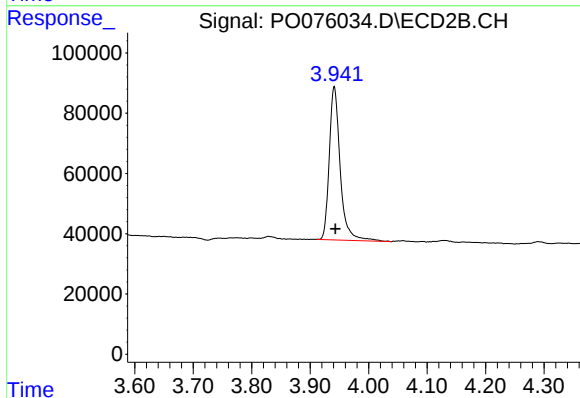


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 663319
Conc: 14.87 ng/ml

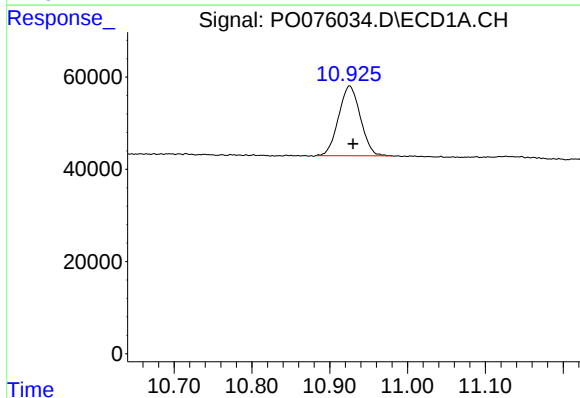

#2 Decachlorobiphenyl

R.T.: 10.926 min
Delta R.T.: -0.004 min
Response: 294322
Conc: 8.96 ng/ml

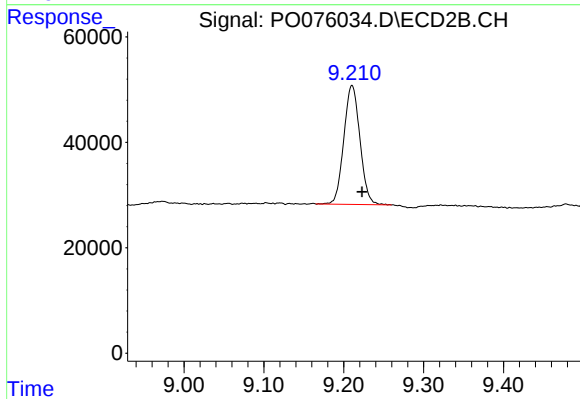

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: -0.013 min
Response: 316247
Conc: 8.70 ng/ml