

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031022\
 Data File : P0085253.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2022 10:29
 Operator : YP\AJ
 Sample : N1645-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:05:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.590	2889662	915483	16.829	20.063
2) SA Decachlor...	10.407	8.607	1335396	840267	20.393m	22.070
Target Compounds						
8) L2 AR-1221-1	4.709	3.805	168308	12974	91.086	23.536 #
9) L2 AR-1221-2	4.806	3.889	57934	32352	43.553	76.095 #
10) L2 AR-1221-3	4.874	3.967	99667	32322	25.549	24.813



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031022\
Data File : P0085253.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2022 10:29
Operator : YP\AJ
Sample : N1645-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:05:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

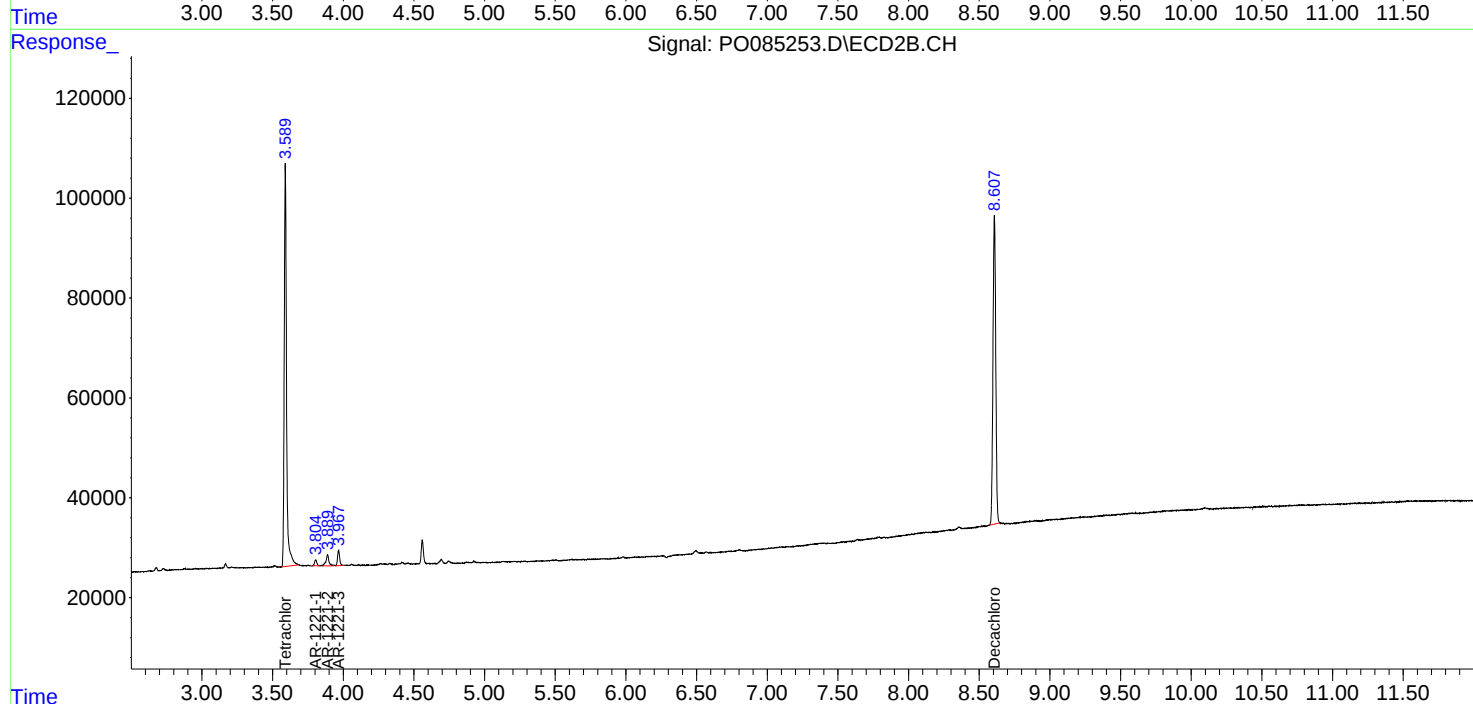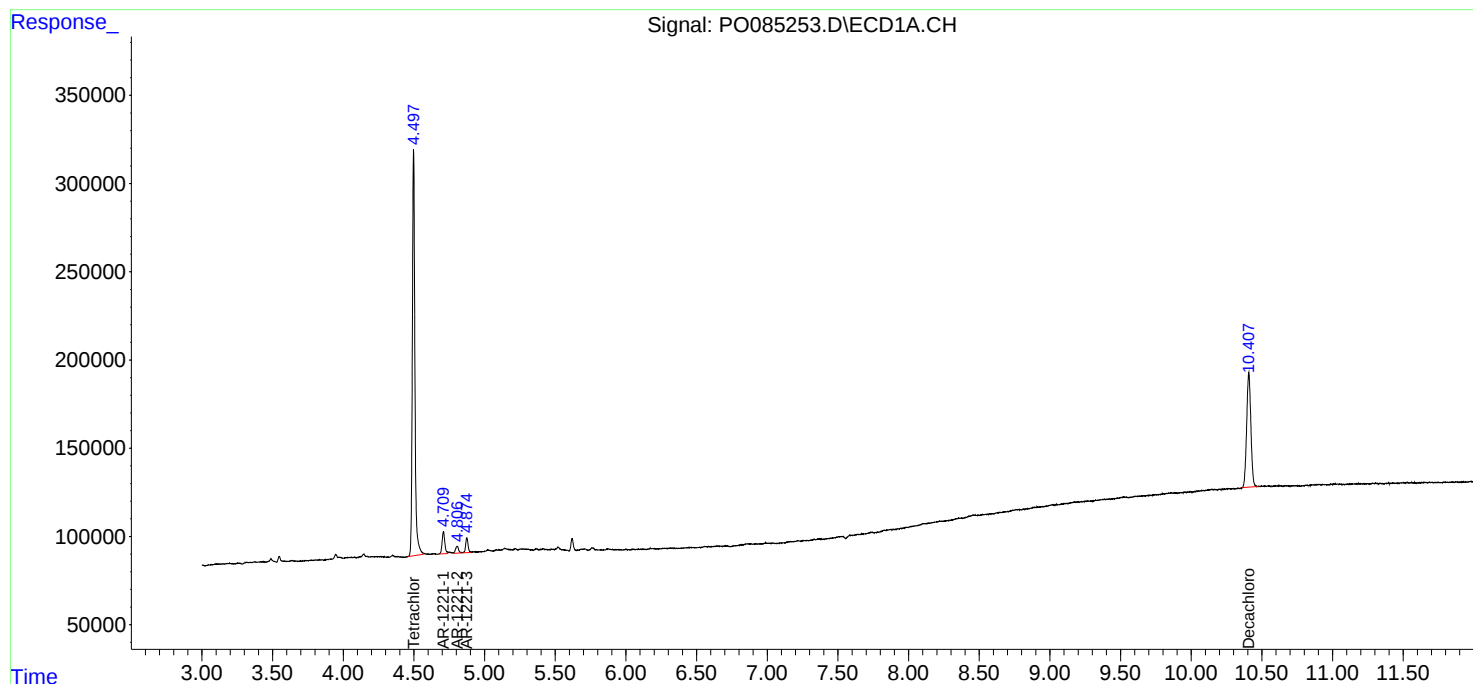


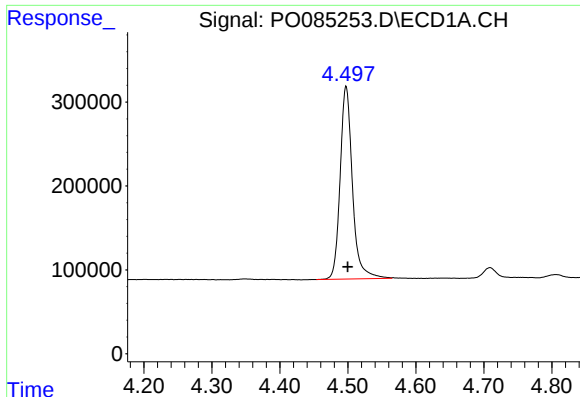

#1 Tetrachloro-m-xylene


R.T.: 4.497 min
Delta R.T.: -0.003 min
Response: 2889662
Conc: 16.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

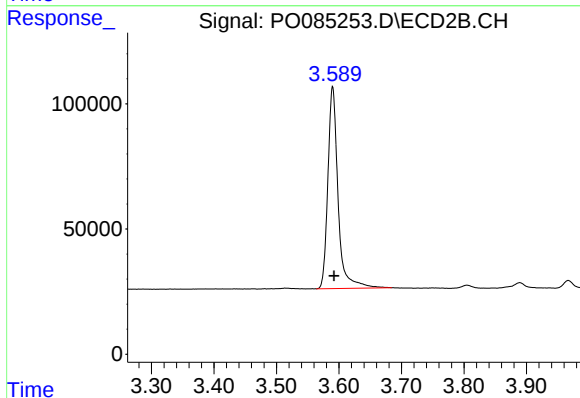


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.002 min
Response: 915483
Conc: 20.06 ng/ml

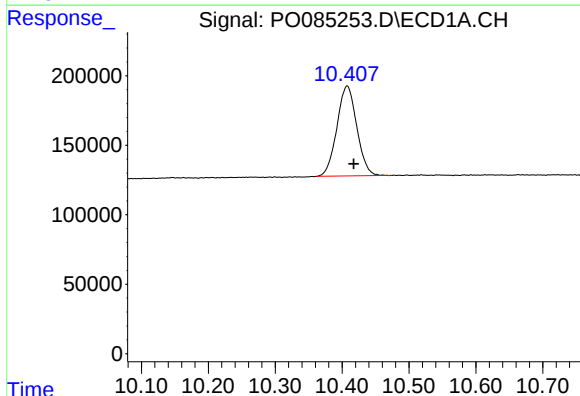


#2 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.010 min
Response: 1335396
Conc: 20.39 ng/ml m

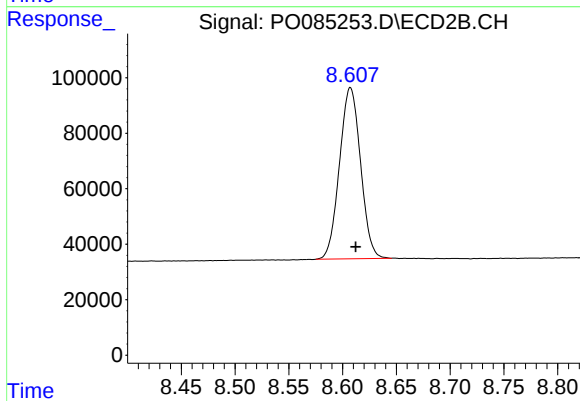

#2 Decachlorobiphenyl


R.T.: 8.607 min
Delta R.T.: -0.005 min
Response: 840267
Conc: 22.07 ng/ml

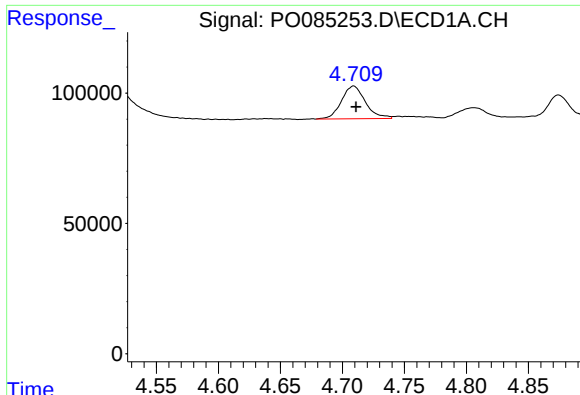

#8 AR-1221-1


R.T.: 4.709 min
Delta R.T.: -0.002 min
Response: 168308
Conc: 91.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

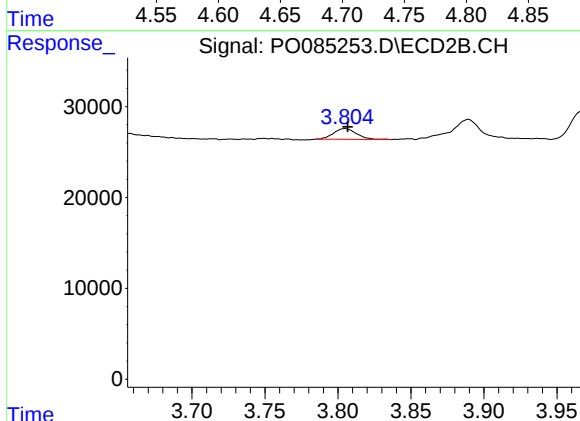


#8 AR-1221-1

R.T.: 3.805 min
Delta R.T.: -0.002 min
Response: 12974
Conc: 23.54 ng/ml

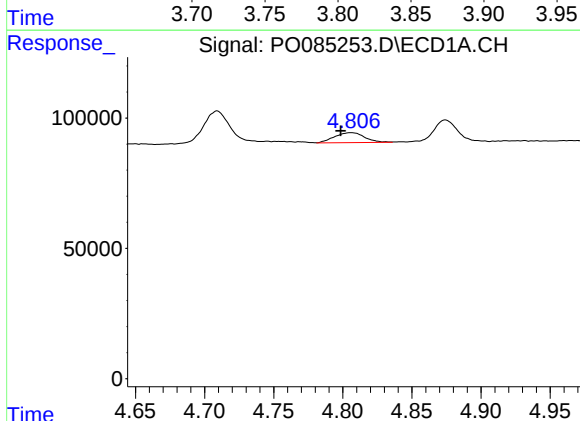


#9 AR-1221-2

R.T.: 4.806 min
Delta R.T.: 0.008 min
Response: 57934
Conc: 43.55 ng/ml

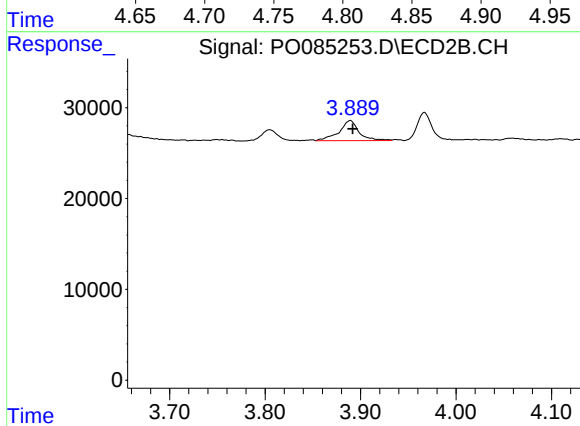

#9 AR-1221-2


R.T.: 3.889 min
Delta R.T.: -0.002 min
Response: 32352
Conc: 76.09 ng/ml

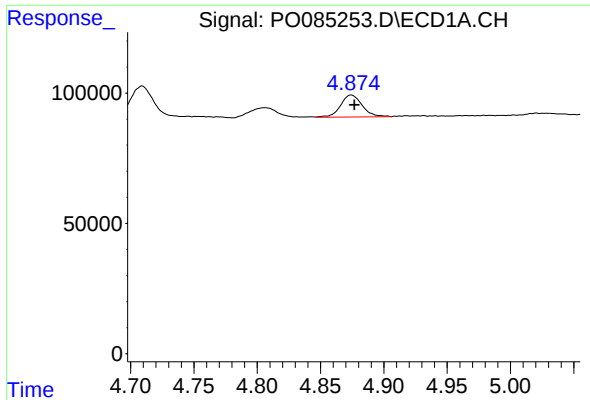

#10 AR-1221-3

R.T.: 4.874 min
Delta R.T.: -0.002 min
Response: 99667
Conc: 25.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2022

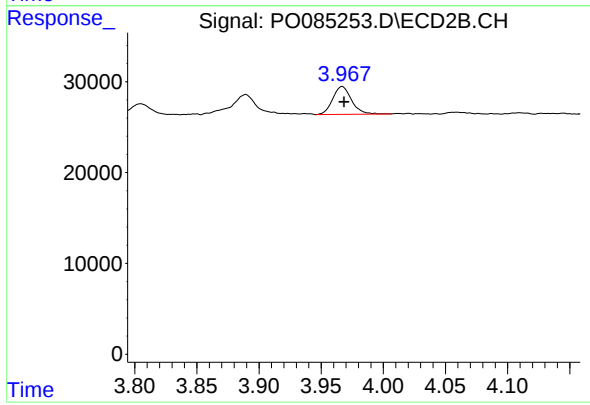

#10 AR-1221-3

R.T.: 3.967 min
Delta R.T.: -0.002 min
Response: 32322
Conc: 24.81 ng/ml